

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061022\
 Data File : FB027391.D
 Signal(s) : FID2B.CH
 Acq On : 10 Jun 2022 23:09
 Operator : AJ/MA
 Sample : 10 GRO STD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 11 00:31:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Sat Jun 11 00:30:50 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	112365	8.970 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	240830	13.718 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	242859	13.145 ng/ml
3) t n-Heptane	7.752	81760	4.459 ng/ml
4) t Benzene	7.889	94062	4.340 ng/ml
6) t Toluene	10.621	267709	13.187 ng/ml
7) t Ethylbenzene	13.058	83240	4.413 ng/ml
8) t m-Xylene	13.191	164176	8.767 ng/ml
9) t O-Xylene	13.918	160114	8.803 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	162872	9.201 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061022\
Data File : FB027391.D
Signal(s) : FID2B.CH
Acq On : 10 Jun 2022 23:09
Operator : AJ/MA
Sample : 10 GRO STD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 11 00:31:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Sat Jun 11 00:30:50 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

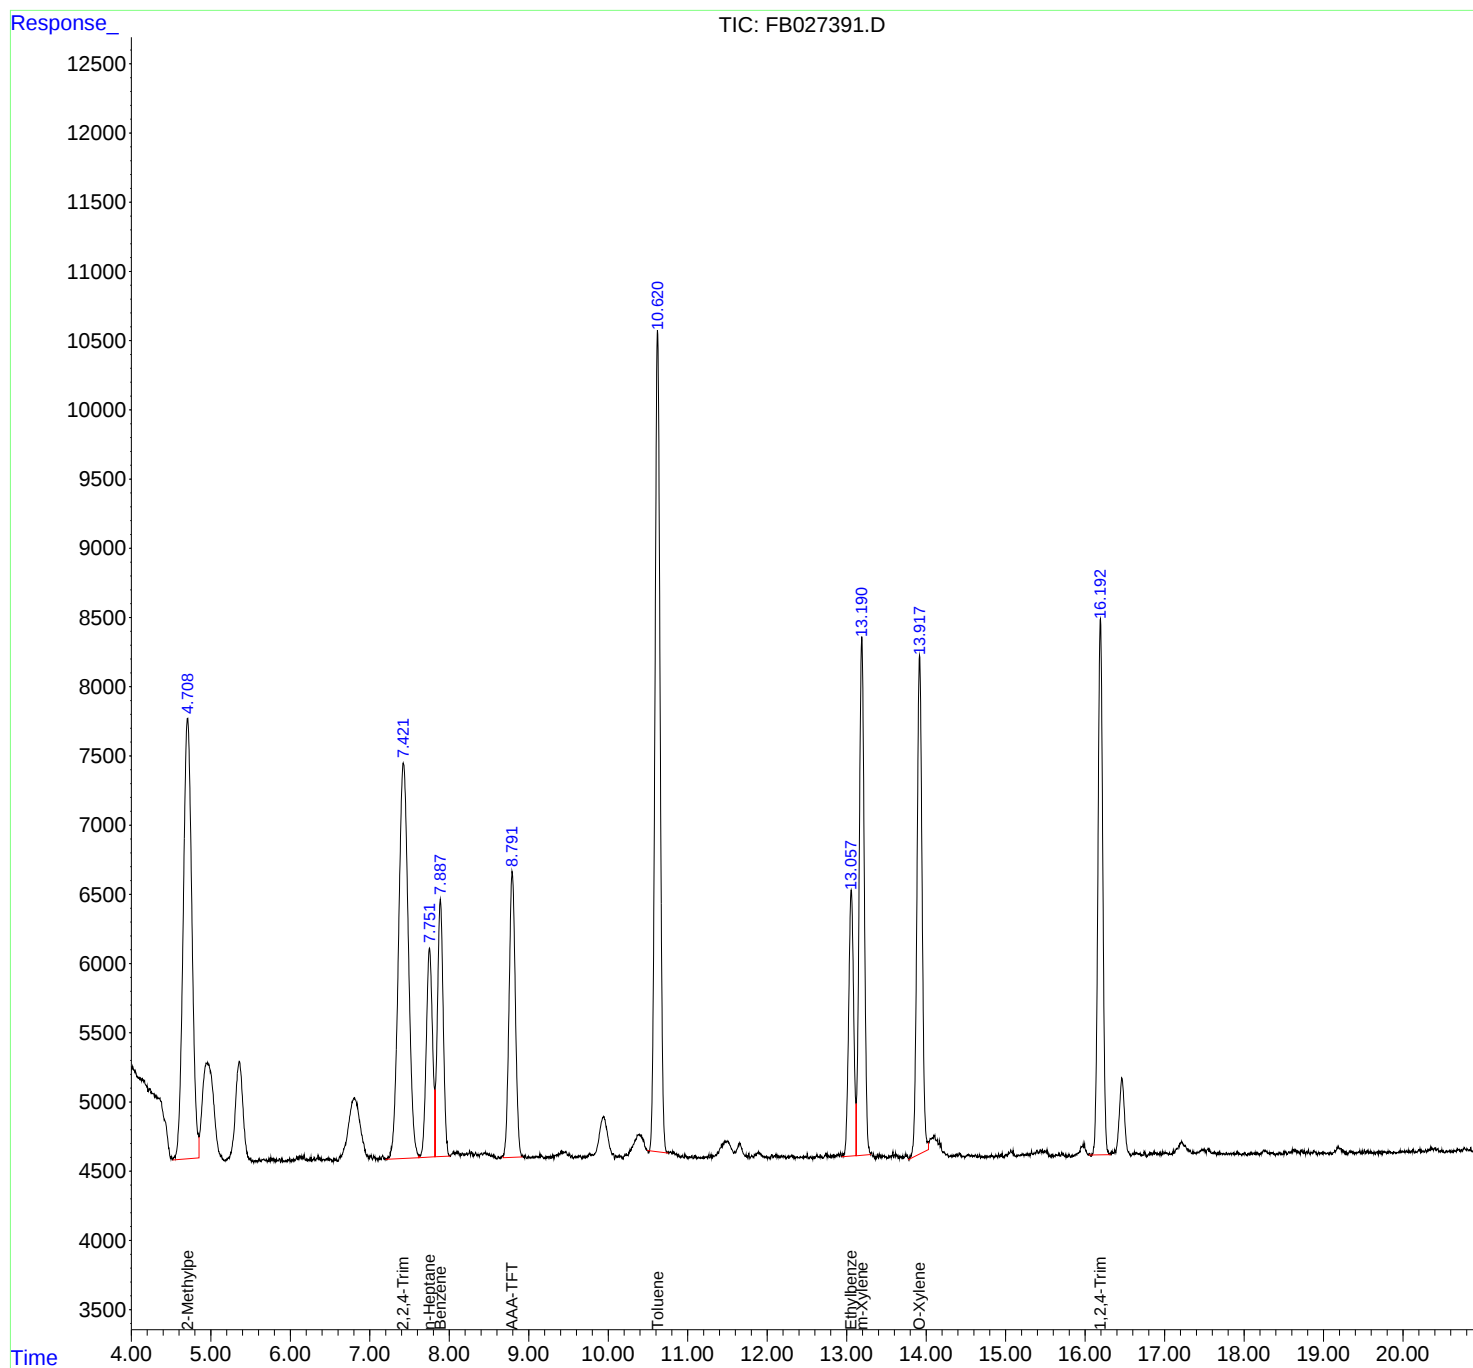

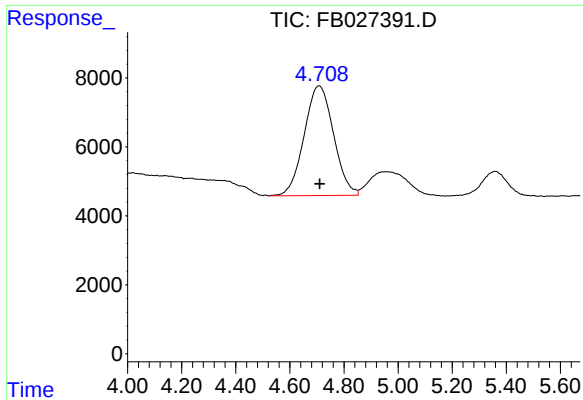


#1 2-Methylpentane

R.T.: 4.709 min
Delta R.T.: -0.001 min
Response: 240830
Conc: 13.72 ng/ml

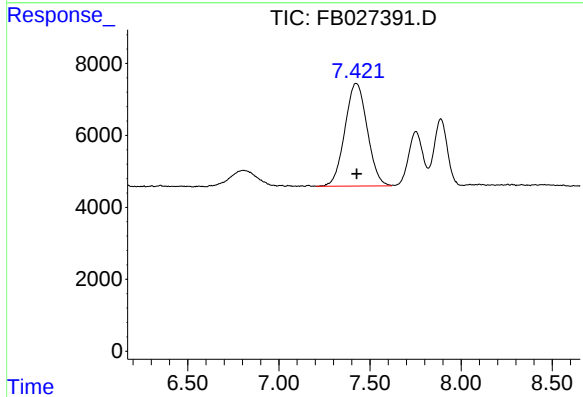


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: -0.006 min
Response: 242859
Conc: 13.15 ng/ml

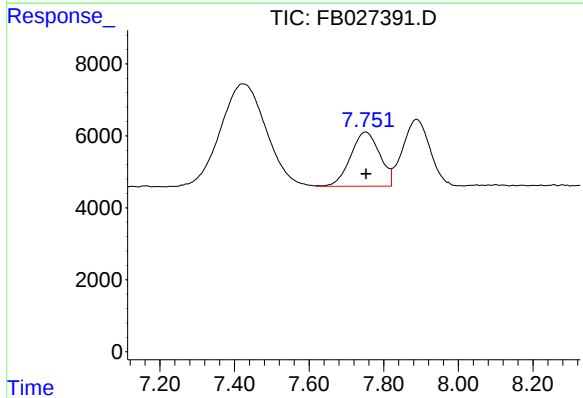


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 81760
Conc: 4.46 ng/ml

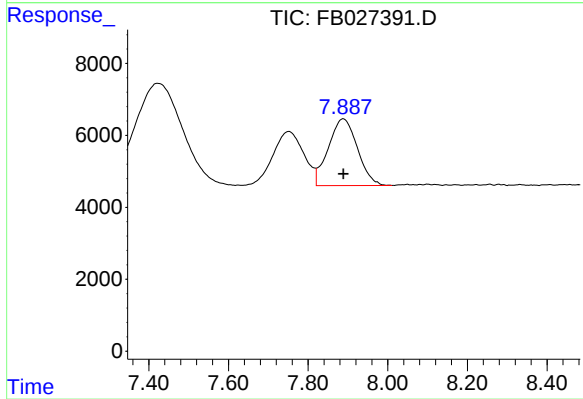


#4 Benzene

R.T.: 7.889 min
Delta R.T.: 0.000 min
Response: 94062
Conc: 4.34 ng/ml

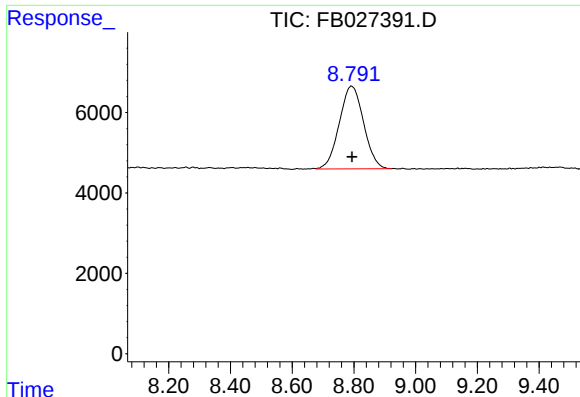


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: -0.002 min
Response: 112365
Conc: 8.97 ng/ml

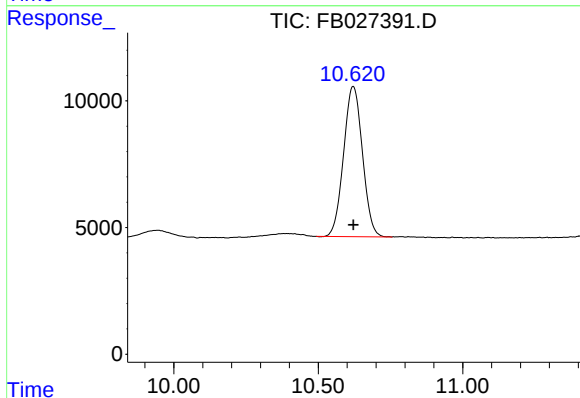


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 267709
Conc: 13.19 ng/ml

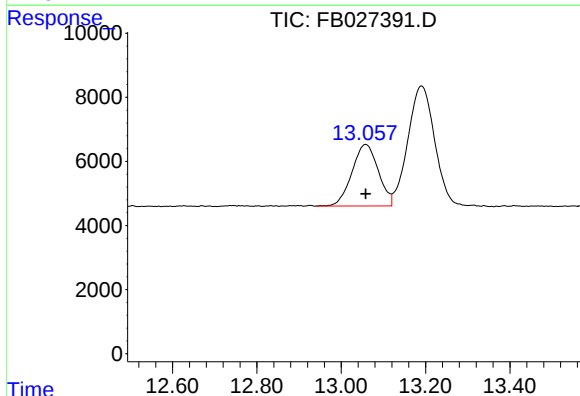


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 83240
Conc: 4.41 ng/ml

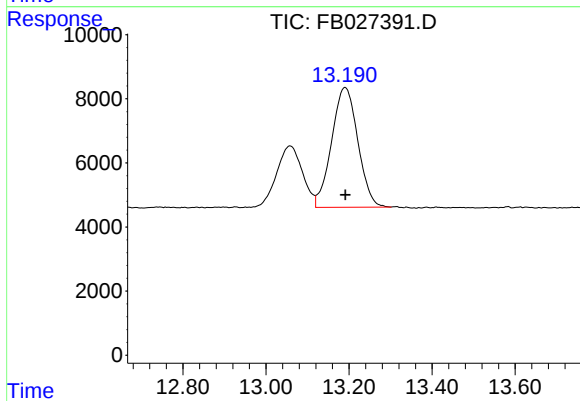


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 164176
Conc: 8.77 ng/ml

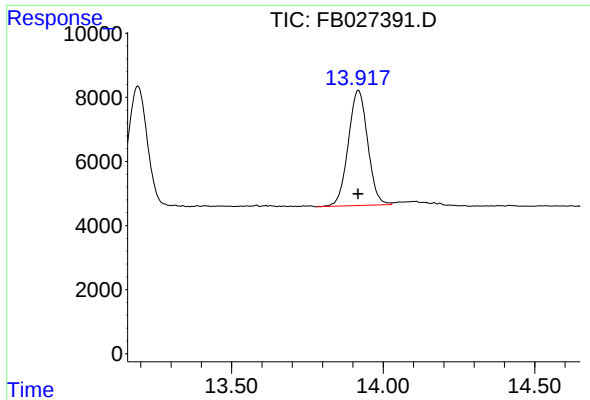

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 160114
Conc: 8.80 ng/ml

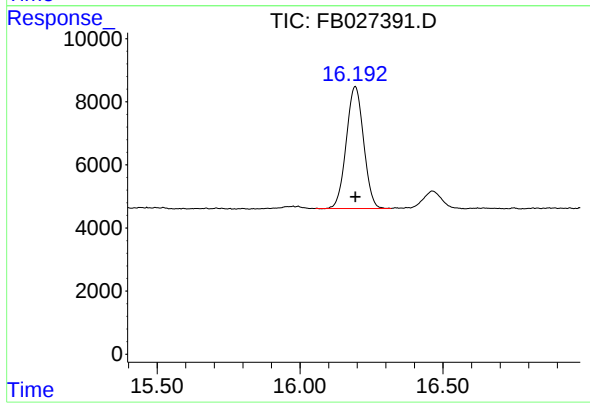

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 162872
Conc: 9.20 ng/ml