

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061418\
 Data File : FB016140.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2018 11:14
 Operator : MJ/SJ
 Sample : BSF0614S1
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0614S1

Integration File: Calibration.e
 Quant Time: Jun 15 04:33:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Fri Jun 01 13:25:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.117	145501	20.704 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.970	260903	21.516 ng/ml
2) t 2,2,4-Trimethylpentane	7.734	310229	26.788 ng/ml
3) t n-Heptane	8.074	77634	7.094 ng/ml
4) t Benzene	8.212	133535	8.993 ng/ml
6) t Toluene	10.967	332197	26.763 ng/ml
7) t Ethylbenzene	13.417	126134	9.011 ng/ml
8) t m-Xylene	13.550	273488	17.968 ng/ml
9) t O-Xylene	14.281	292601	18.750 ng/ml
10) t 1,2,4-Trimethylbenzene	16.564	320727	18.622 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061418\
Data File : FB016140.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2018 11:14
Operator : MJ/SJ
Sample : BSF0614S1
Misc : 5.00g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0614S1

Integration File: Calibration.e
Quant Time: Jun 15 04:33:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Fri Jun 01 13:25:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

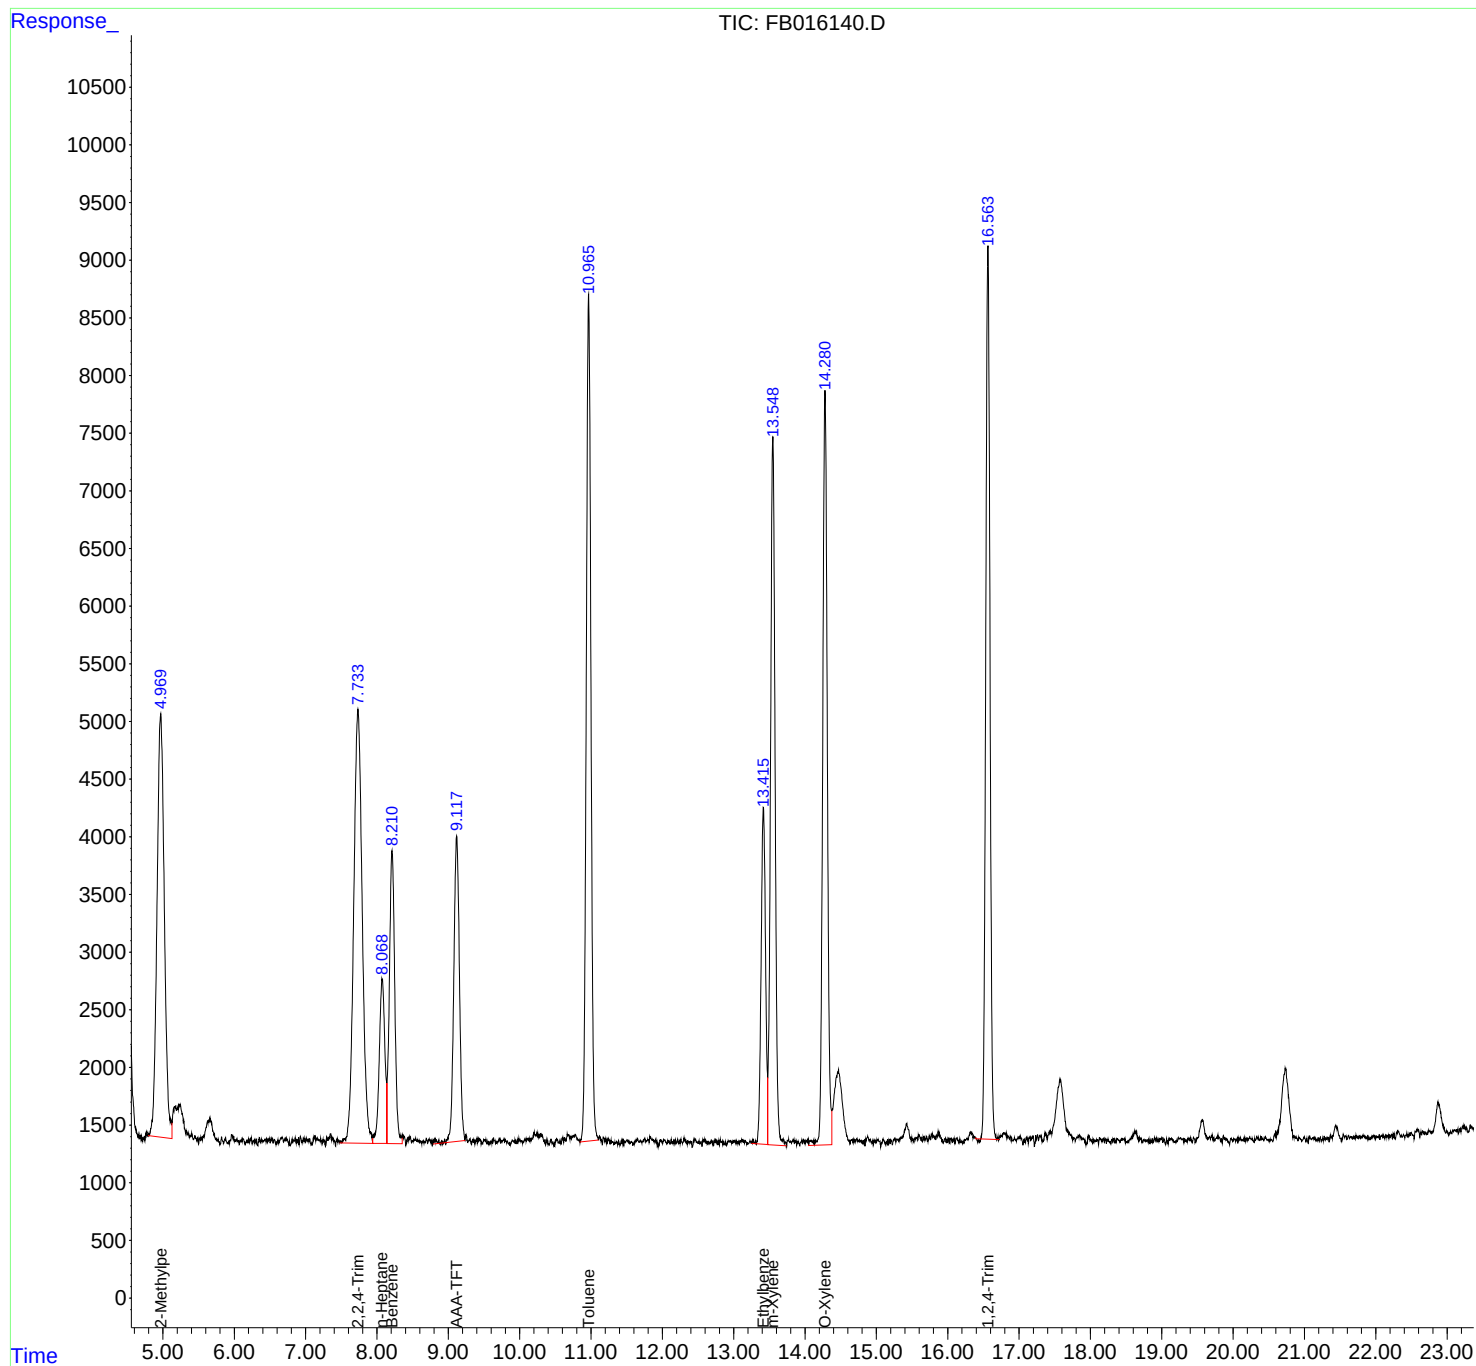


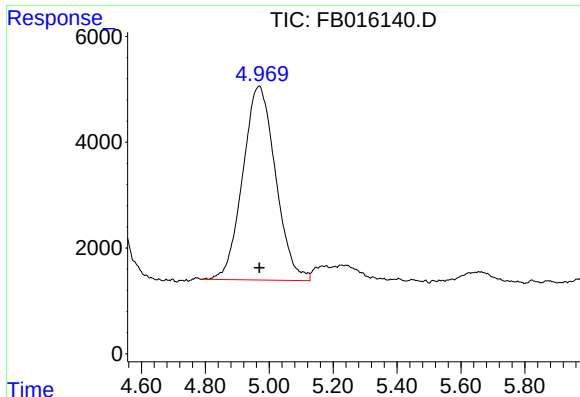

#1 2-Methylpentane


R.T.: 4.970 min
Delta R.T.: 0.000 min
Response: 260903
Conc: 21.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0614S1

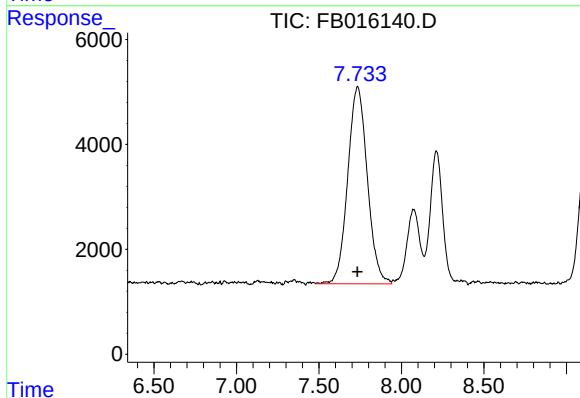


#2 2,2,4-Trimethylpentane

R.T.: 7.734 min
Delta R.T.: 0.000 min
Response: 310229
Conc: 26.79 ng/ml

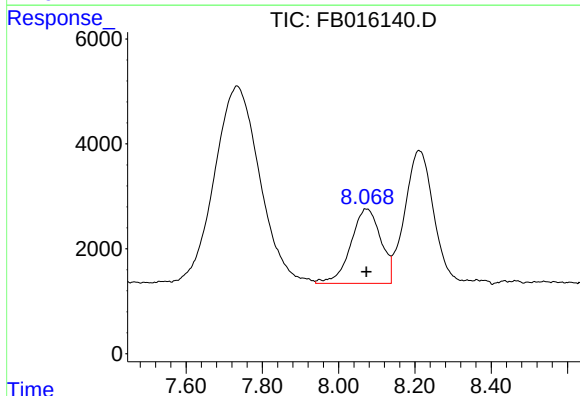


#3 n-Heptane

R.T.: 8.074 min
Delta R.T.: 0.000 min
Response: 77634
Conc: 7.09 ng/ml

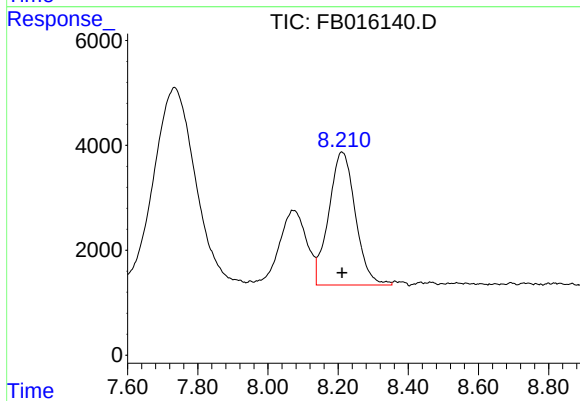

#4 Benzene


R.T.: 8.212 min
Delta R.T.: 0.000 min
Response: 133535
Conc: 8.99 ng/ml

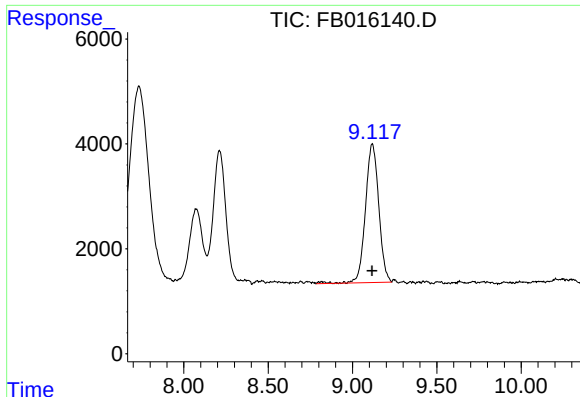

#5 AAA-TFT


R.T.: 9.117 min
Delta R.T.: 0.000 min
Response: 145501
Conc: 20.70 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0614S1

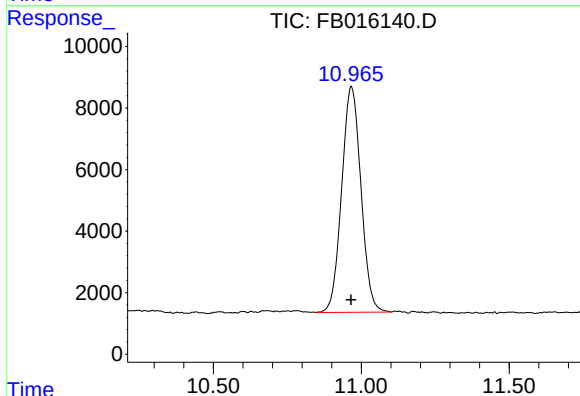


#6 Toluene

R.T.: 10.967 min
Delta R.T.: 0.001 min
Response: 332197
Conc: 26.76 ng/ml

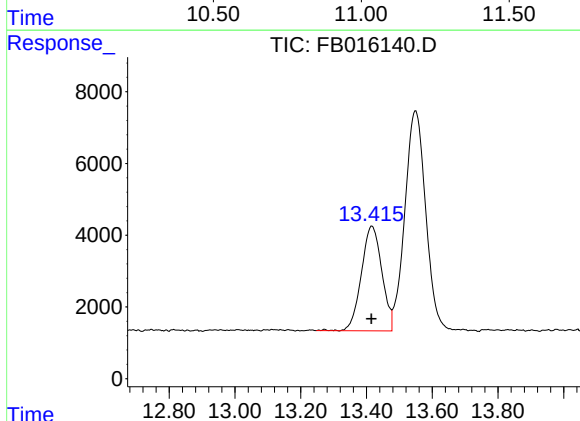


#7 Ethylbenzene

R.T.: 13.417 min
Delta R.T.: 0.002 min
Response: 126134
Conc: 9.01 ng/ml

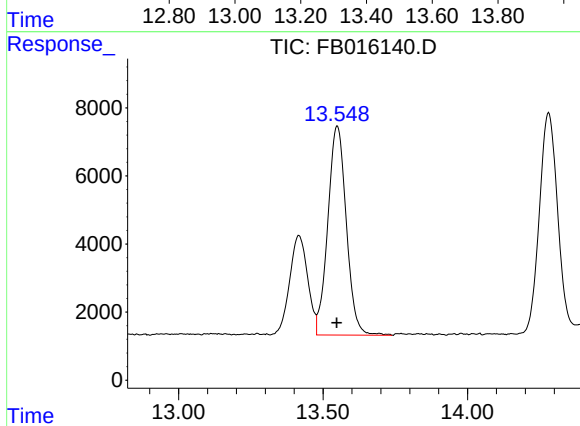

#8 m-Xylene


R.T.: 13.550 min
Delta R.T.: 0.002 min
Response: 273488
Conc: 17.97 ng/ml

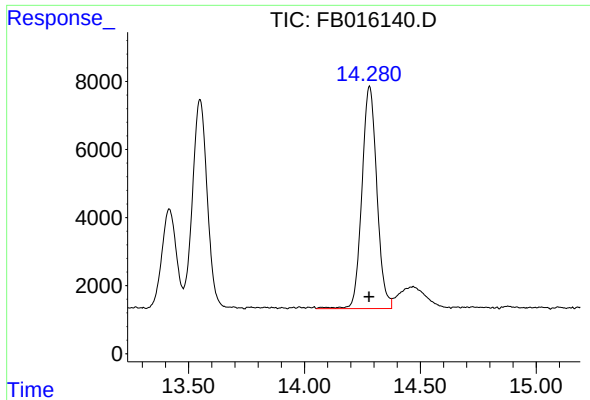

#9 O-Xylene

R.T.: 14.281 min
Delta R.T.: 0.003 min
Response: 292601
Conc: 18.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0614S1

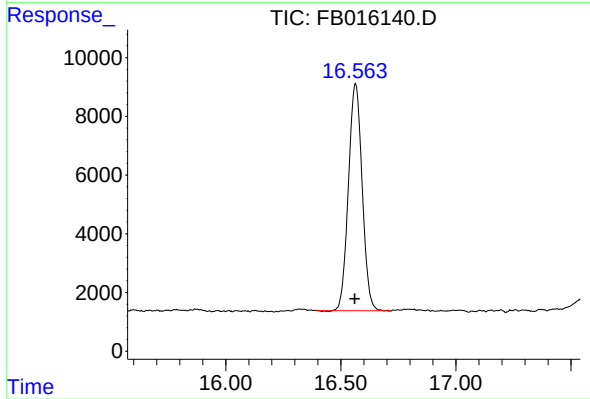

#10 1,2,4-Trimethylbenzene

R.T.: 16.564 min
Delta R.T.: 0.004 min
Response: 320727
Conc: 18.62 ng/ml