

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061418\
 Data File : FB016145.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2018 13:48
 Operator : MJ/SJ
 Sample : J3239-13MS
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-06-061318-CMS

Integration File: Calibration.e
 Quant Time: Jun 15 04:33:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Fri Jun 01 13:25:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.119	143063	20.357 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.973	243017	20.041 ng/ml
2) t 2,2,4-Trimethylpentane	7.737	282563	24.399 ng/ml
3) t n-Heptane	8.076	71533	6.536 ng/ml
4) t Benzene	8.215	125595	8.459 ng/ml
6) t Toluene	10.969	327541	26.388 ng/ml
7) t Ethylbenzene	13.418	131894	9.423 ng/ml
8) t m-Xylene	13.552	278385	18.290 ng/ml
9) t O-Xylene	14.283	296806	19.019 ng/ml
10) t 1,2,4-Trimethylbenzene	16.565	332283	19.293 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061418\
Data File : FB061415.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2018 13:48
Operator : MJ/SJ
Sample : J3239-13MS
Misc : 5.00g/5.00mL DI Water
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-06-061318-CMS

Integration File: Calibration.e
Quant Time: Jun 15 04:33:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Fri Jun 01 13:25:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

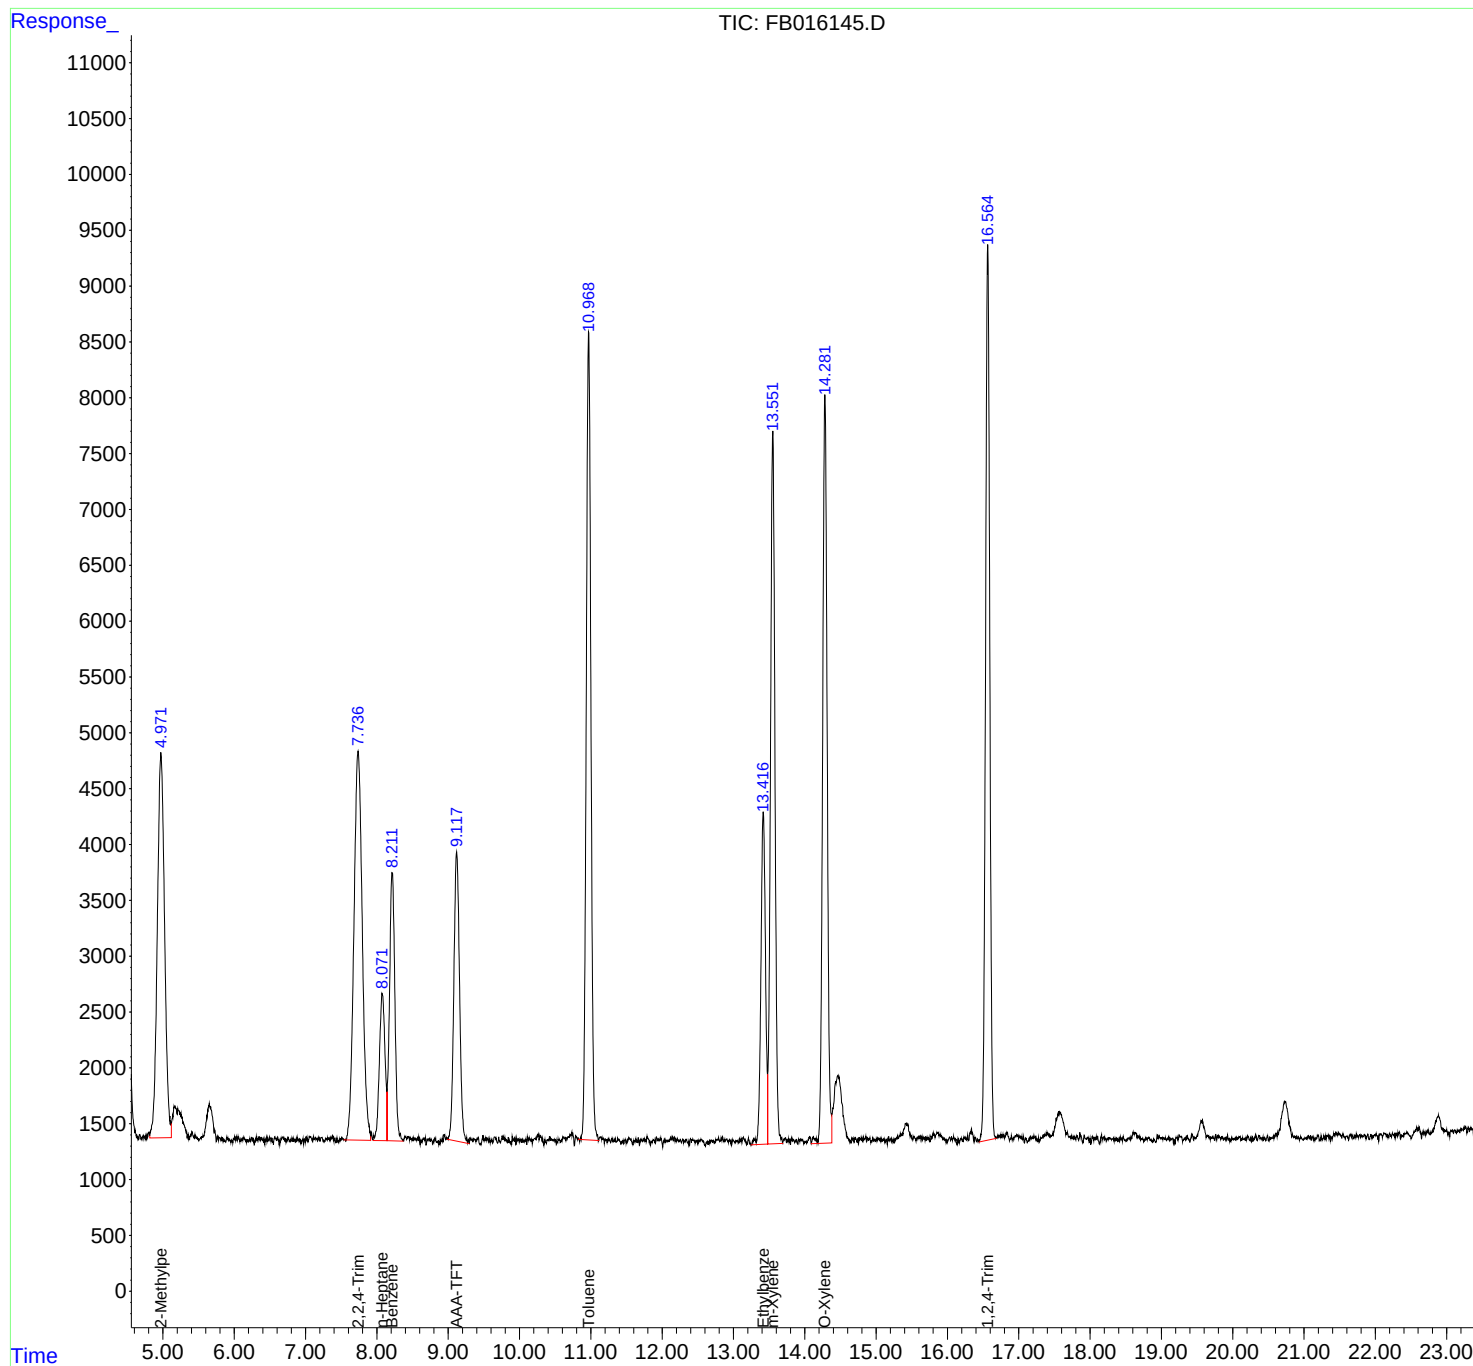


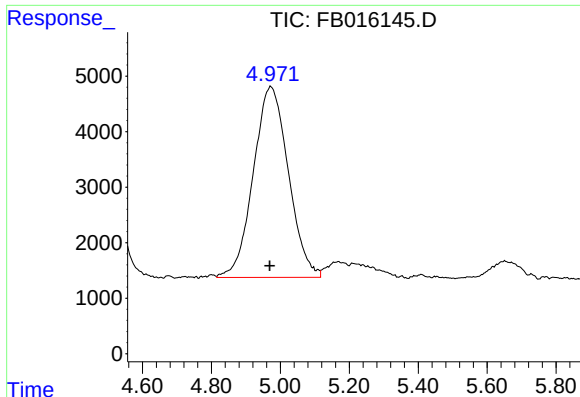

#1 2-Methylpentane


R.T.: 4.973 min
Delta R.T.: 0.004 min
Response: 243017
Conc: 20.04 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-061318-CMS

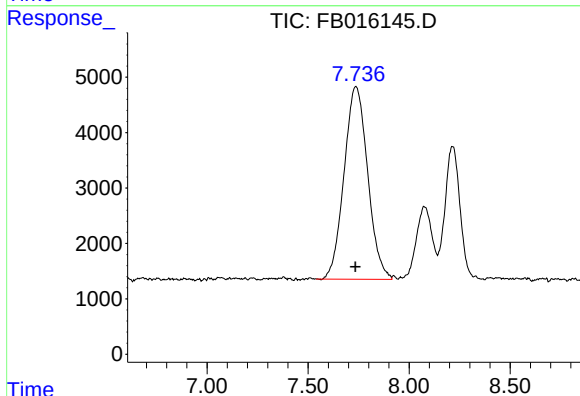


#2 2,2,4-Trimethylpentane

R.T.: 7.737 min
Delta R.T.: 0.003 min
Response: 282563
Conc: 24.40 ng/ml

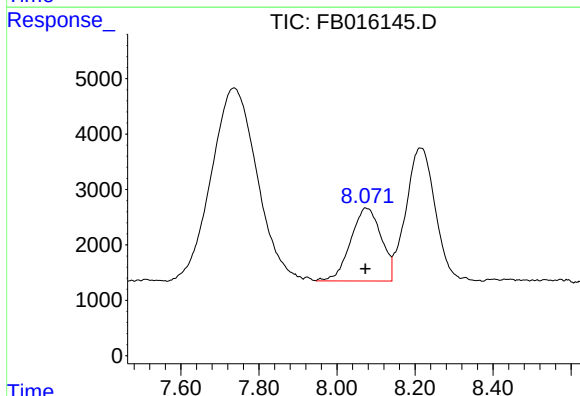


#3 n-Heptane

R.T.: 8.076 min
Delta R.T.: 0.003 min
Response: 71533
Conc: 6.54 ng/ml

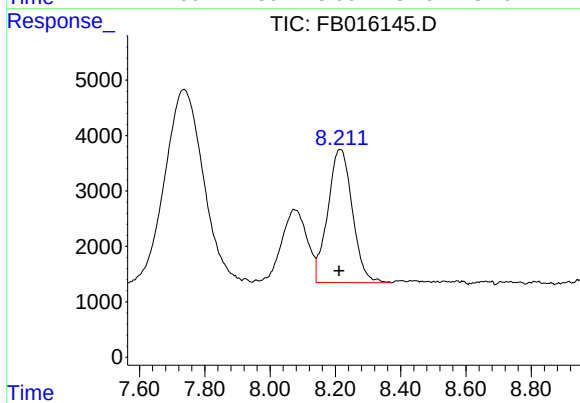

#4 Benzene


R.T.: 8.215 min
Delta R.T.: 0.004 min
Response: 125595
Conc: 8.46 ng/ml

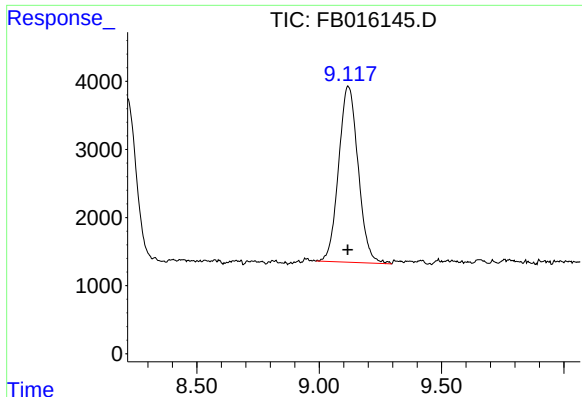

#5 AAA-TFT


R.T.: 9.119 min
Delta R.T.: 0.002 min
Response: 143063
Conc: 20.36 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-061318-CMS

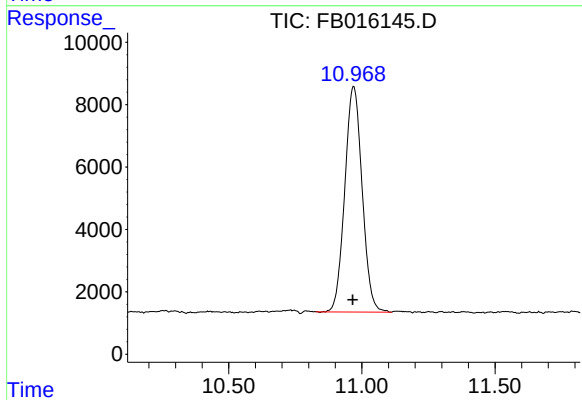


#6 Toluene

R.T.: 10.969 min
Delta R.T.: 0.004 min
Response: 327541
Conc: 26.39 ng/ml

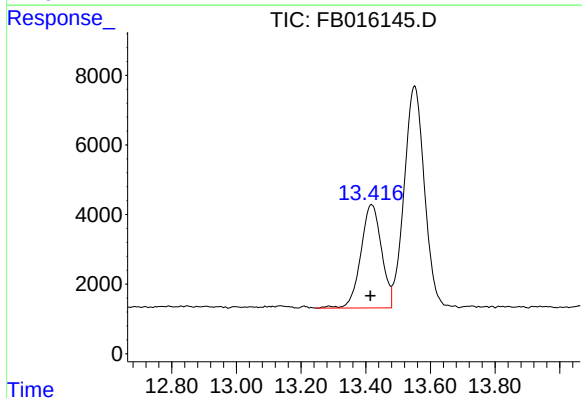


#7 Ethylbenzene

R.T.: 13.418 min
Delta R.T.: 0.004 min
Response: 131894
Conc: 9.42 ng/ml

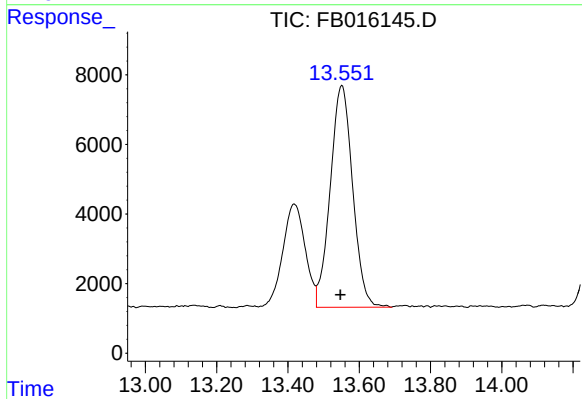

#8 m-Xylene


R.T.: 13.552 min
Delta R.T.: 0.004 min
Response: 278385
Conc: 18.29 ng/ml

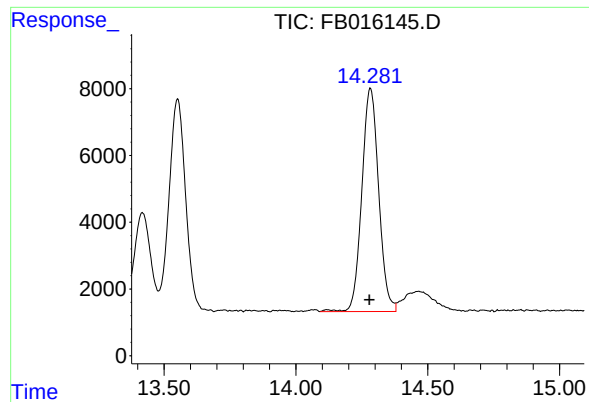

#9 O-Xylene

R.T.: 14.283 min
Delta R.T.: 0.004 min
Response: 296806
Conc: 19.02 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-061318-CMS

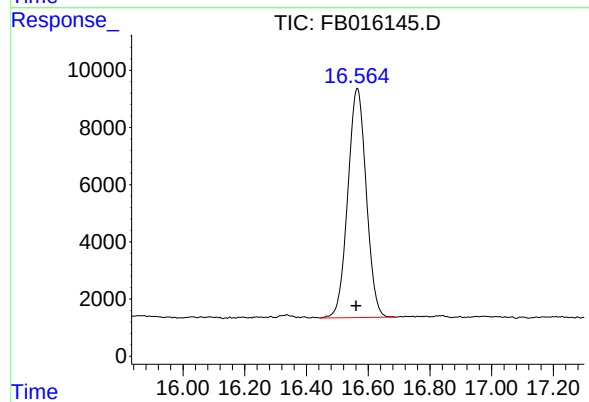

#10 1,2,4-Trimethylbenzene

R.T.: 16.565 min
Delta R.T.: 0.005 min
Response: 332283
Conc: 19.29 ng/ml