

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061418\
 Data File : FB016146.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jun 2018 14:19
 Operator : MJ/SJ
 Sample : J3239-13MSD
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-06-061318-CMSD

Integration File: Calibration.e
 Quant Time: Jun 15 04:34:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Fri Jun 01 13:25:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.120	154773	22.023 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.973	260750	21.503 ng/ml
2) t 2,2,4-Trimethylpentane	7.739	305068	26.342 ng/ml
3) t n-Heptane	8.077	77480	7.079 ng/ml
4) t Benzene	8.215	134602	9.065 ng/ml
6) t Toluene	10.969	342272	27.574 ng/ml
7) t Ethylbenzene	13.419	132817	9.489 ng/ml
8) t m-Xylene	13.551	284395	18.685 ng/ml
9) t O-Xylene	14.283	302330	19.373 ng/ml
10) t 1,2,4-Trimethylbenzene	16.565	338449	19.651 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061418\
Data File : FB016146.D
Signal(s) : FID2B.CH
Acq On : 14 Jun 2018 14:19
Operator : MJ/SJ
Sample : J3239-13MSD
Misc : 5.01g/5.00mL DI Water
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-06-061318-CMSD

Integration File: Calibration.e
Quant Time: Jun 15 04:34:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Fri Jun 01 13:25:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

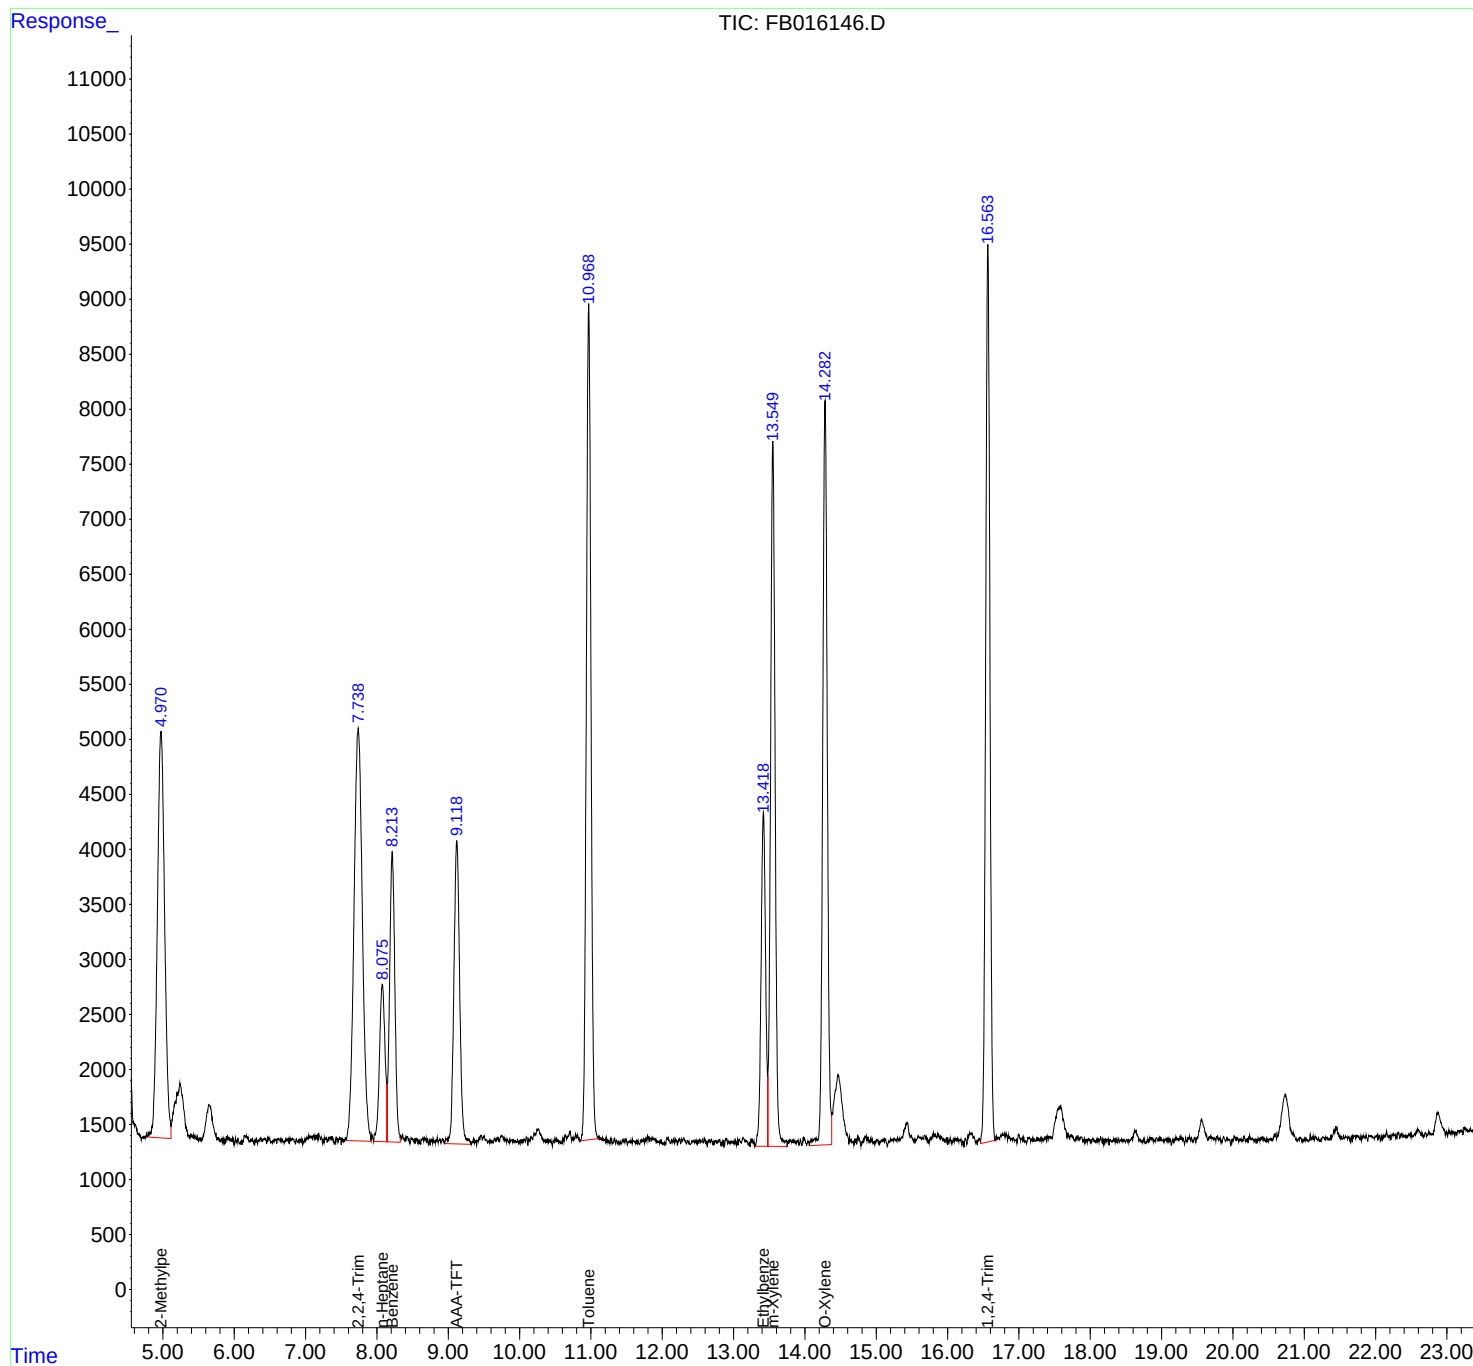


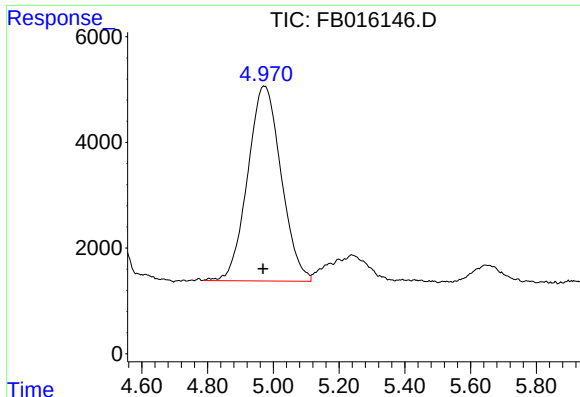

#1 2-Methylpentane


R.T.: 4.973 min
Delta R.T.: 0.004 min
Response: 260750
Conc: 21.50 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-061318-CMSD

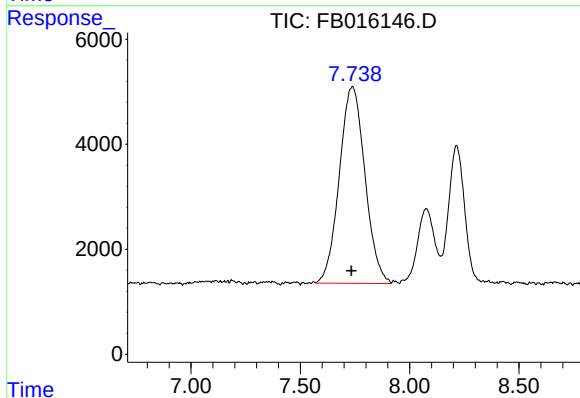


#2 2,2,4-Trimethylpentane

R.T.: 7.739 min
Delta R.T.: 0.005 min
Response: 305068
Conc: 26.34 ng/ml

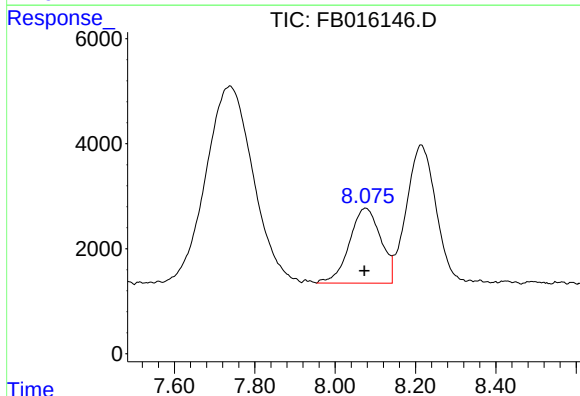


#3 n-Heptane

R.T.: 8.077 min
Delta R.T.: 0.004 min
Response: 77480
Conc: 7.08 ng/ml

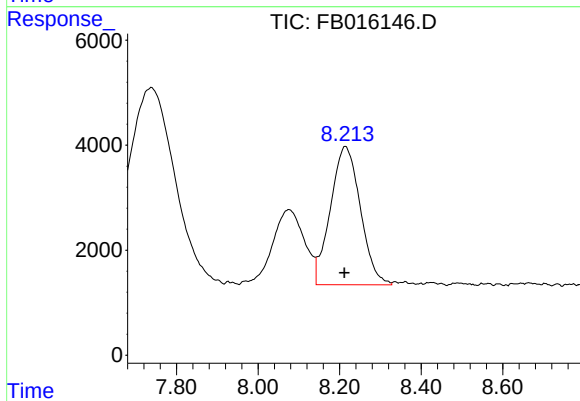

#4 Benzene


R.T.: 8.215 min
Delta R.T.: 0.003 min
Response: 134602
Conc: 9.07 ng/ml

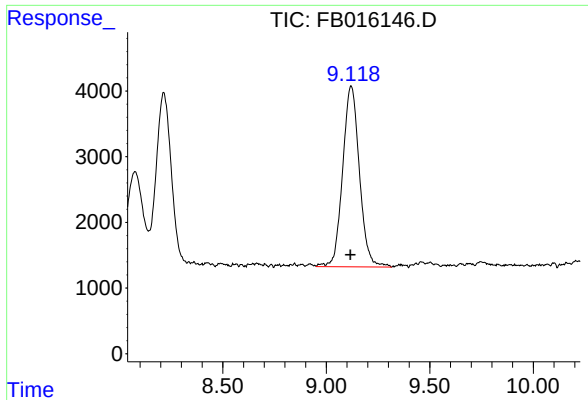

#5 AAA-TFT


R.T.: 9.120 min
Delta R.T.: 0.003 min
Response: 154773
Conc: 22.02 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-061318-CMSD

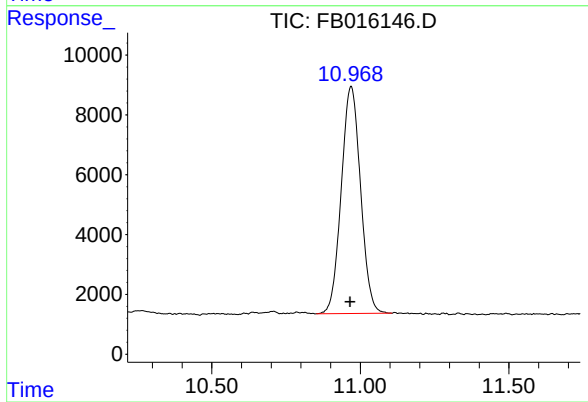


#6 Toluene

R.T.: 10.969 min
Delta R.T.: 0.004 min
Response: 342272
Conc: 27.57 ng/ml

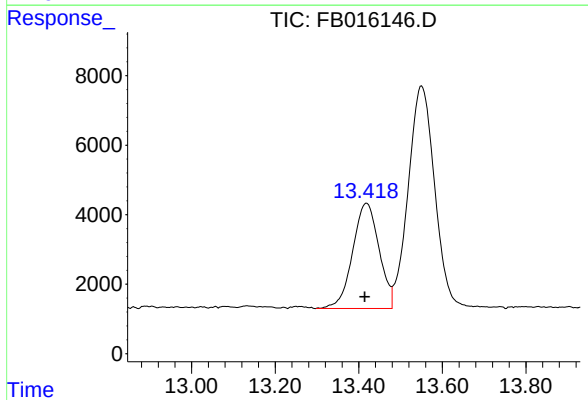


#7 Ethylbenzene

R.T.: 13.419 min
Delta R.T.: 0.004 min
Response: 132817
Conc: 9.49 ng/ml

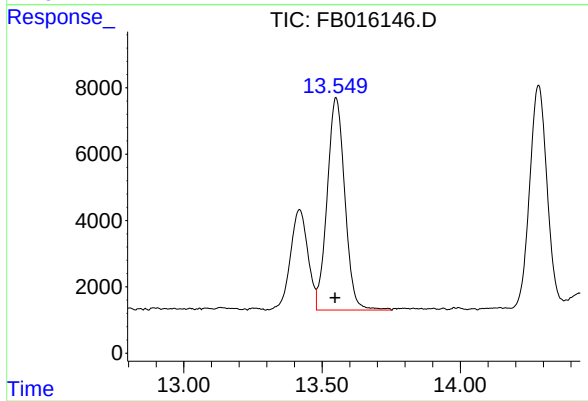

#8 m-Xylene


R.T.: 13.551 min
Delta R.T.: 0.004 min
Response: 284395
Conc: 18.68 ng/ml

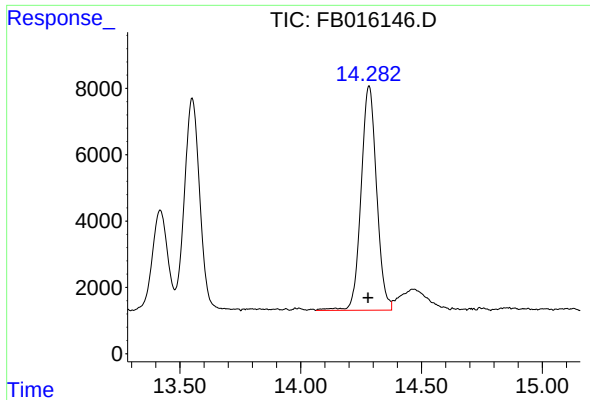

#9 O-Xylene

R.T.: 14.283 min
Delta R.T.: 0.005 min
Response: 302330
Conc: 19.37 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-061318-CMSD

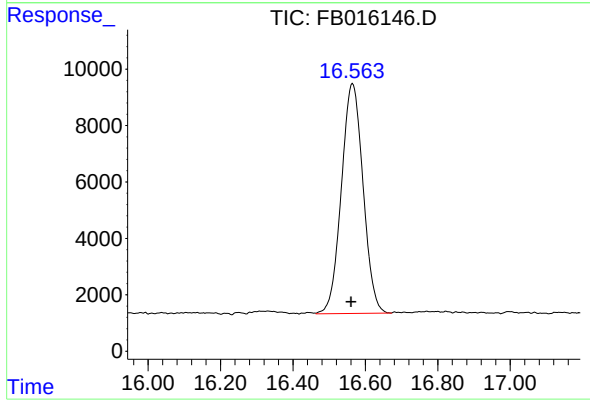

#10 1,2,4-Trimethylbenzene

R.T.: 16.565 min
Delta R.T.: 0.005 min
Response: 338449
Conc: 19.65 ng/ml