

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061518\
 Data File : FB016181.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jun 2018 17:48
 Operator : MJ/SJ
 Sample : J3244-01MSD
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 HD-01-061518MSD

Integration File: Calibration.e
 Quant Time: Jun 16 01:34:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Fri Jun 01 13:25:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.119	128731	18.318 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.971	229627	18.936 ng/ml
2) t 2,2,4-Trimethylpentane	7.735	258584	22.328 ng/ml
3) t n-Heptane	8.075	61409	5.611 ng/ml
4) t Benzene	8.212	126656	8.530 ng/ml
6) t Toluene	10.968	317117	25.548 ng/ml
7) t Ethylbenzene	13.417	120248	8.591 ng/ml
8) t m-Xylene	13.550	252519	16.590 ng/ml
9) t O-Xylene	14.282	275613	17.661 ng/ml
10) t 1,2,4-Trimethylbenzene	16.564	304875	17.702 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061518\
Data File : FB0616181.D
Signal(s) : FID2B.CH
Acq On : 15 Jun 2018 17:48
Operator : MJ/SJ
Sample : J3244-01MSD
Misc : 5.00g/5.00mL DI Water
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
HD-01-061518MSD

Integration File: Calibration.e
Quant Time: Jun 16 01:34:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Fri Jun 01 13:25:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

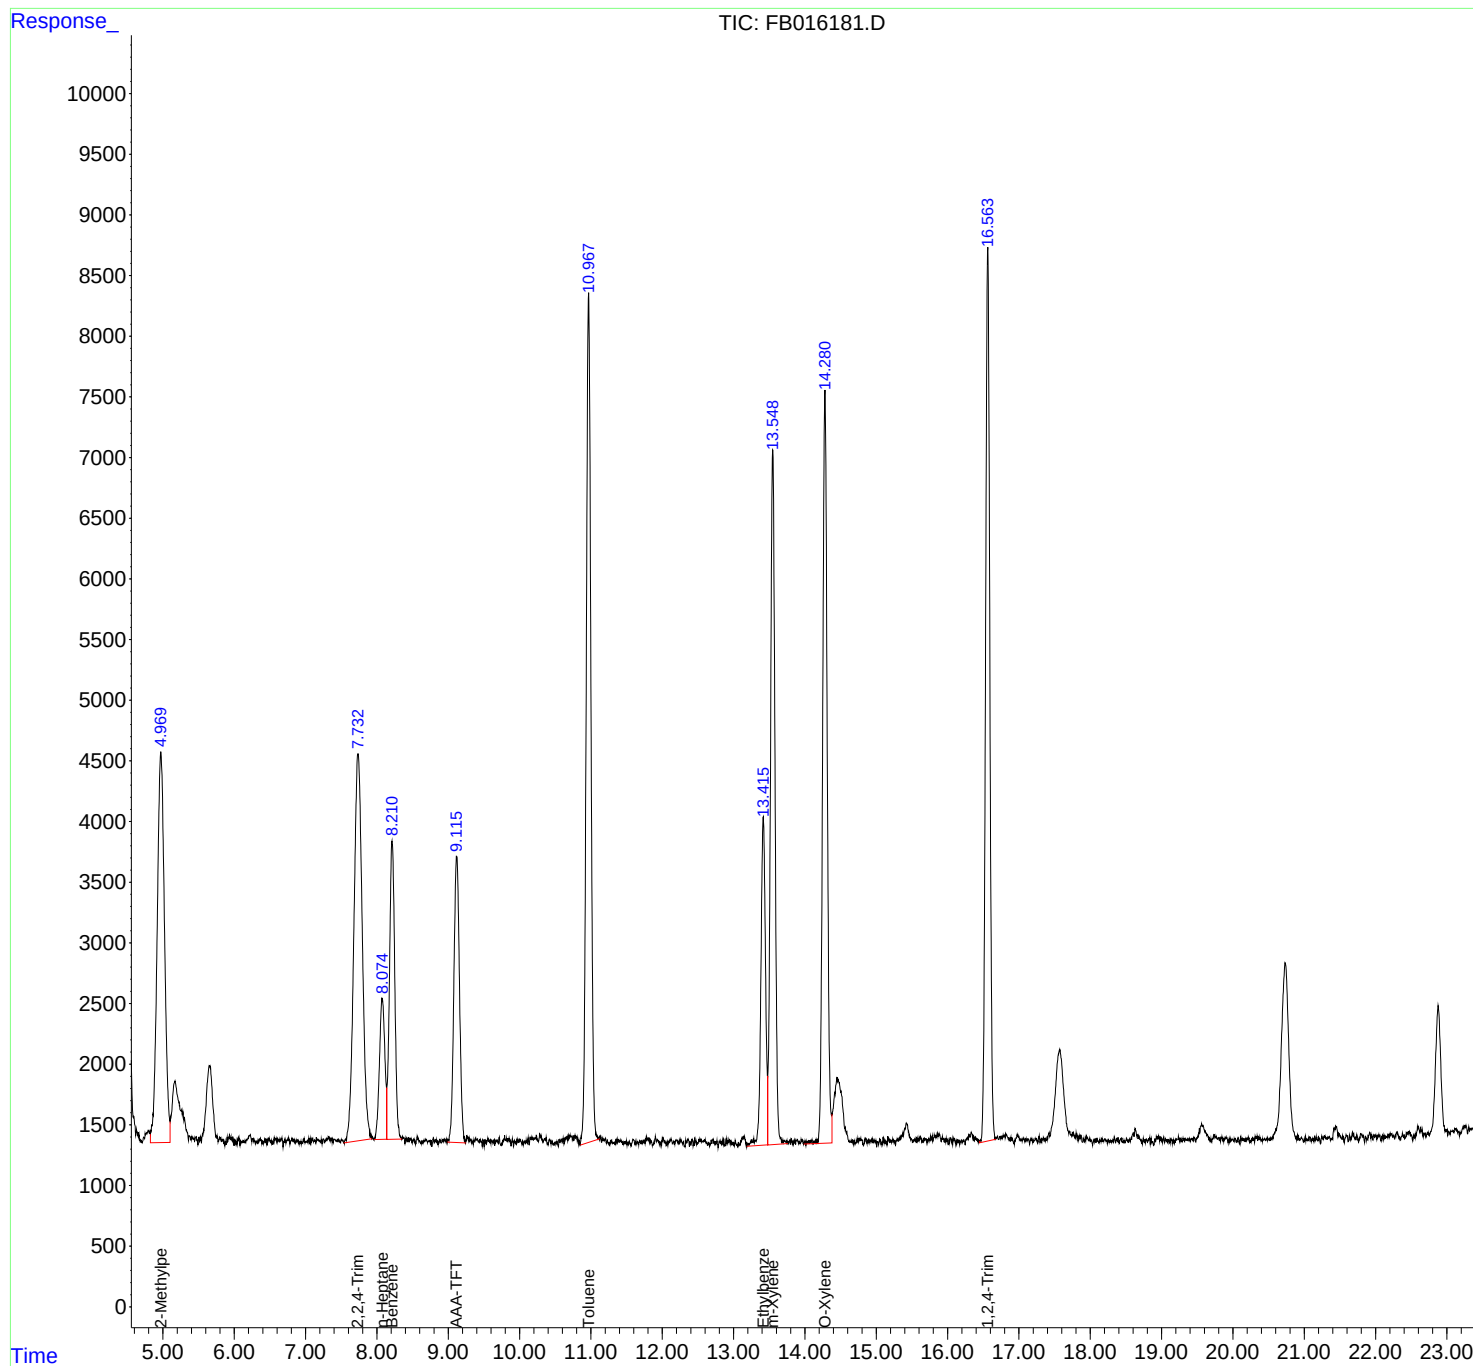


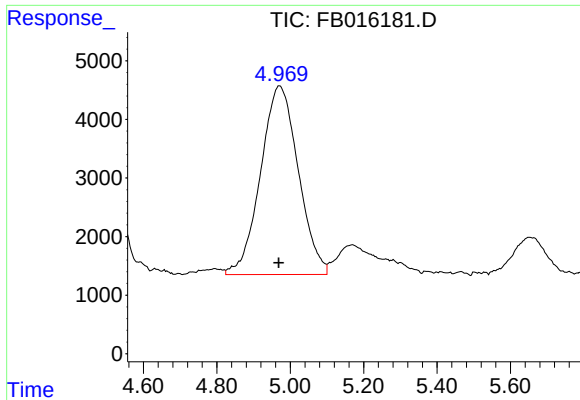

#1 2-Methylpentane


R.T.: 4.971 min
Delta R.T.: 0.002 min
Response: 229627
Conc: 18.94 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-061518MSD

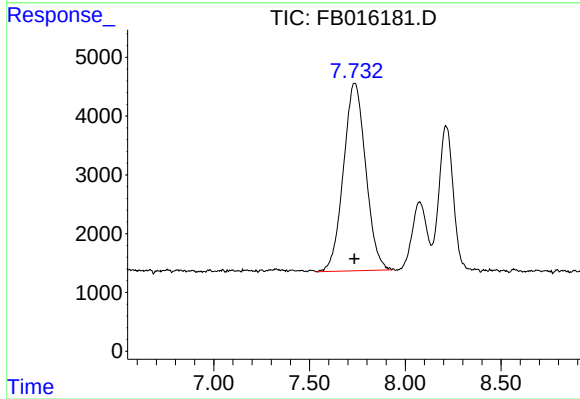


#2 2,2,4-Trimethylpentane

R.T.: 7.735 min
Delta R.T.: 0.002 min
Response: 258584
Conc: 22.33 ng/ml

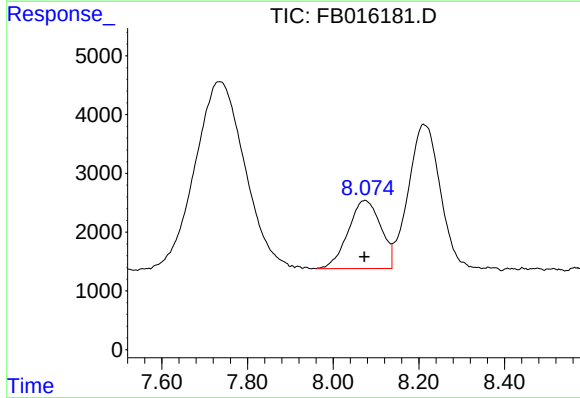


#3 n-Heptane

R.T.: 8.075 min
Delta R.T.: 0.002 min
Response: 61409
Conc: 5.61 ng/ml

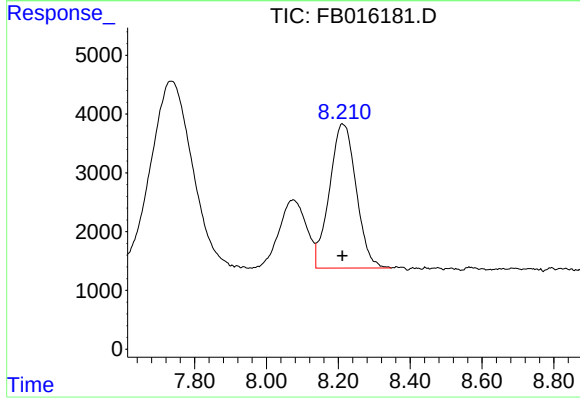

#4 Benzene


R.T.: 8.212 min
Delta R.T.: 0.000 min
Response: 126656
Conc: 8.53 ng/ml

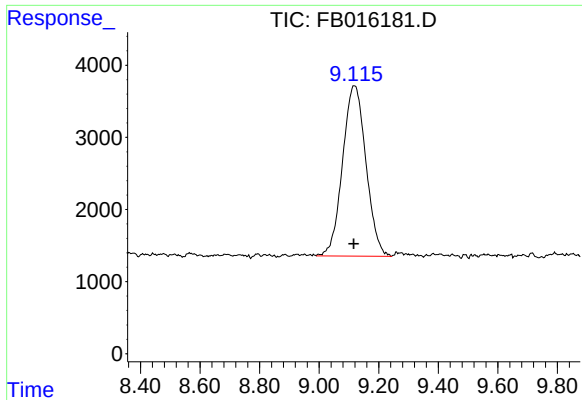

#5 AAA-TFT


R.T.: 9.119 min
Delta R.T.: 0.002 min
Response: 128731
Conc: 18.32 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-061518MSD

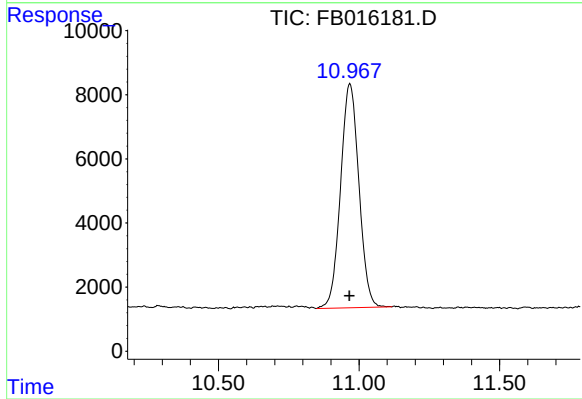


#6 Toluene

R.T.: 10.968 min
Delta R.T.: 0.002 min
Response: 317117
Conc: 25.55 ng/ml

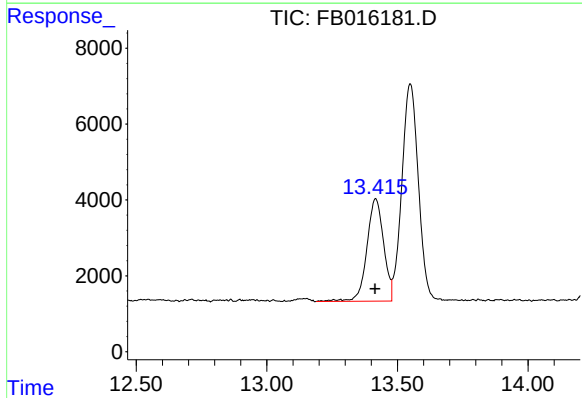


#7 Ethylbenzene

R.T.: 13.417 min
Delta R.T.: 0.003 min
Response: 120248
Conc: 8.59 ng/ml

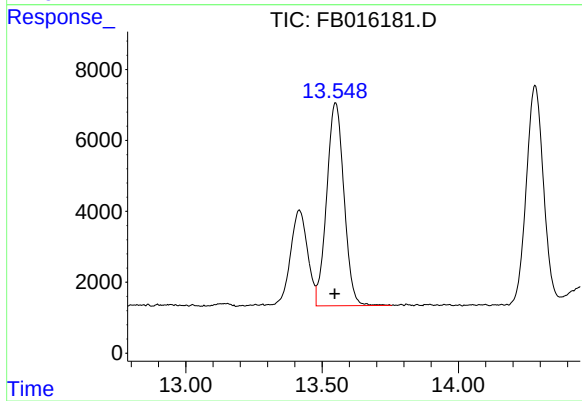

#8 m-Xylene


R.T.: 13.550 min
Delta R.T.: 0.003 min
Response: 252519
Conc: 16.59 ng/ml

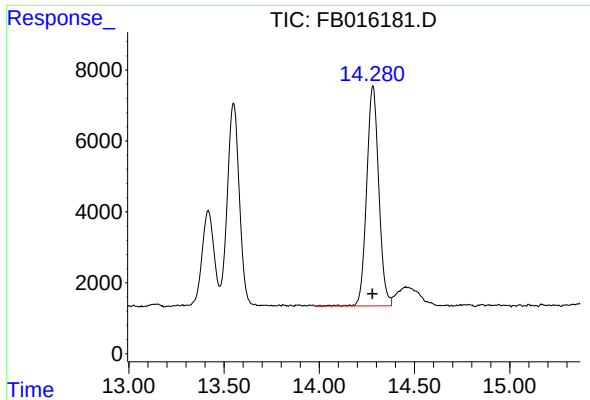

#9 O-Xylene

R.T.: 14.282 min
Delta R.T.: 0.003 min
Response: 275613
Conc: 17.66 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-061518MSD

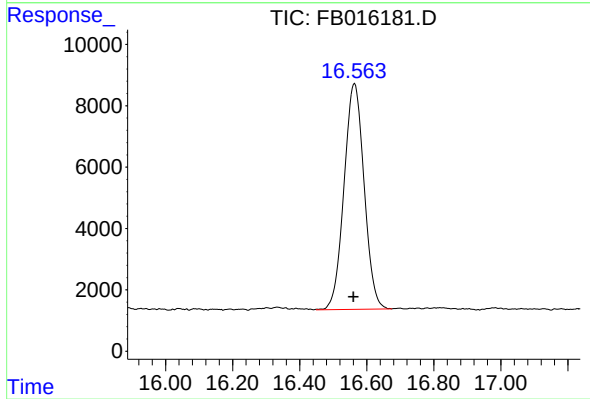

#10 1,2,4-Trimethylbenzene

R.T.: 16.564 min
Delta R.T.: 0.003 min
Response: 304875
Conc: 17.70 ng/ml