

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062218\
 Data File : FB016320.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jun 2018 14:11
 Operator : MJ/SJ
 Sample : BSF0622S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0622S1

Integration File: Calibration.e
 Quant Time: Jun 25 10:12:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Fri Jun 01 13:25:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.116	162191	23.079 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.969	308885	25.473 ng/ml
2) t 2,2,4-Trimethylpentane	7.733	335350	28.957 ng/ml
3) t n-Heptane	8.074	98208	8.973 ng/ml
4) t Benzene	8.212	146149	9.843 ng/ml
6) t Toluene	10.966	356147	28.692 ng/ml
7) t Ethylbenzene	13.416	129793	9.273 ng/ml
8) t m-Xylene	13.548	276908	18.193 ng/ml
9) t O-Xylene	14.280	295884	18.960 ng/ml
10) t 1,2,4-Trimethylbenzene	16.562	340281	19.758 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062218\
Data File : FB016320.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2018 14:11
Operator : MJ/SJ
Sample : BSF0622S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0622S1

Integration File: Calibration.e
Quant Time: Jun 25 10:12:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Fri Jun 01 13:25:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

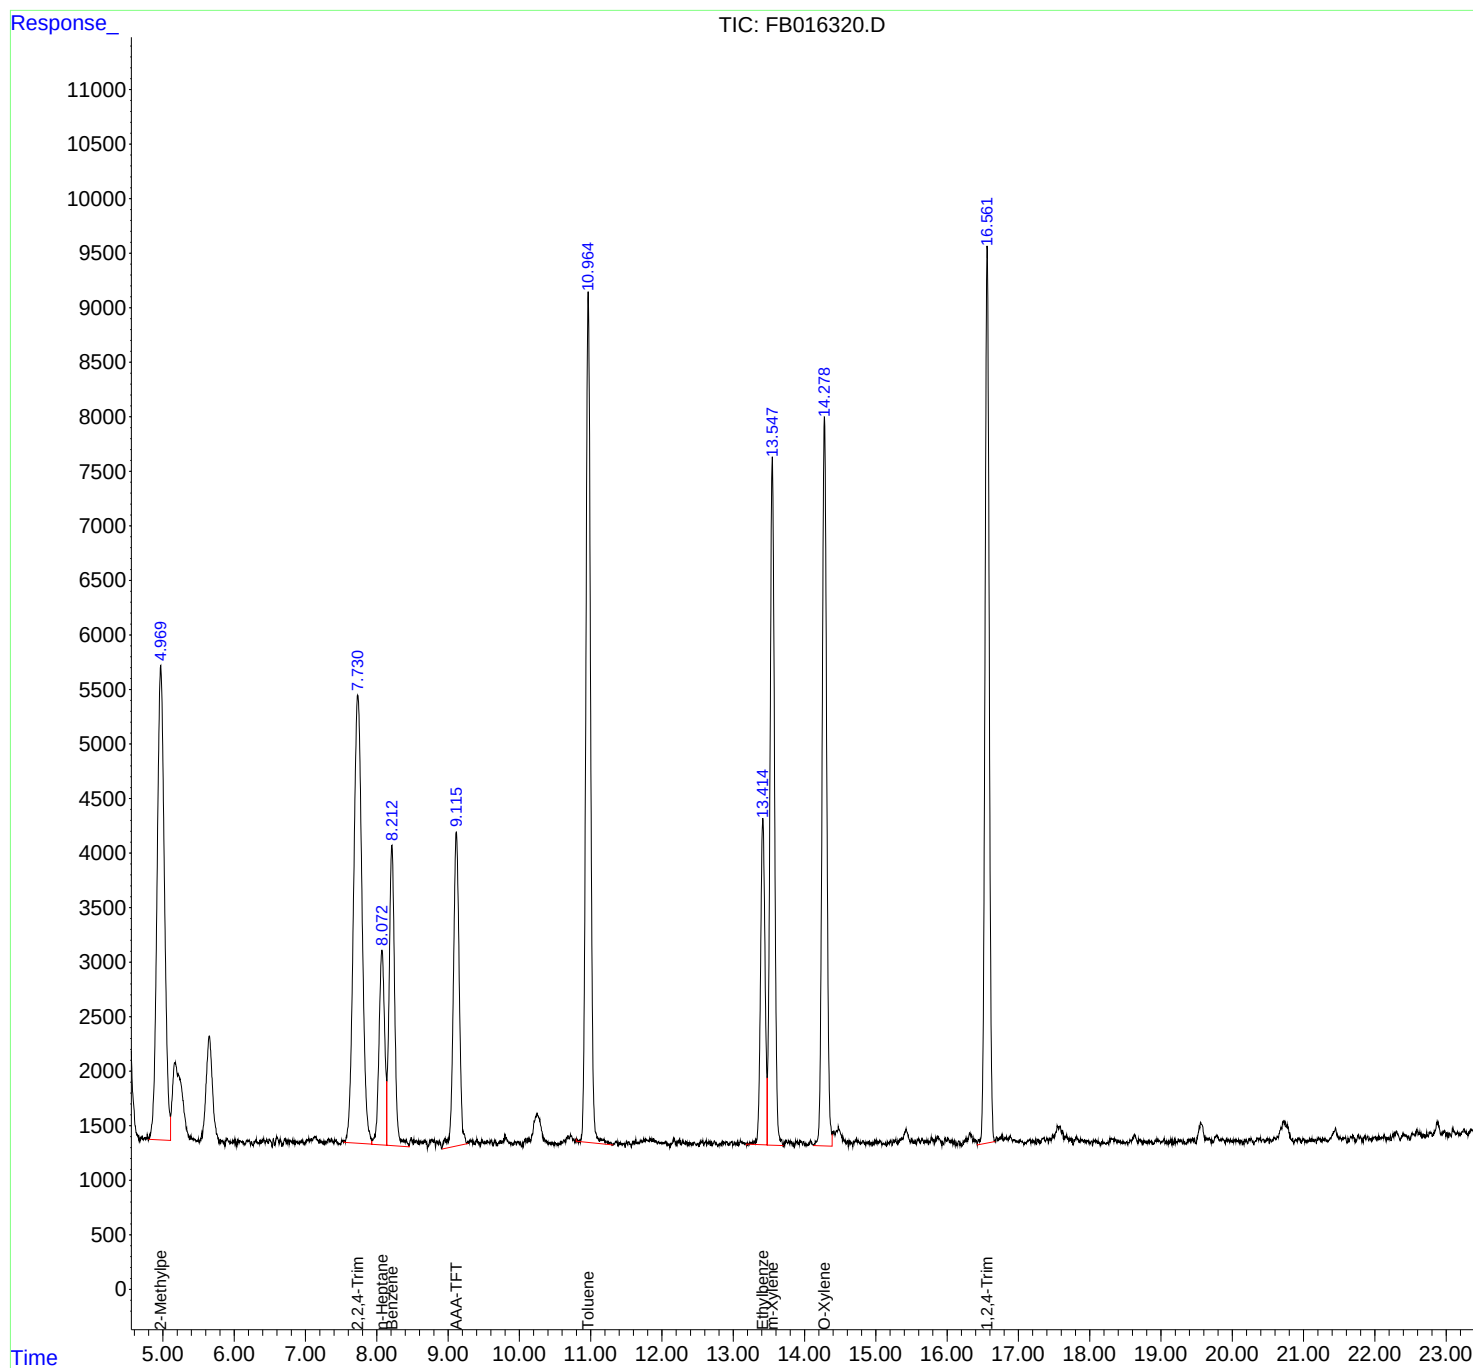


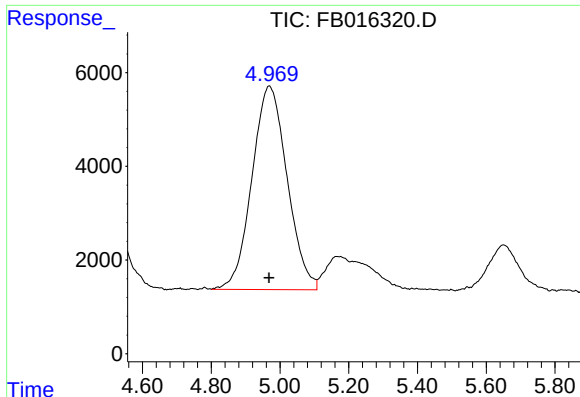

#1 2-Methylpentane


R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 308885
Conc: 25.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0622S1

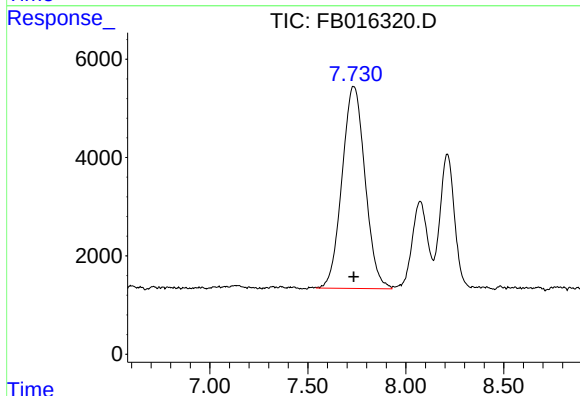


#2 2,2,4-Trimethylpentane

R.T.: 7.733 min
Delta R.T.: -0.001 min
Response: 335350
Conc: 28.96 ng/ml

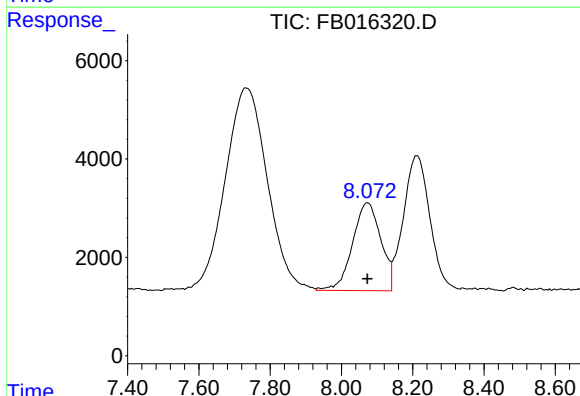


#3 n-Heptane

R.T.: 8.074 min
Delta R.T.: 0.000 min
Response: 98208
Conc: 8.97 ng/ml

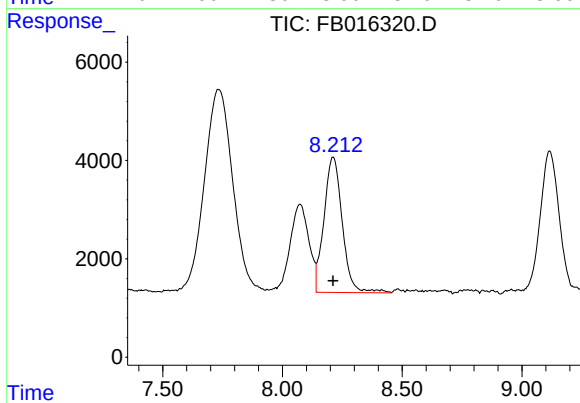

#4 Benzene


R.T.: 8.212 min
Delta R.T.: 0.000 min
Response: 146149
Conc: 9.84 ng/ml

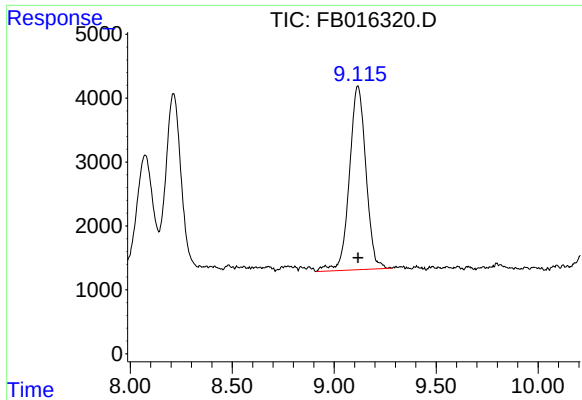

#5 AAA-TFT


R.T.: 9.116 min
Delta R.T.: 0.000 min
Response: 162191
Conc: 23.08 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0622S1

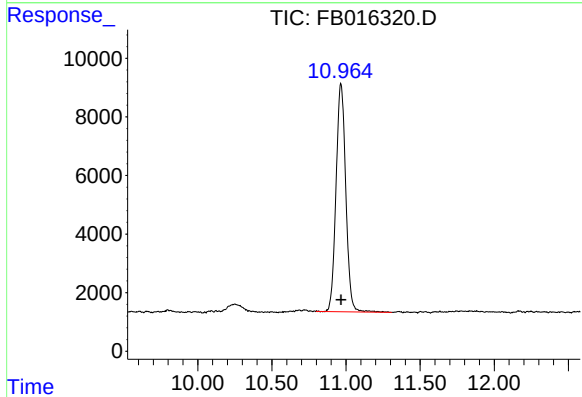


#6 Toluene

R.T.: 10.966 min
Delta R.T.: 0.000 min
Response: 356147
Conc: 28.69 ng/ml

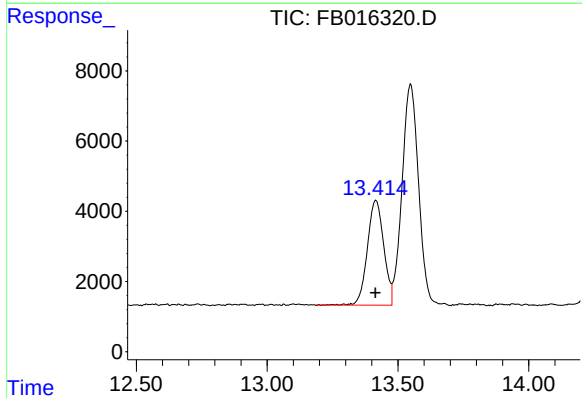


#7 Ethylbenzene

R.T.: 13.416 min
Delta R.T.: 0.001 min
Response: 129793
Conc: 9.27 ng/ml

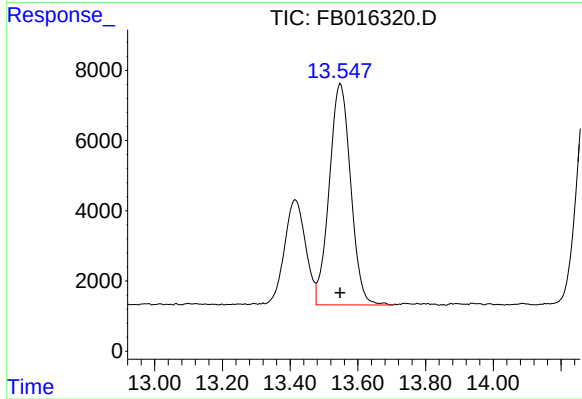

#8 m-Xylene


R.T.: 13.548 min
Delta R.T.: 0.001 min
Response: 276908
Conc: 18.19 ng/ml

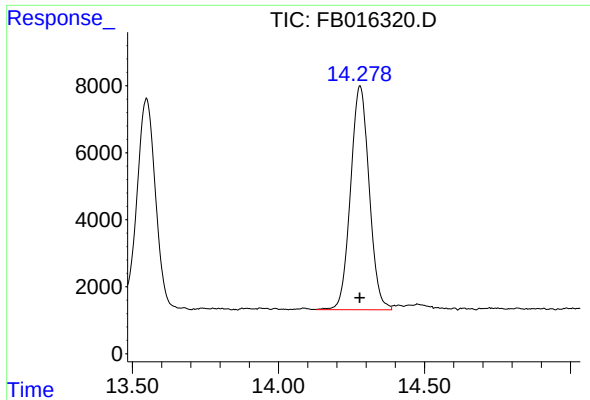

#9 O-Xylene

R.T.: 14.280 min
Delta R.T.: 0.001 min
Response: 295884
Conc: 18.96 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0622S1

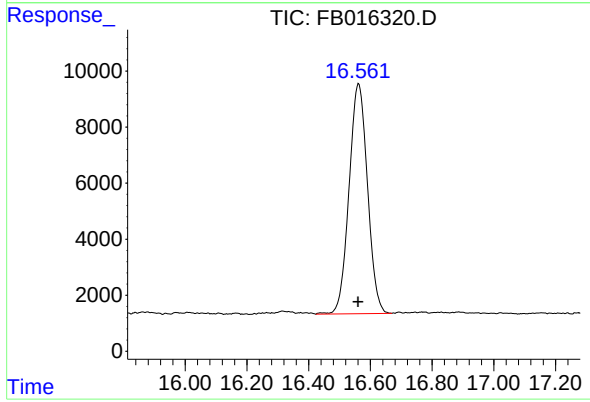

#10 1,2,4-Trimethylbenzene

R.T.: 16.562 min
Delta R.T.: 0.002 min
Response: 340281
Conc: 19.76 ng/ml