

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062218\
 Data File : FB016323.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jun 2018 15:43
 Operator : MJ/SJ
 Sample : J3622-18MS
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SP-D-2MS

Integration File: Calibration.e
 Quant Time: Jun 25 10:12:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Fri Jun 01 13:25:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.116	129284	18.396 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.968	249002	20.534 ng/ml
2) t 2,2,4-Trimethylpentane	7.733	279322	24.119 ng/ml
3) t n-Heptane	8.075	80837	7.386 ng/ml
4) t Benzene	8.211	115675	7.791 ng/ml
6) t Toluene	10.965	296863	23.916 ng/ml
7) t Ethylbenzene	13.416	112825	8.060 ng/ml
8) t m-Xylene	13.548	241028	15.835 ng/ml
9) t O-Xylene	14.280	254327	16.297 ng/ml
10) t 1,2,4-Trimethylbenzene	16.562	284171	16.500 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062218\
Data File : FB016323.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2018 15:43
Operator : MJ/SJ
Sample : J3622-18MS
Misc : 5.00g/5.00mL DI Water
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SP-D-2MS

Integration File: Calibration.e
Quant Time: Jun 25 10:12:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Fri Jun 01 13:25:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

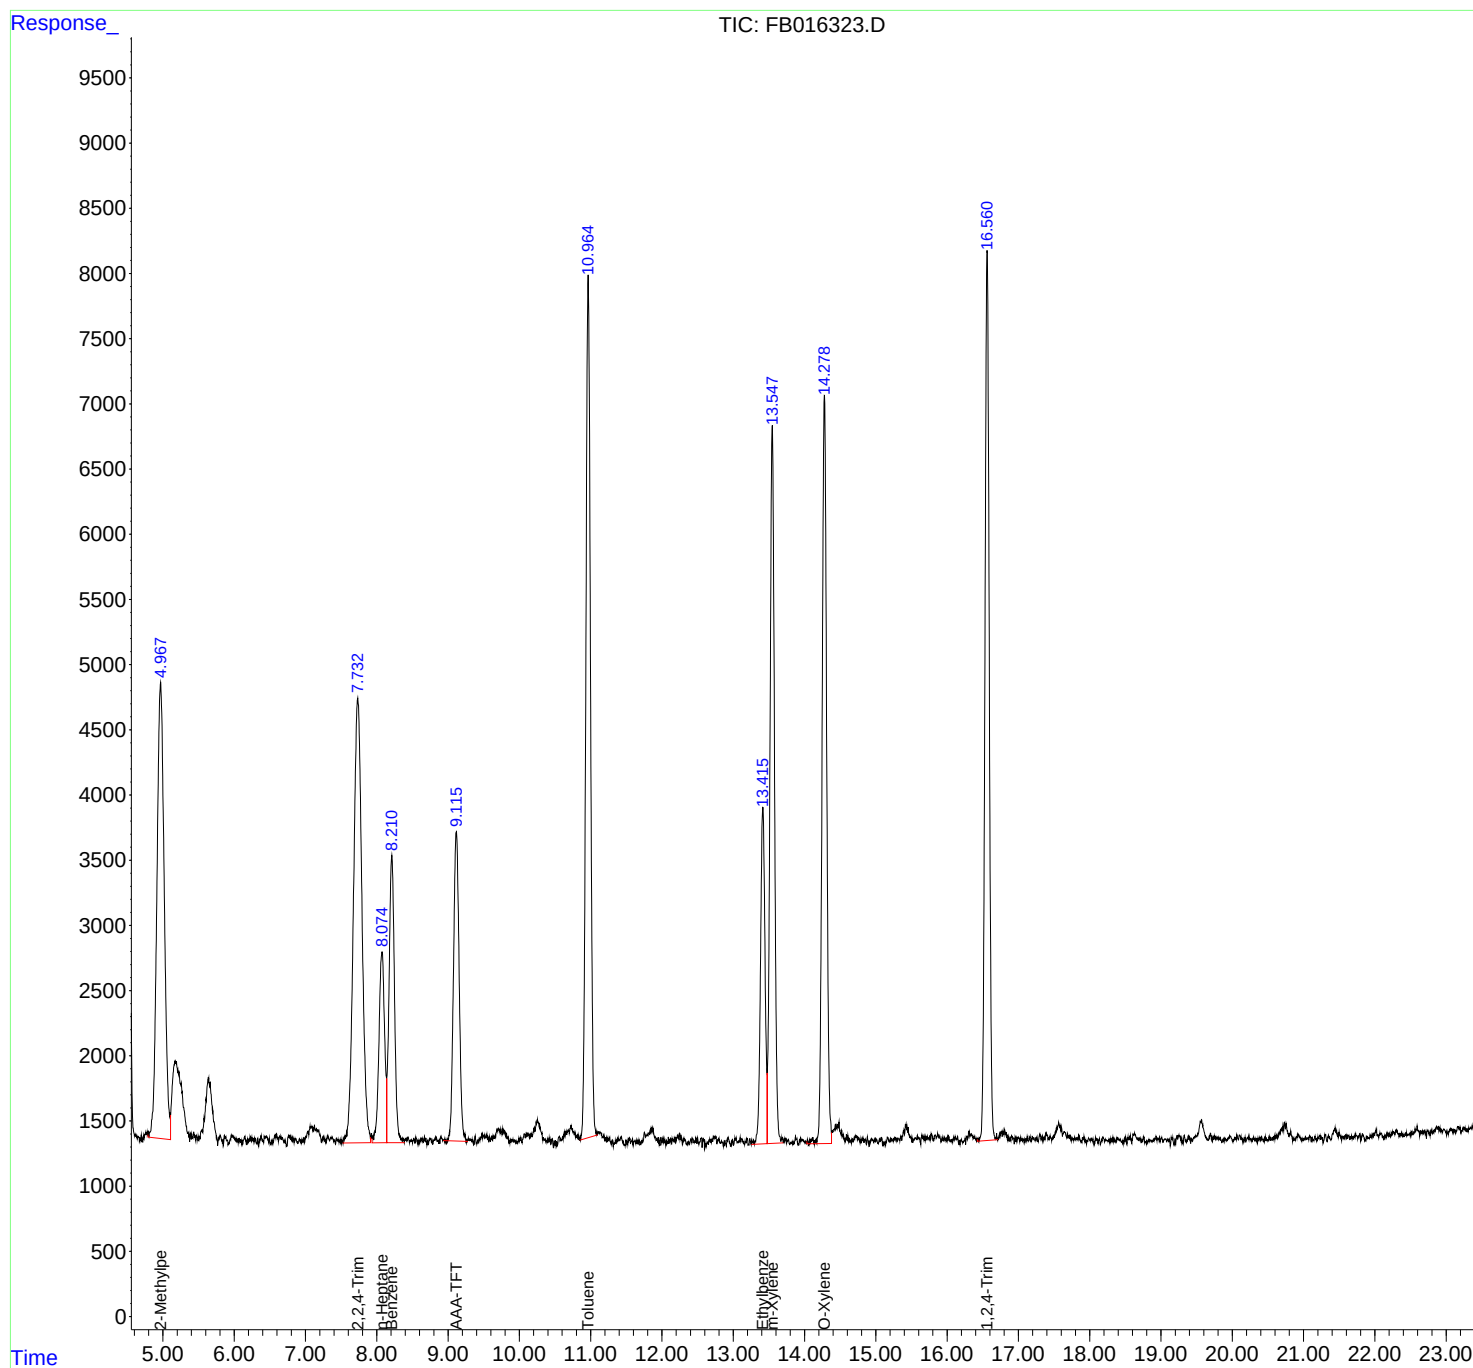


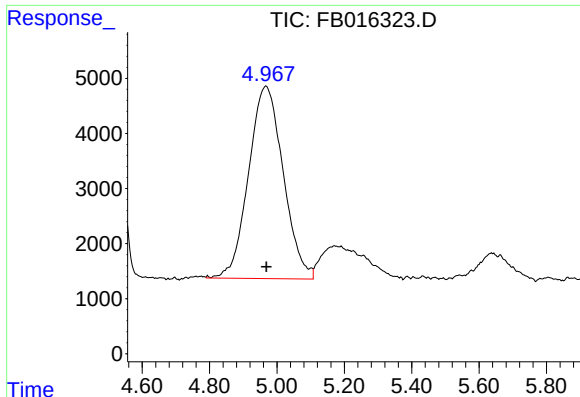

#1 2-Methylpentane


R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 249002
Conc: 20.53 ng/ml

Instrument :
FID_B
ClientSampleId :
SP-D-2MS

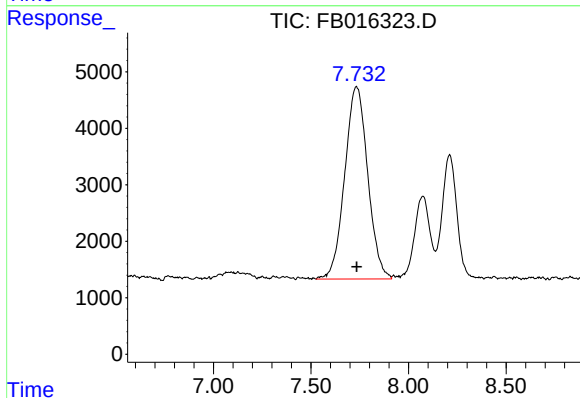


#2 2,2,4-Trimethylpentane

R.T.: 7.733 min
Delta R.T.: -0.001 min
Response: 279322
Conc: 24.12 ng/ml

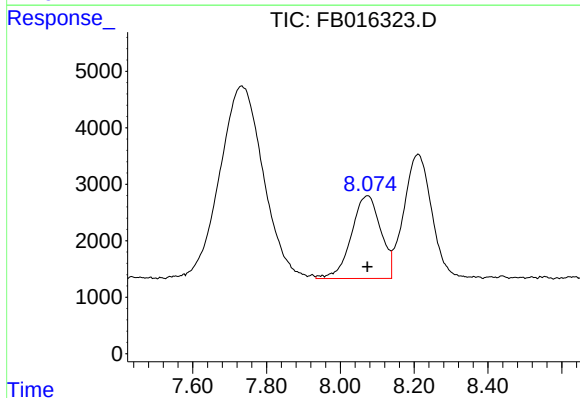


#3 n-Heptane

R.T.: 8.075 min
Delta R.T.: 0.002 min
Response: 80837
Conc: 7.39 ng/ml

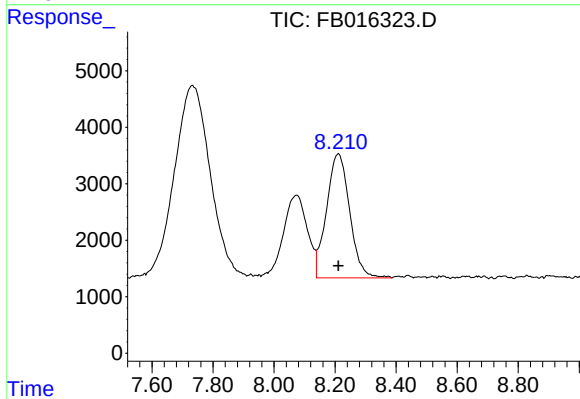

#4 Benzene


R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 115675
Conc: 7.79 ng/ml

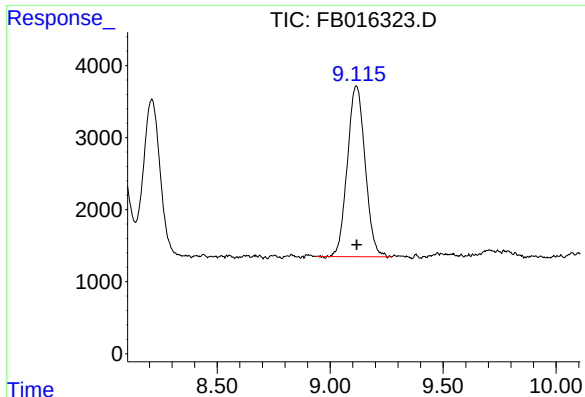

#5 AAA-TFT


R.T.: 9.116 min
Delta R.T.: 0.000 min
Response: 129284
Conc: 18.40 ng/ml

Instrument :
FID_B
ClientSampleId :
SP-D-2MS

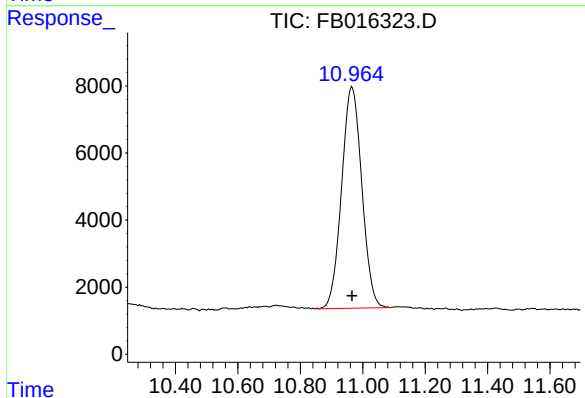


#6 Toluene

R.T.: 10.965 min
Delta R.T.: 0.000 min
Response: 296863
Conc: 23.92 ng/ml

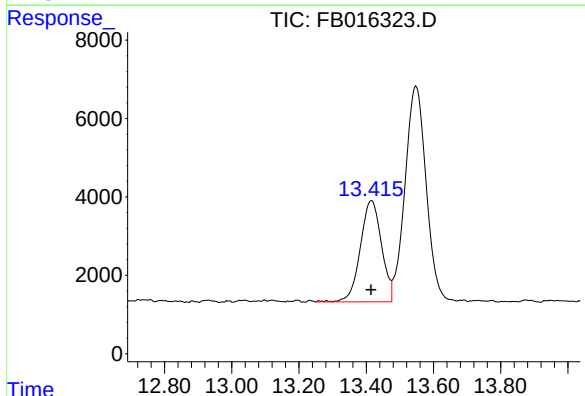


#7 Ethylbenzene

R.T.: 13.416 min
Delta R.T.: 0.001 min
Response: 112825
Conc: 8.06 ng/ml

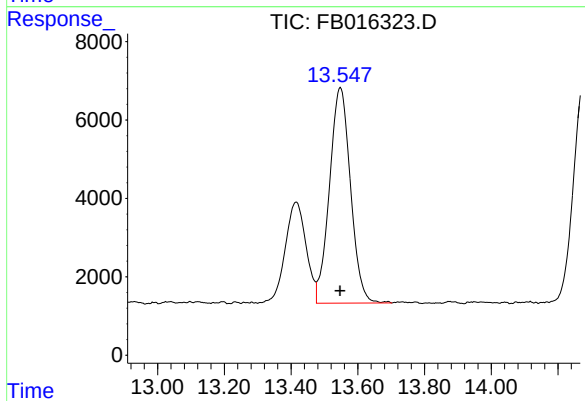

#8 m-Xylene


R.T.: 13.548 min
Delta R.T.: 0.001 min
Response: 241028
Conc: 15.84 ng/ml

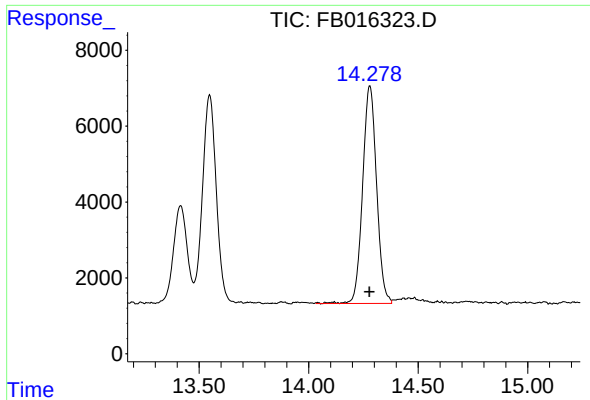

#9 O-Xylene

R.T.: 14.280 min
Delta R.T.: 0.001 min
Response: 254327
Conc: 16.30 ng/ml

Instrument :
FID_B
ClientSampleId :
SP-D-2MS

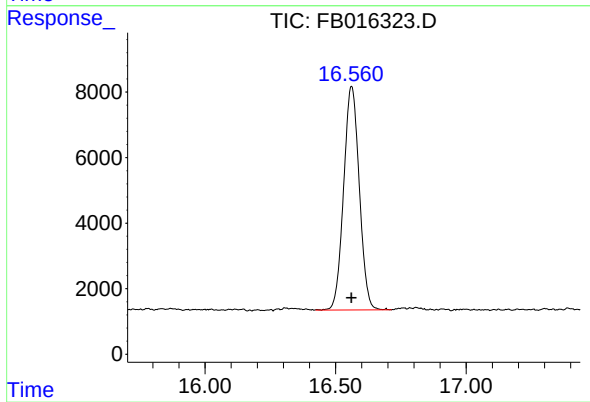

#10 1,2,4-Trimethylbenzene

R.T.: 16.562 min
Delta R.T.: 0.001 min
Response: 284171
Conc: 16.50 ng/ml