

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062218\
 Data File : FB016324.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jun 2018 16:14
 Operator : MJ/SJ
 Sample : J3622-18MSD
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SP-D-2MSD

Integration File: Calibration.e
 Quant Time: Jun 25 10:12:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Fri Jun 01 13:25:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.118	146151	20.796 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.969	307288	25.341 ng/ml
2) t 2,2,4-Trimethylpentane	7.734	327931	28.316 ng/ml
3) t n-Heptane	8.073	90754	8.292 ng/ml
4) t Benzene	8.212	138461	9.325 ng/ml
6) t Toluene	10.966	335071	26.994 ng/ml
7) t Ethylbenzene	13.416	119614	8.545 ng/ml
8) t m-Xylene	13.548	257530	16.920 ng/ml
9) t O-Xylene	14.280	271693	17.410 ng/ml
10) t 1,2,4-Trimethylbenzene	16.563	291161	16.906 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062218\
Data File : FB016324.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2018 16:14
Operator : MJ/SJ
Sample : J3622-18MSD
Misc : 5.00g/5.00mL DI Water
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SP-D-2MSD

Integration File: Calibration.e
Quant Time: Jun 25 10:12:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Fri Jun 01 13:25:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

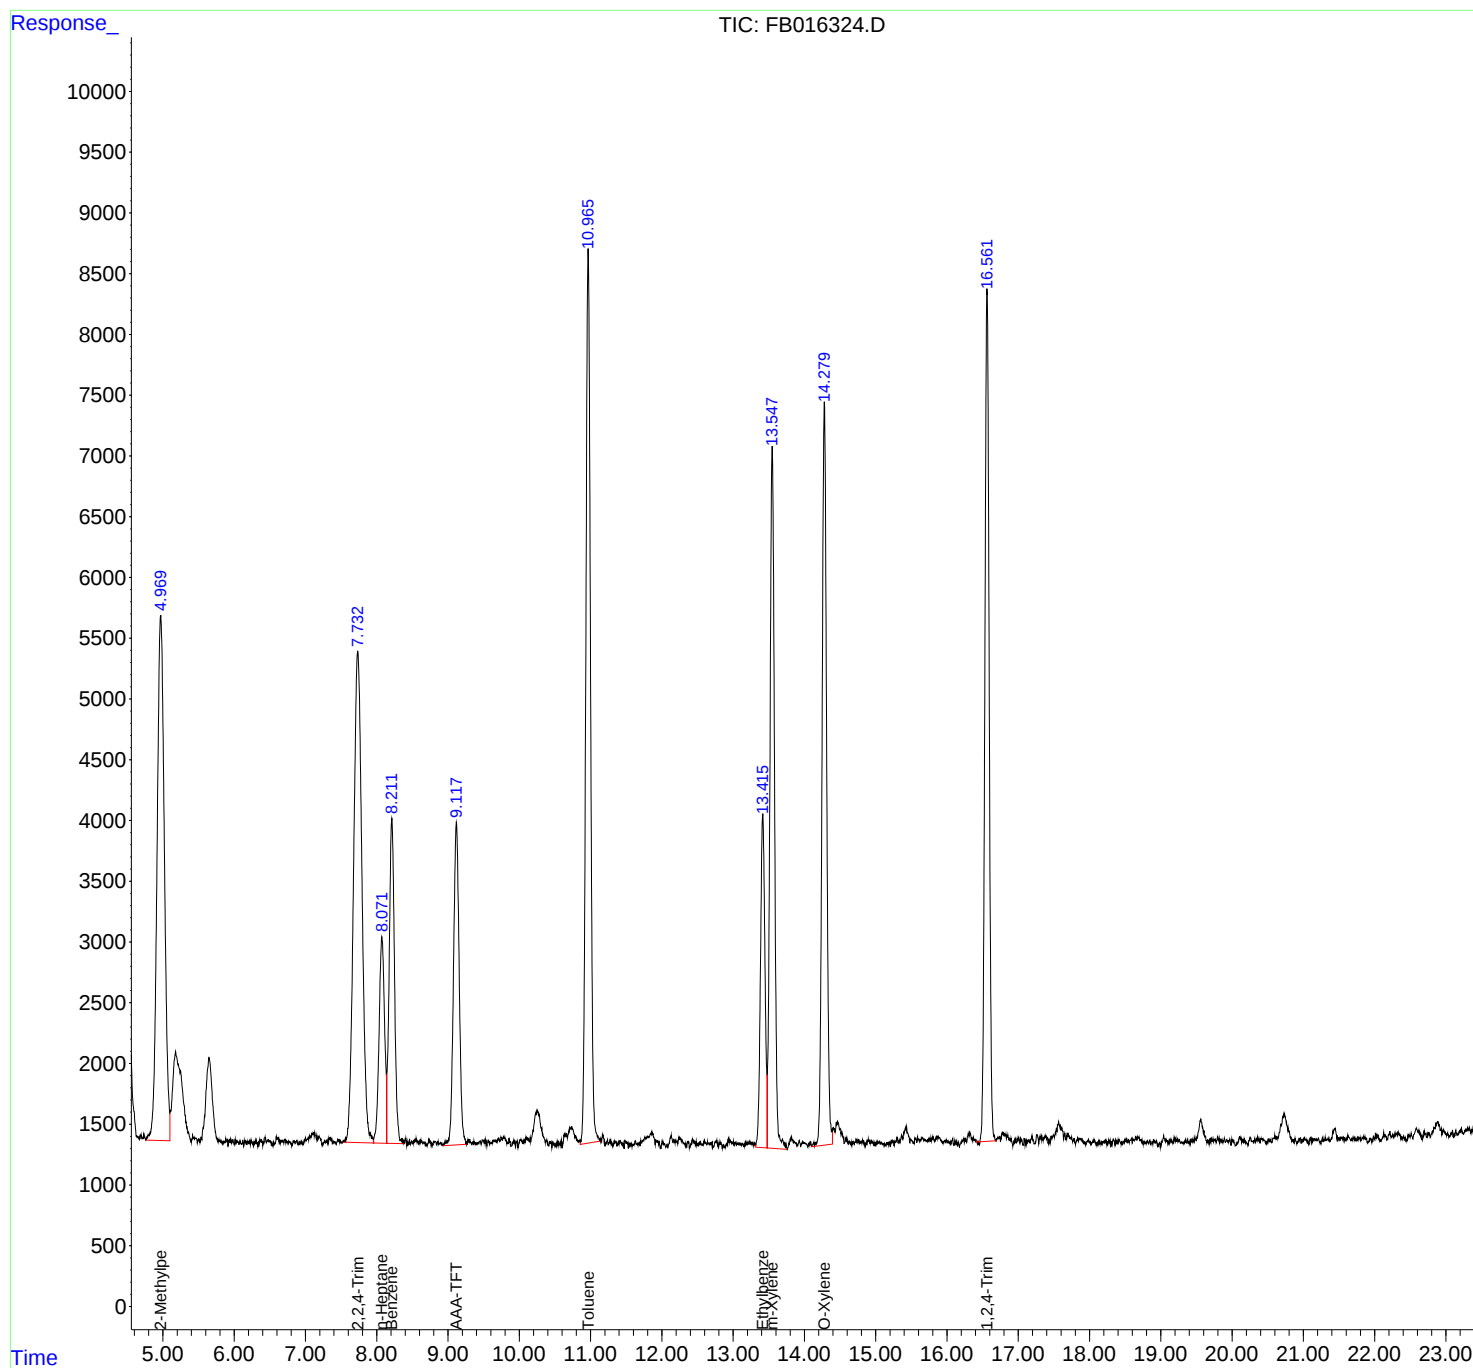


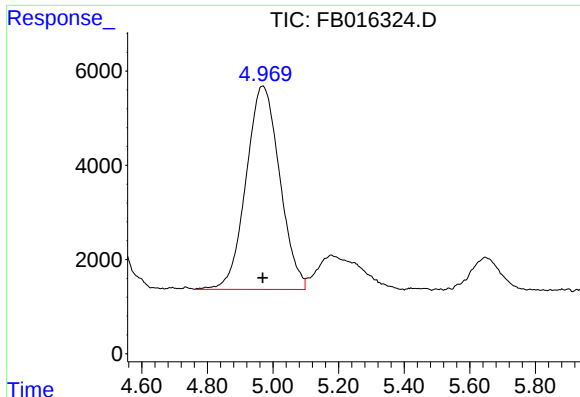

#1 2-Methylpentane


R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 307288
Conc: 25.34 ng/ml

Instrument :
FID_B
ClientSampleId :
SP-D-2MSD

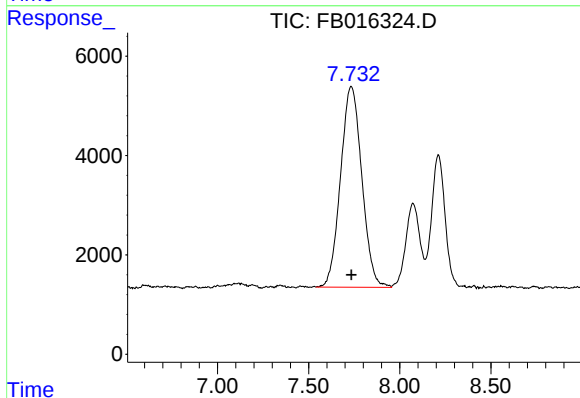


#2 2,2,4-Trimethylpentane

R.T.: 7.734 min
Delta R.T.: 0.000 min
Response: 327931
Conc: 28.32 ng/ml

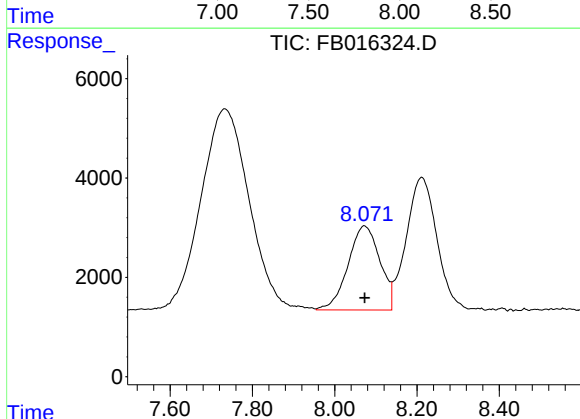


#3 n-Heptane

R.T.: 8.073 min
Delta R.T.: 0.000 min
Response: 90754
Conc: 8.29 ng/ml

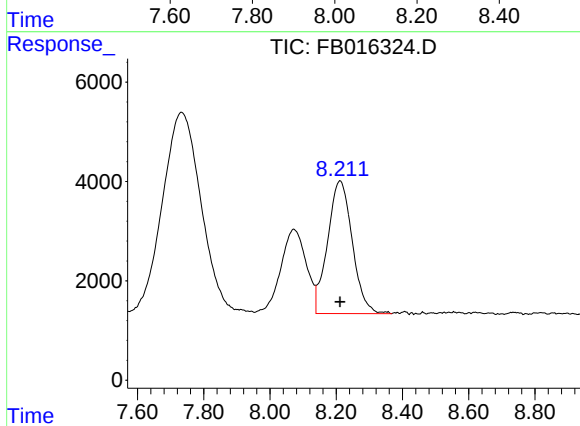

#4 Benzene


R.T.: 8.212 min
Delta R.T.: 0.000 min
Response: 138461
Conc: 9.33 ng/ml

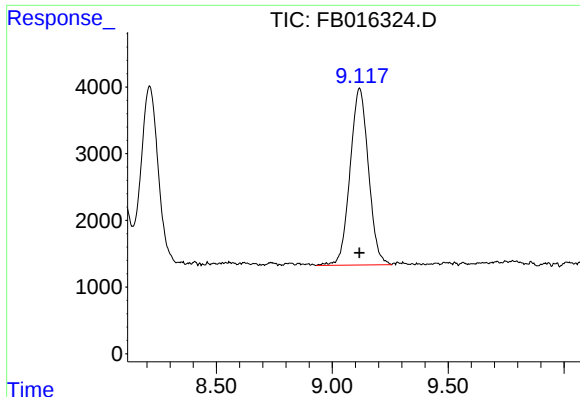

#5 AAA-TFT


R.T.: 9.118 min
Delta R.T.: 0.001 min
Response: 146151
Conc: 20.80 ng/ml

Instrument :
FID_B
ClientSampleId :
SP-D-2MSD

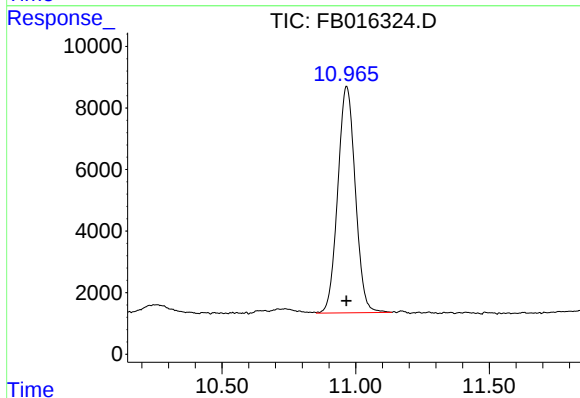


#6 Toluene

R.T.: 10.966 min
Delta R.T.: 0.000 min
Response: 335071
Conc: 26.99 ng/ml

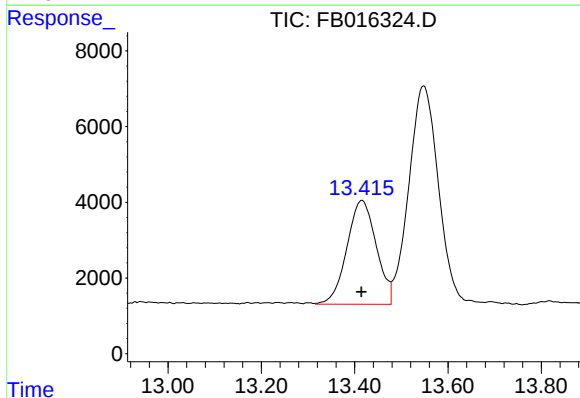


#7 Ethylbenzene

R.T.: 13.416 min
Delta R.T.: 0.002 min
Response: 119614
Conc: 8.55 ng/ml

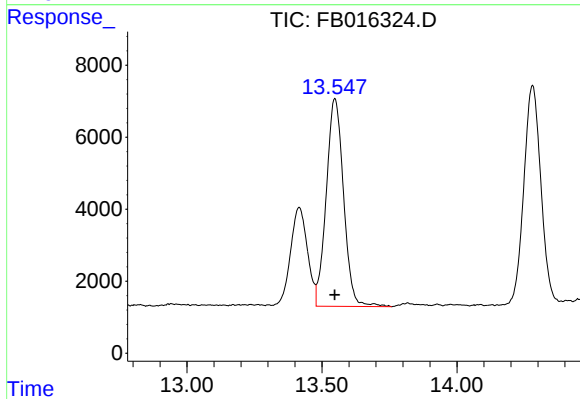

#8 m-Xylene


R.T.: 13.548 min
Delta R.T.: 0.001 min
Response: 257530
Conc: 16.92 ng/ml

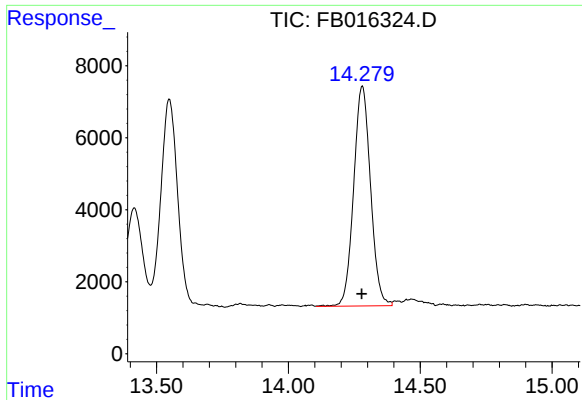

#9 O-Xylene

R.T.: 14.280 min
Delta R.T.: 0.002 min
Response: 271693
Conc: 17.41 ng/ml

Instrument :
FID_B
ClientSampleId :
SP-D-2MSD

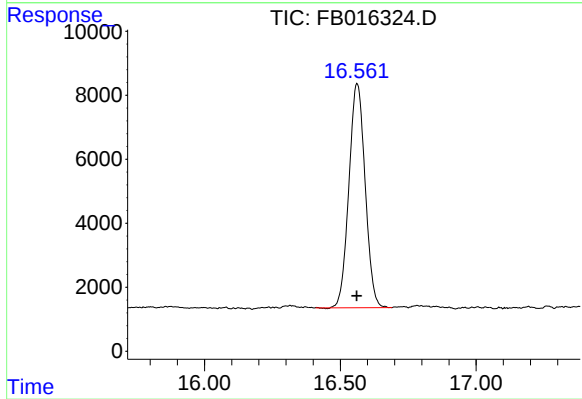

#10 1,2,4-Trimethylbenzene

R.T.: 16.563 min
Delta R.T.: 0.002 min
Response: 291161
Conc: 16.91 ng/ml