

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062518\
 Data File : FB016366.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jun 2018 16:21
 Operator : MJ/SJ
 Sample : BSF0625S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0625S1

Integration File: Calibration.e
 Quant Time: Jun 25 18:27:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Fri Jun 01 13:25:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.118	151204	21.515 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.968	427054	35.217 ng/ml
2) t 2,2,4-Trimethylpentane	7.732	409520	35.361 ng/ml
3) t n-Heptane	8.072	128553	11.746 ng/ml
4) t Benzene	8.211	187069	12.599 ng/ml
6) t Toluene	10.966	391178	31.514 ng/ml
7) t Ethylbenzene	13.415	138027	9.861 ng/ml
8) t m-Xylene	13.547	296955	19.510 ng/ml
9) t O-Xylene	14.279	313000	20.057 ng/ml
10) t 1,2,4-Trimethylbenzene	16.562	348414	20.230 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062518\
Data File : FB016366.D
Signal(s) : FID2B.CH
Acq On : 25 Jun 2018 16:21
Operator : MJ/SJ
Sample : BSF0625S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0625S1

Integration File: Calibration.e
Quant Time: Jun 25 18:27:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Fri Jun 01 13:25:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

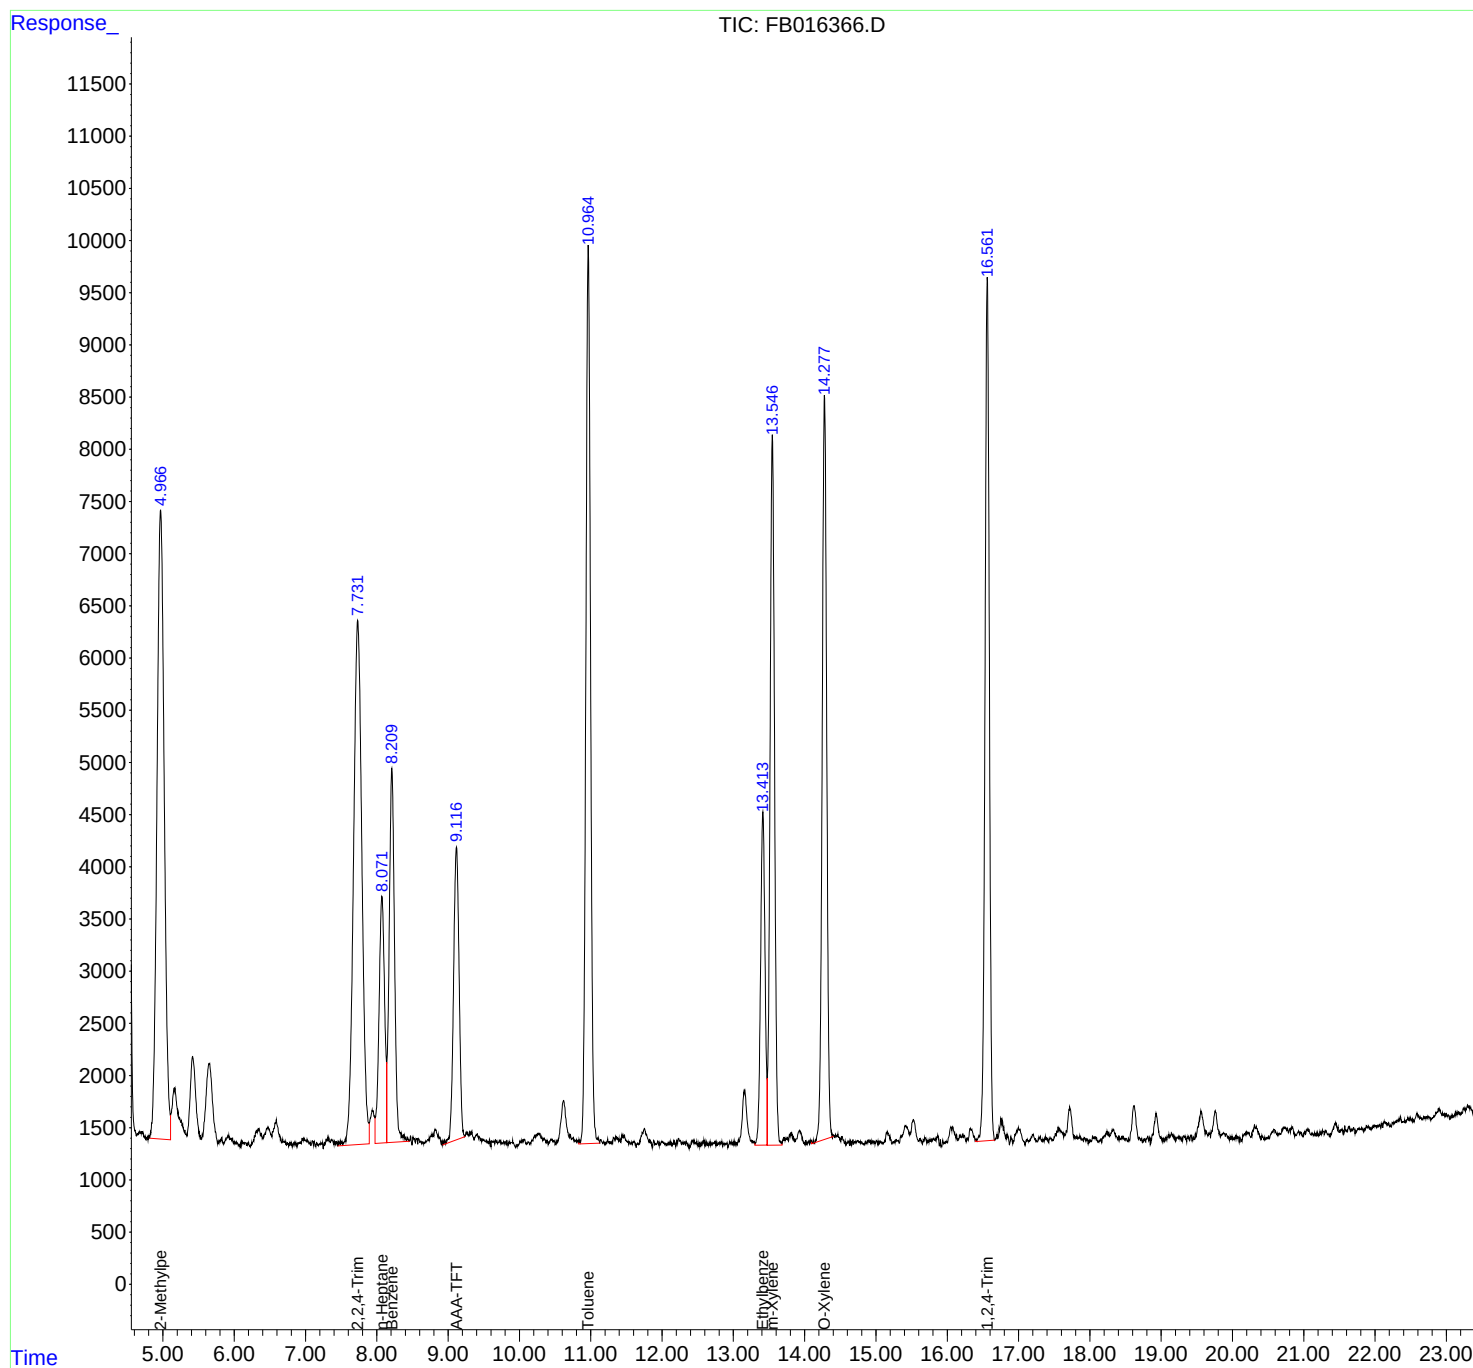


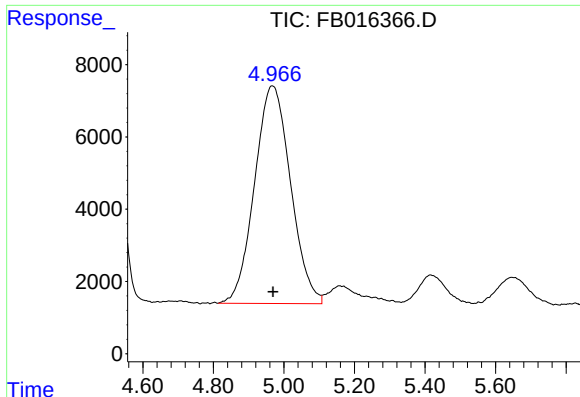

#1 2-Methylpentane


R.T.: 4.968 min
Delta R.T.: -0.001 min
Response: 427054
Conc: 35.22 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0625S1

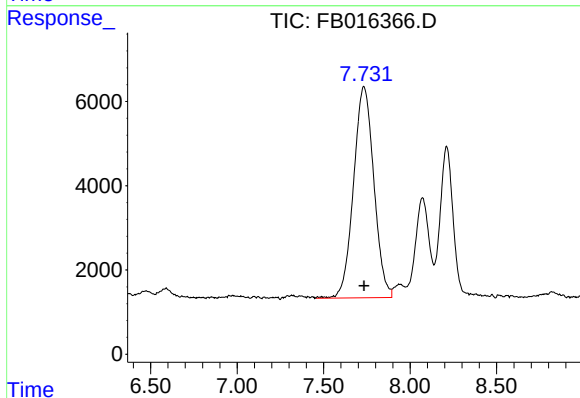


#2 2,2,4-Trimethylpentane

R.T.: 7.732 min
Delta R.T.: -0.001 min
Response: 409520
Conc: 35.36 ng/ml

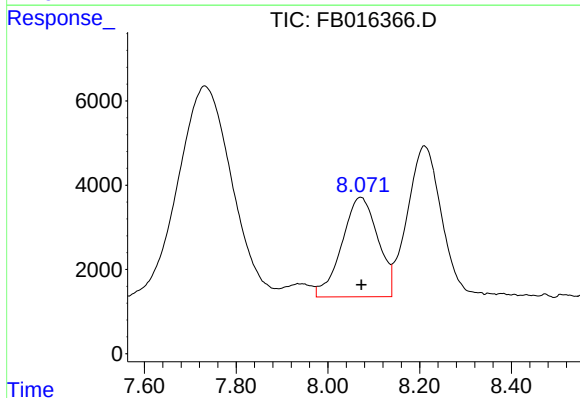


#3 n-Heptane

R.T.: 8.072 min
Delta R.T.: -0.001 min
Response: 128553
Conc: 11.75 ng/ml

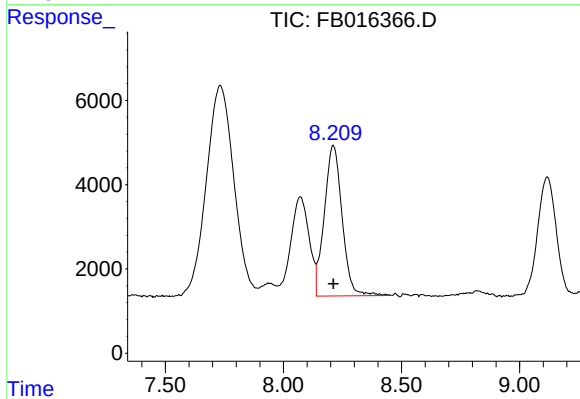

#4 Benzene


R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 187069
Conc: 12.60 ng/ml

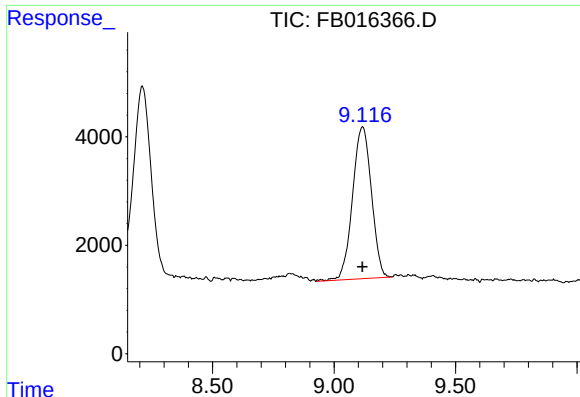

#5 AAA-TFT


R.T.: 9.118 min
Delta R.T.: 0.000 min
Response: 151204
Conc: 21.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0625S1

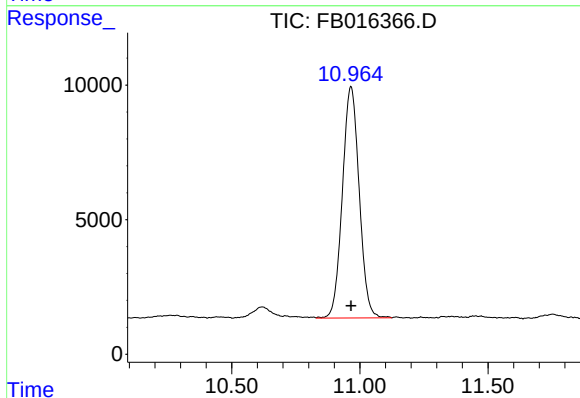


#6 Toluene

R.T.: 10.966 min
Delta R.T.: 0.000 min
Response: 391178
Conc: 31.51 ng/ml

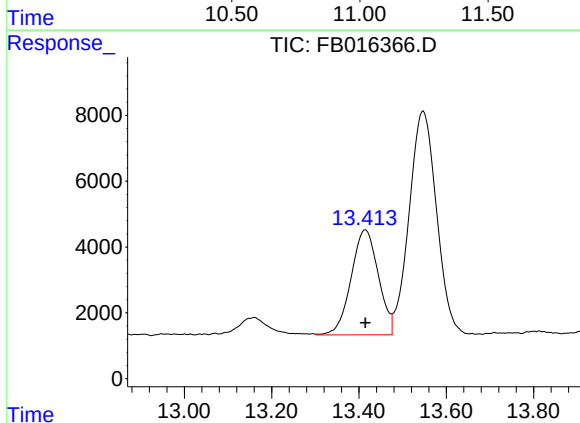


#7 Ethylbenzene

R.T.: 13.415 min
Delta R.T.: 0.000 min
Response: 138027
Conc: 9.86 ng/ml

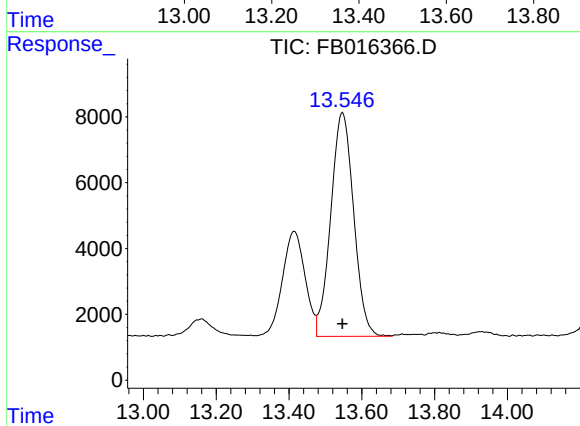

#8 m-Xylene


R.T.: 13.547 min
Delta R.T.: 0.000 min
Response: 296955
Conc: 19.51 ng/ml

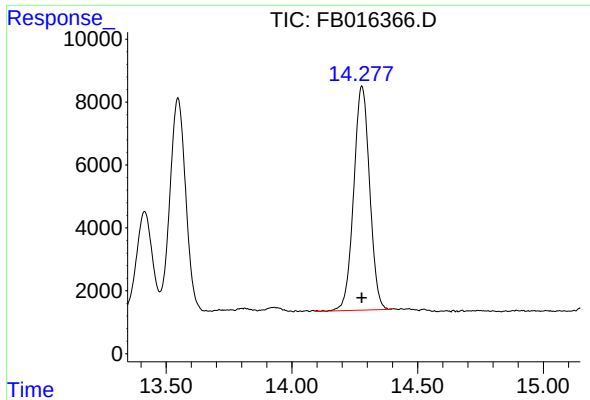

#9 O-Xylene

R.T.: 14.279 min
Delta R.T.: 0.000 min
Response: 313000
Conc: 20.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0625S1

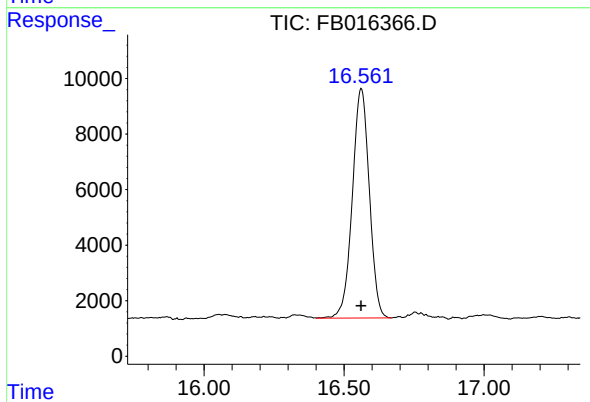

#10 1,2,4-Trimethylbenzene

R.T.: 16.562 min
Delta R.T.: 0.001 min
Response: 348414
Conc: 20.23 ng/ml