

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062518\
 Data File : FB016369.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jun 2018 17:53
 Operator : MJ/SJ
 Sample : J3706-03MS
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 RO-124030MS

Integration File: Calibration.e
 Quant Time: Jun 25 18:27:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Fri Jun 01 13:25:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.117	156329	22.245 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.969	306039	25.238 ng/ml
2) t 2,2,4-Trimethylpentane	7.734	327261	28.258 ng/ml
3) t n-Heptane	8.073	92106	8.416 ng/ml
4) t Benzene	8.212	160823	10.831 ng/ml
6) t Toluene	10.966	334652	26.961 ng/ml
7) t Ethylbenzene	13.415	125304	8.952 ng/ml
8) t m-Xylene	13.548	266798	17.528 ng/ml
9) t O-Xylene	14.279	278158	17.824 ng/ml
10) t 1,2,4-Trimethylbenzene	16.562	331646	19.256 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062518\
Data File : FB016369.D
Signal(s) : FID2B.CH
Acq On : 25 Jun 2018 17:53
Operator : MJ/SJ
Sample : J3706-03MS
Misc : 5.00g/5.00mL DI Water
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RO-124030MS

Integration File: Calibration.e
Quant Time: Jun 25 18:27:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Fri Jun 01 13:25:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

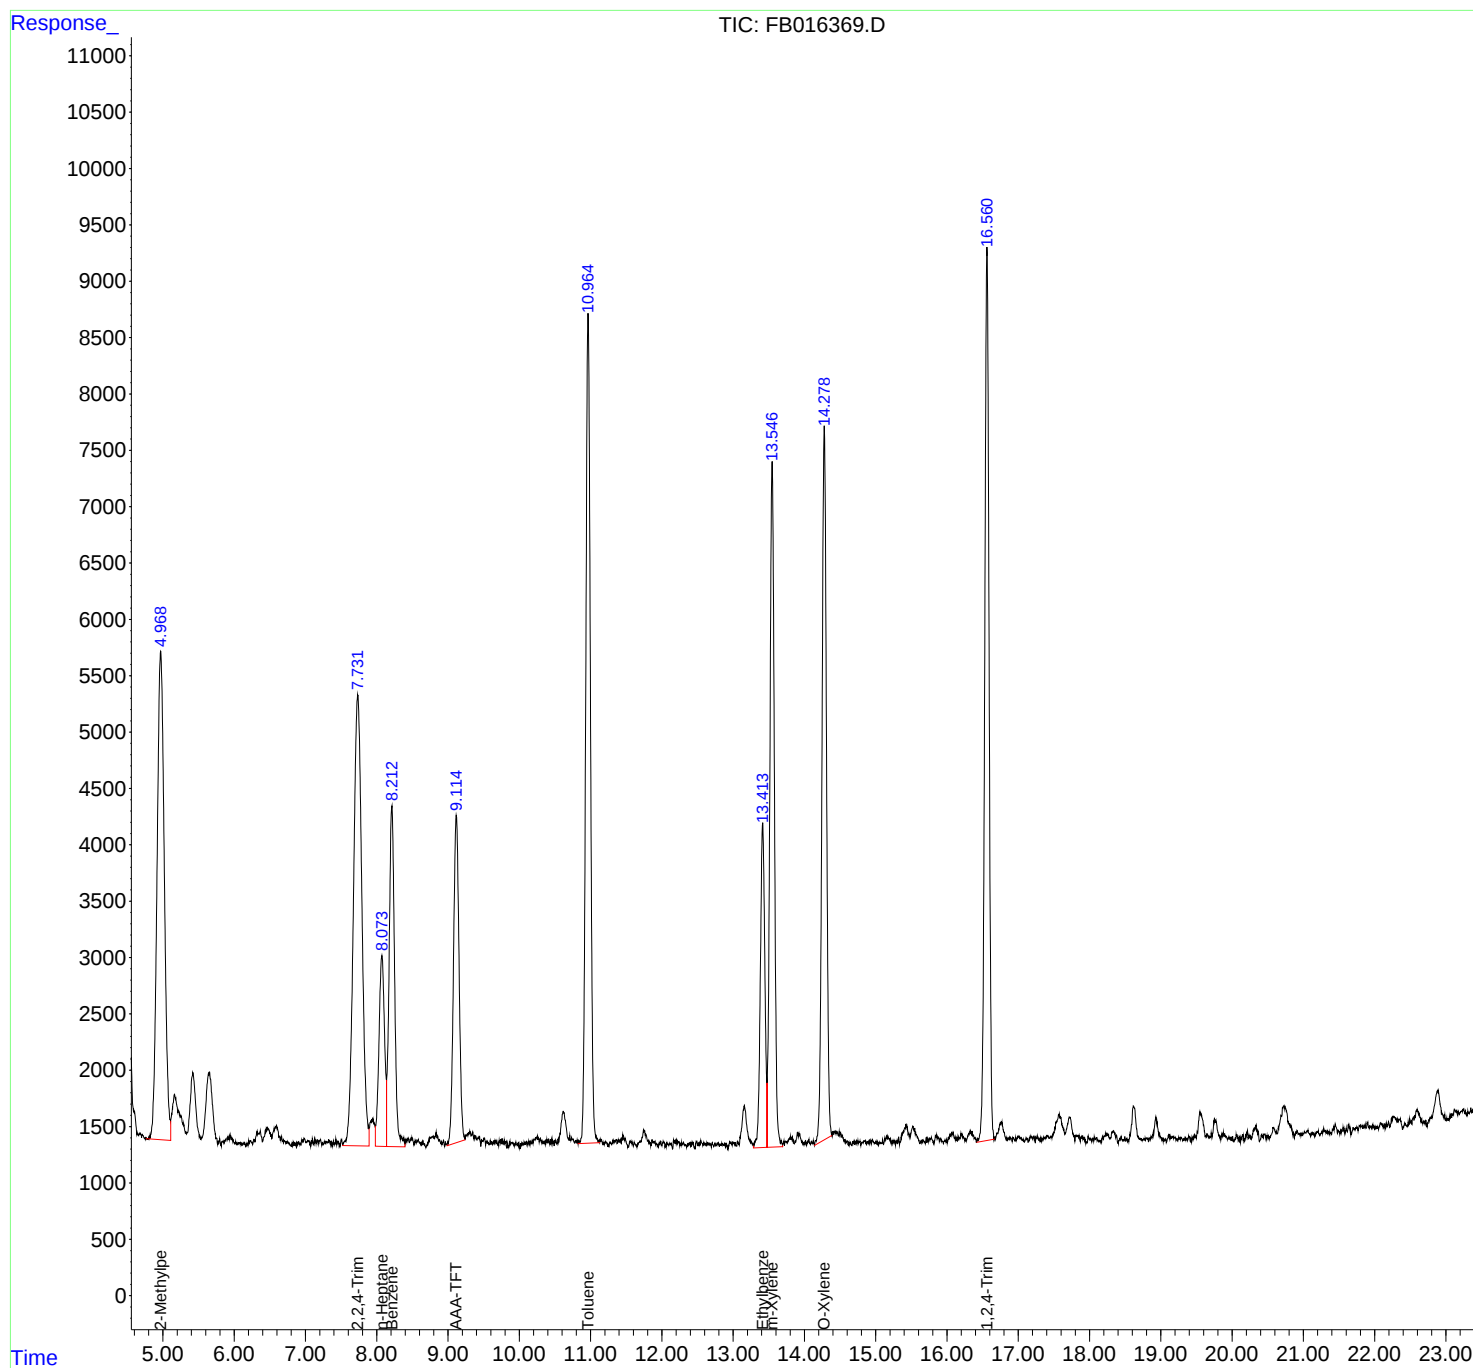


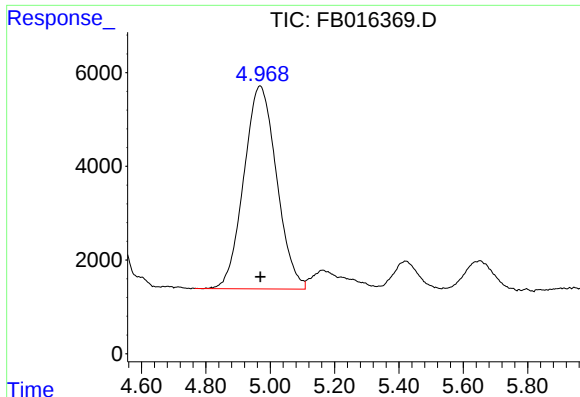

#1 2-Methylpentane


R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 306039
Conc: 25.24 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-124030MS

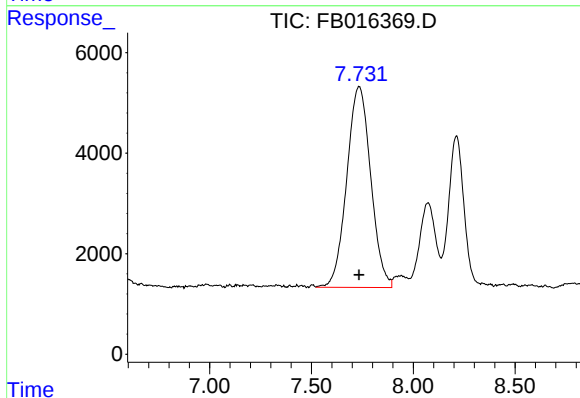


#2 2,2,4-Trimethylpentane

R.T.: 7.734 min
Delta R.T.: 0.000 min
Response: 327261
Conc: 28.26 ng/ml

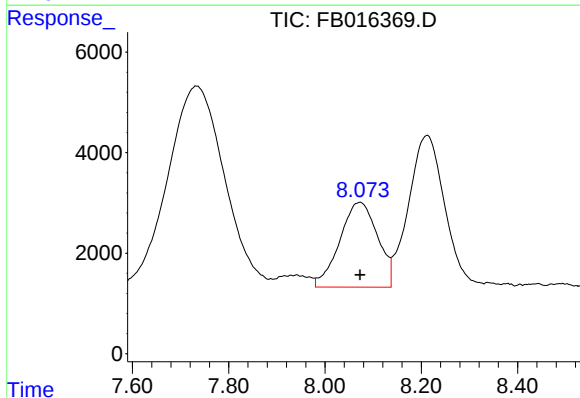


#3 n-Heptane

R.T.: 8.073 min
Delta R.T.: 0.000 min
Response: 92106
Conc: 8.42 ng/ml

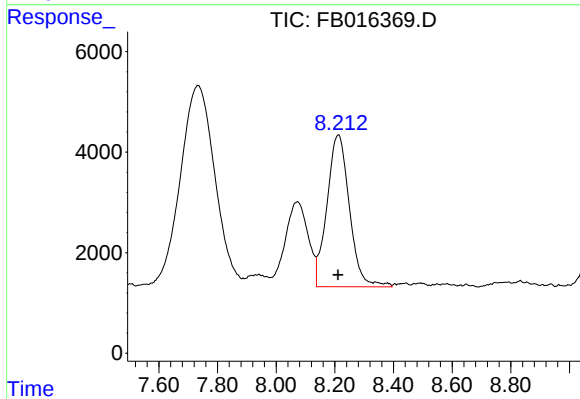

#4 Benzene


R.T.: 8.212 min
Delta R.T.: 0.000 min
Response: 160823
Conc: 10.83 ng/ml

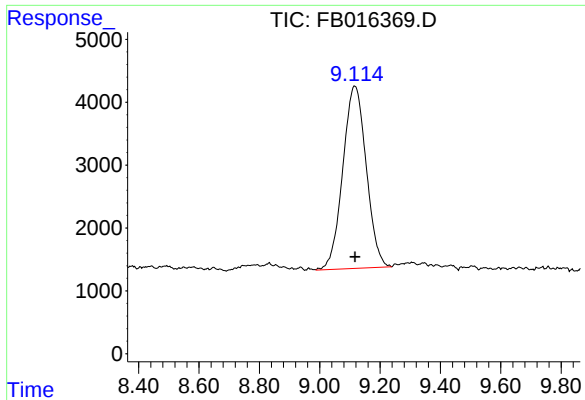

#5 AAA-TFT


R.T.: 9.117 min
Delta R.T.: 0.000 min
Response: 156329
Conc: 22.24 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-124030MS

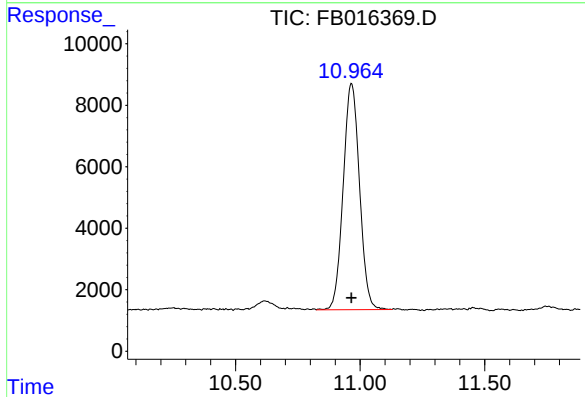


#6 Toluene

R.T.: 10.966 min
Delta R.T.: 0.000 min
Response: 334652
Conc: 26.96 ng/ml

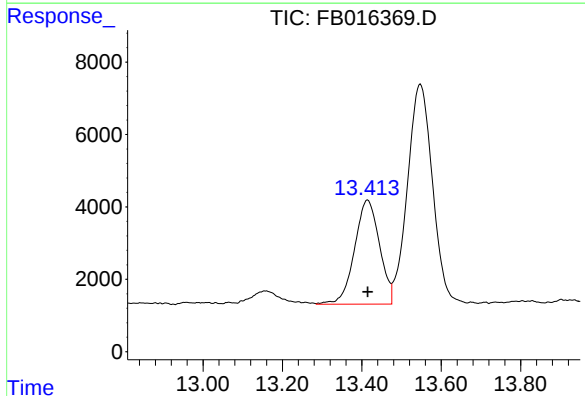


#7 Ethylbenzene

R.T.: 13.415 min
Delta R.T.: 0.000 min
Response: 125304
Conc: 8.95 ng/ml

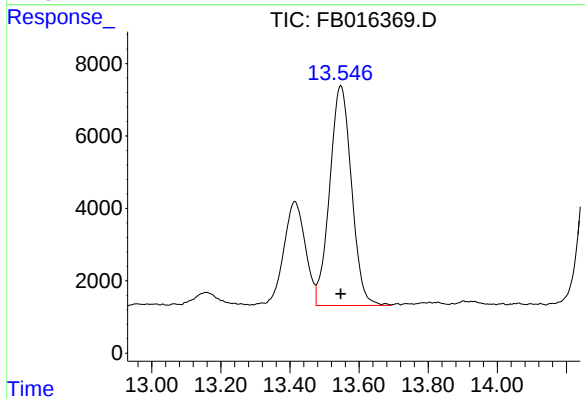

#8 m-Xylene


R.T.: 13.548 min
Delta R.T.: 0.000 min
Response: 266798
Conc: 17.53 ng/ml

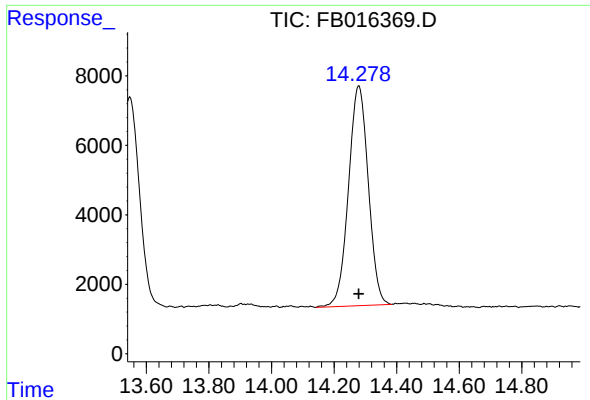

#9 O-Xylene

R.T.: 14.279 min
Delta R.T.: 0.000 min
Response: 278158
Conc: 17.82 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-124030MS

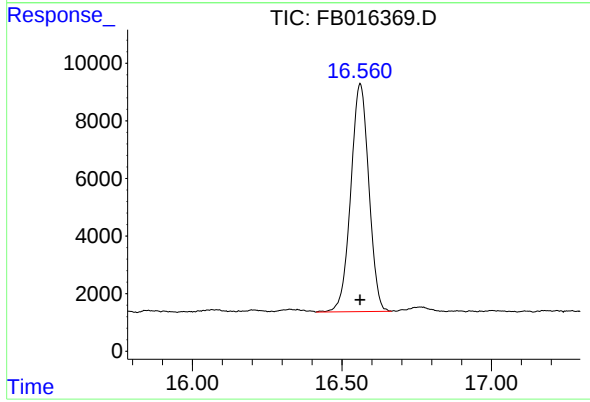

#10 1,2,4-Trimethylbenzene

R.T.: 16.562 min
Delta R.T.: 0.001 min
Response: 331646
Conc: 19.26 ng/ml