

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062518\
 Data File : FB016370.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jun 2018 18:24
 Operator : MJ/SJ
 Sample : J3706-03MSD
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 RO-124030MSD

Integration File: Calibration.e
 Quant Time: Jun 26 08:15:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Fri Jun 01 13:25:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.117	155381	22.110 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.968	318168	26.238 ng/ml
2) t 2,2,4-Trimethylpentane	7.731	331844	28.654 ng/ml
3) t n-Heptane	8.071	91006	8.315 ng/ml
4) t Benzene	8.210	156898	10.567 ng/ml
6) t Toluene	10.965	335039	26.992 ng/ml
7) t Ethylbenzene	13.414	118806	8.488 ng/ml
8) t m-Xylene	13.547	251572	16.528 ng/ml
9) t O-Xylene	14.279	271908	17.424 ng/ml
10) t 1,2,4-Trimethylbenzene	16.562	308256	17.898 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062518\
Data File : FB016370.D
Signal(s) : FID2B.CH
Acq On : 25 Jun 2018 18:24
Operator : MJ/SJ
Sample : J3706-03MSD
Misc : 5.00g/5.00mL DI Water
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RO-124030MSD

Integration File: Calibration.e
Quant Time: Jun 26 08:15:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Fri Jun 01 13:25:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

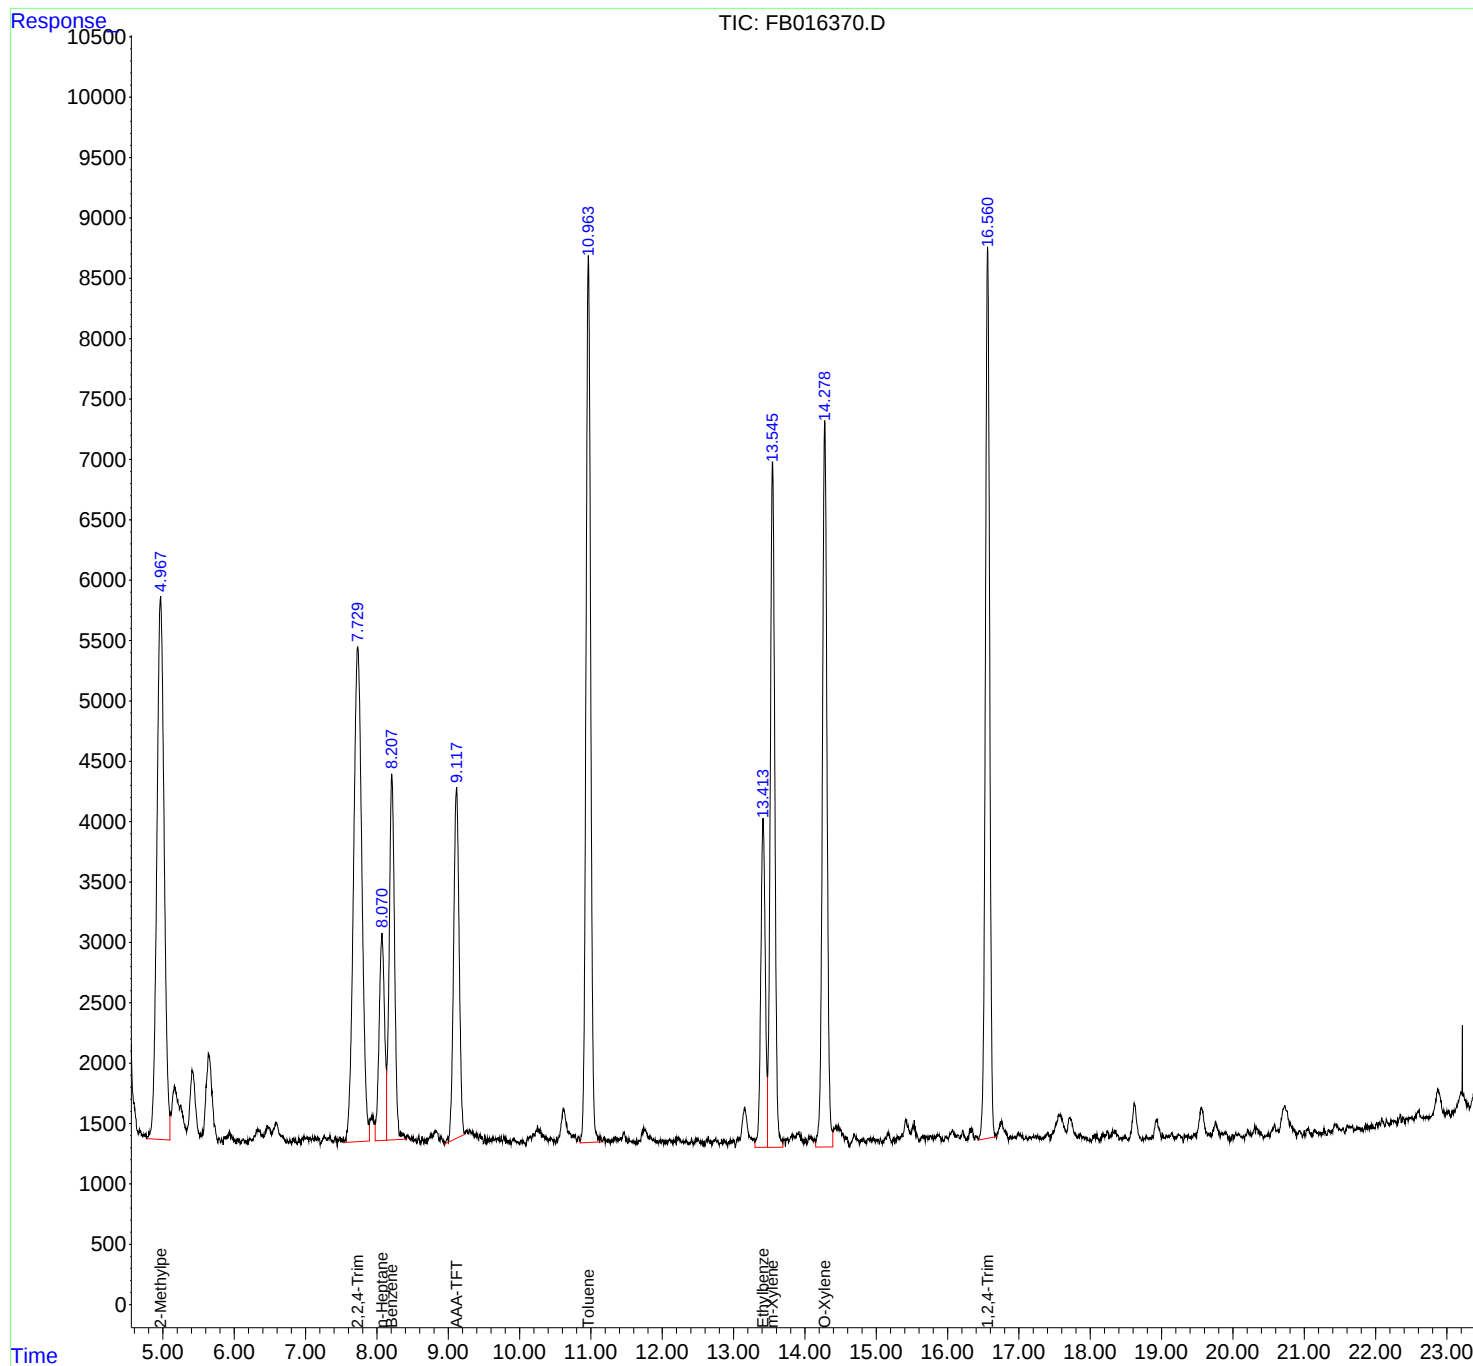


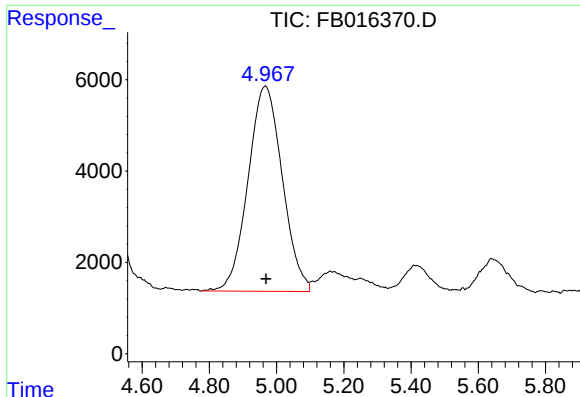

#1 2-Methylpentane


R.T.: 4.968 min
Delta R.T.: -0.001 min
Response: 318168
Conc: 26.24 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-124030MSD

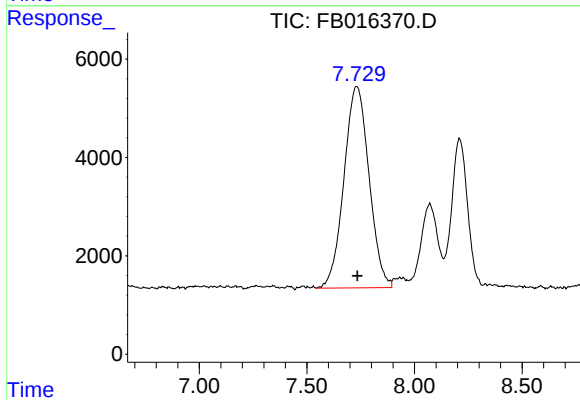


#2 2,2,4-Trimethylpentane

R.T.: 7.731 min
Delta R.T.: -0.003 min
Response: 331844
Conc: 28.65 ng/ml

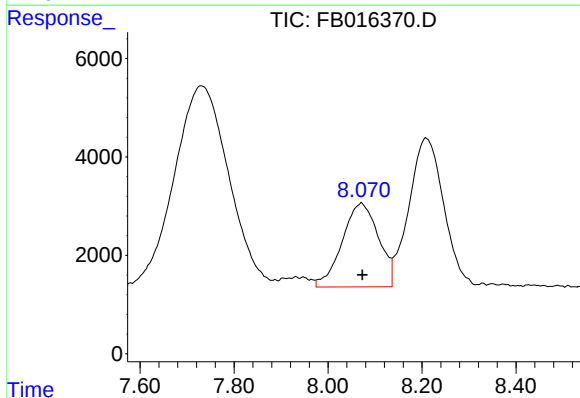


#3 n-Heptane

R.T.: 8.071 min
Delta R.T.: -0.002 min
Response: 91006
Conc: 8.32 ng/ml

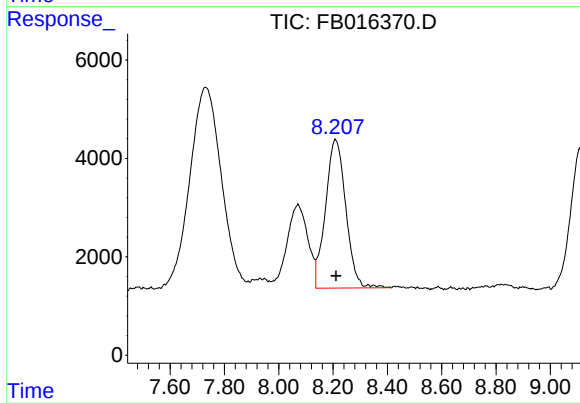

#4 Benzene


R.T.: 8.210 min
Delta R.T.: -0.002 min
Response: 156898
Conc: 10.57 ng/ml

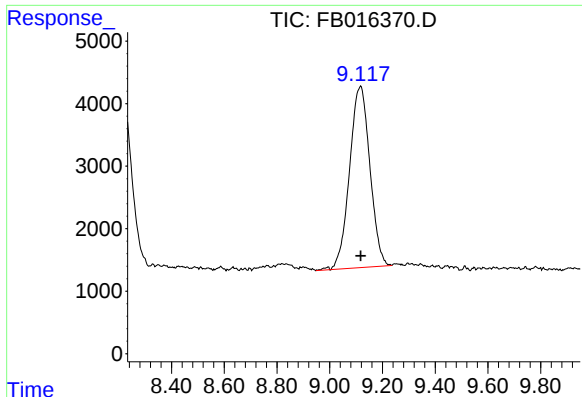

#5 AAA-TFT


R.T.: 9.117 min
Delta R.T.: 0.000 min
Response: 155381
Conc: 22.11 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-124030MSD

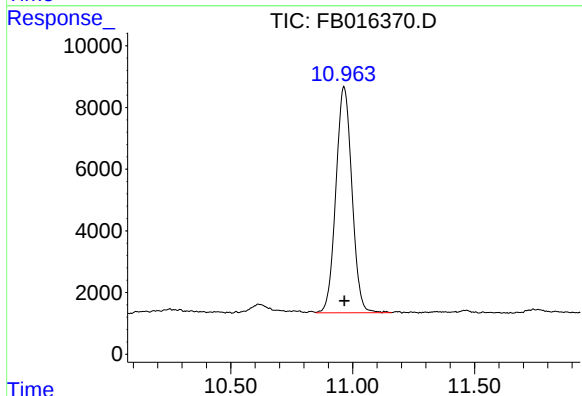


#6 Toluene

R.T.: 10.965 min
Delta R.T.: 0.000 min
Response: 335039
Conc: 26.99 ng/ml

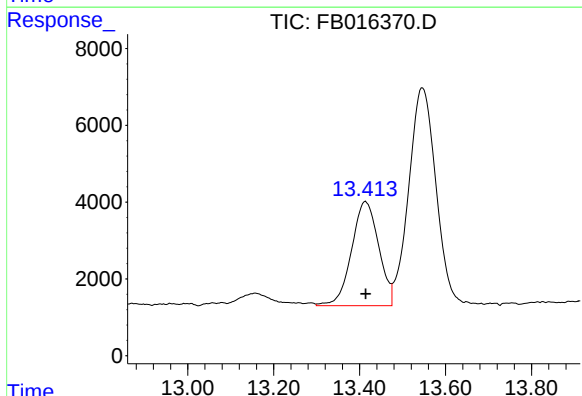


#7 Ethylbenzene

R.T.: 13.414 min
Delta R.T.: 0.000 min
Response: 118806
Conc: 8.49 ng/ml

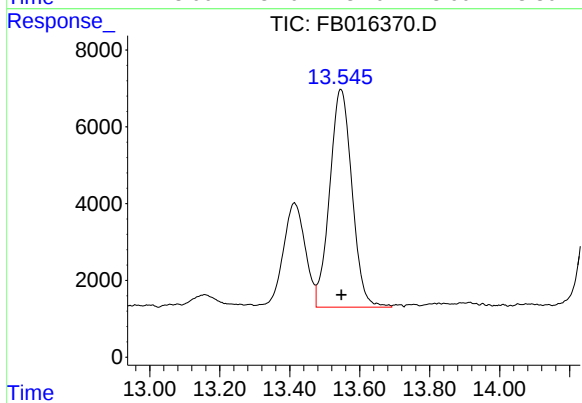

#8 m-Xylene


R.T.: 13.547 min
Delta R.T.: 0.000 min
Response: 251572
Conc: 16.53 ng/ml

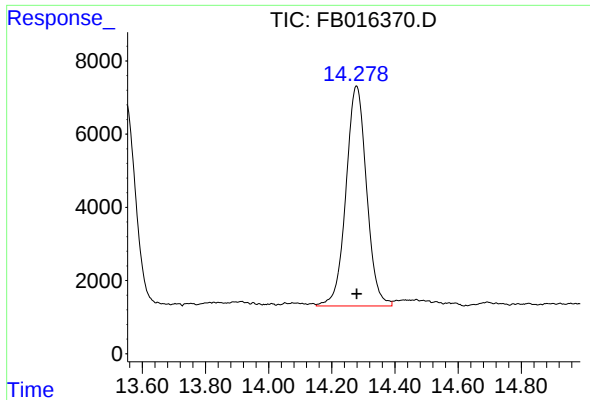

#9 O-Xylene

R.T.: 14.279 min
Delta R.T.: 0.000 min
Response: 271908
Conc: 17.42 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-124030MSD

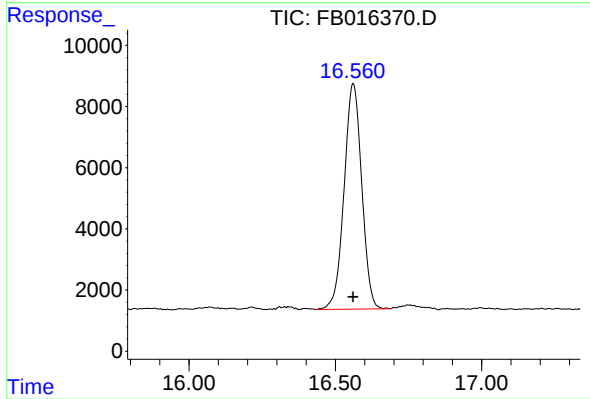

#10 1,2,4-Trimethylbenzene

R.T.: 16.562 min
Delta R.T.: 0.001 min
Response: 308256
Conc: 17.90 ng/ml