

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070318\
 Data File : FB016541.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jul 2018 10:00
 Operator : MJ/SJ
 Sample : BSF0703S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 03 15:16:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070218.M
 Quant Title :
 QLast Update : Mon Jul 02 14:53:33 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.116	158383	19.183 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.968	431696	30.473 ng/ml
2) t 2,2,4-Trimethylpentane	7.732	418957	30.426 ng/ml
3) t n-Heptane	8.070	132366	9.785 ng/ml
4) t Benzene	8.210	169730	9.076 ng/ml
6) t Toluene	10.966	404427	30.171 ng/ml
7) t Ethylbenzene	13.415	149598	10.245 ng/ml
8) t m-Xylene	13.547	323198	20.349 ng/ml
9) t O-Xylene	14.279	340047	19.916 ng/ml
10) t 1,2,4-Trimethylbenzene	16.561	379731	19.919 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070318\
Data File : FB016541.D
Signal(s) : FID2B.CH
Acq On : 3 Jul 2018 10:00
Operator : MJ/SJ
Sample : BSF0703S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 03 15:16:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070218.M
Quant Title :
QLast Update : Mon Jul 02 14:53:33 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

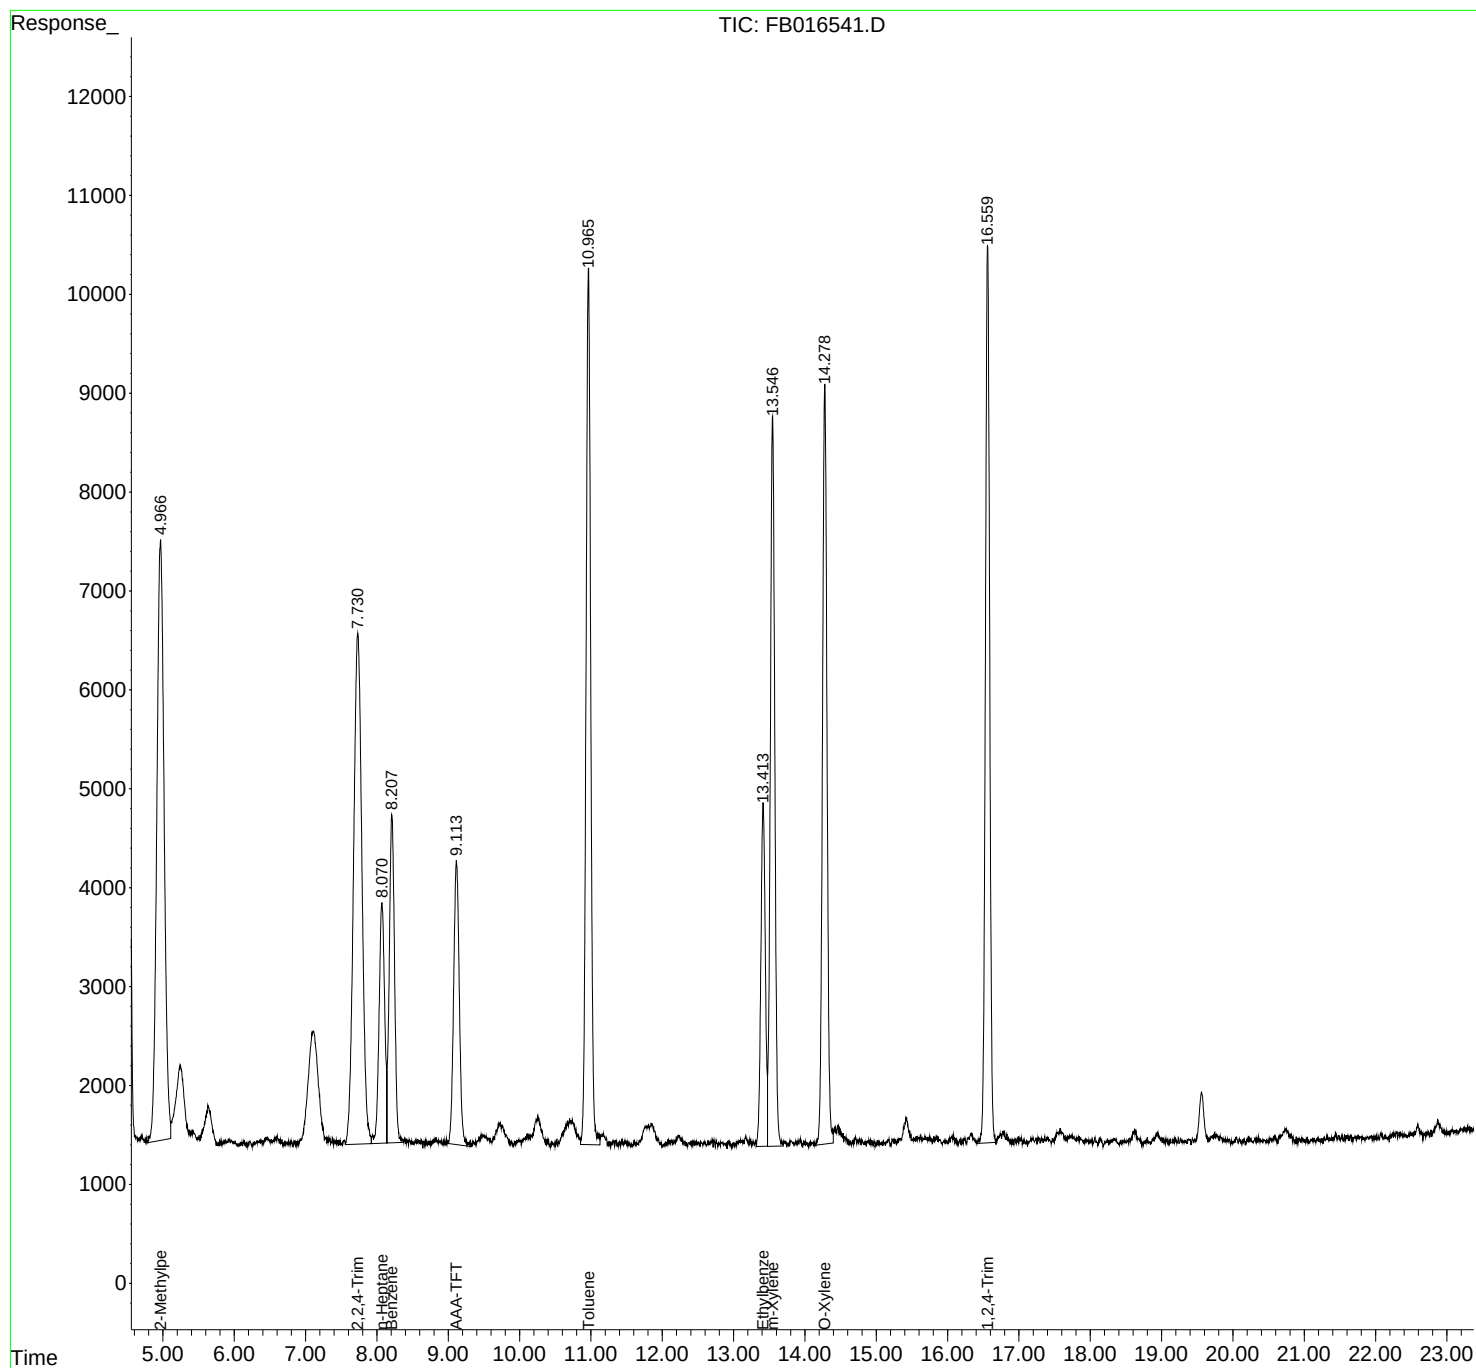

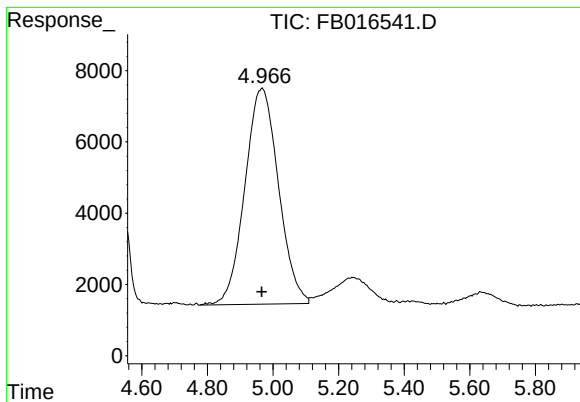


#1 2-Methylpentane

R.T.: 4.968 min
 Delta R.T.: 0.002 min
 Response: 431696
 Conc: 30.47 ng/ml

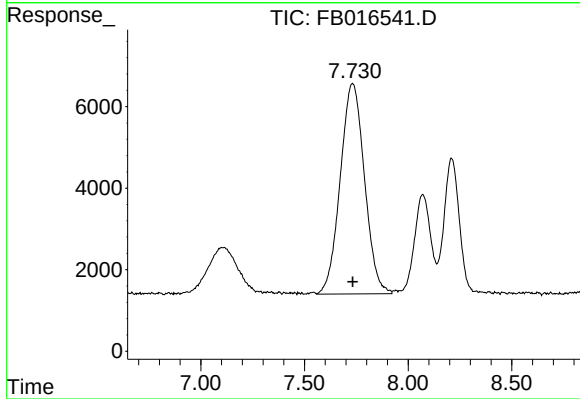


#2 2,2,4-Trimethylpentane

R.T.: 7.732 min
 Delta R.T.: 0.000 min
 Response: 418957
 Conc: 30.43 ng/ml

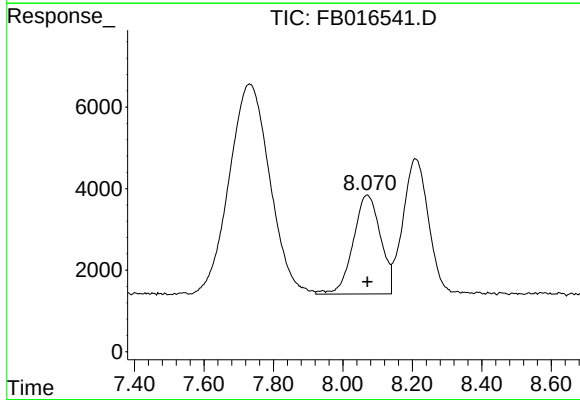


#3 n-Heptane

R.T.: 8.070 min
 Delta R.T.: 0.000 min
 Response: 132366
 Conc: 9.79 ng/ml

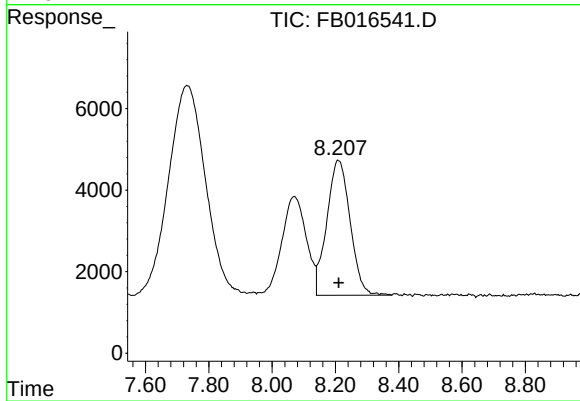


#4 Benzene

R.T.: 8.210 min
 Delta R.T.: 0.000 min
 Response: 169730
 Conc: 9.08 ng/ml

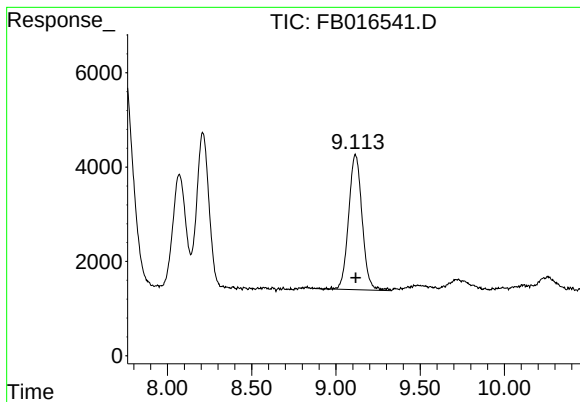


#5 AAA-TFT

R.T.: 9.116 min
Delta R.T.: -0.001 min
Response: 158383
Conc: 19.18 ng/ml

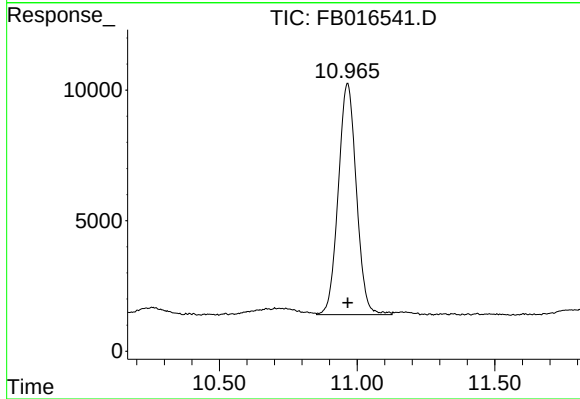


#6 Toluene

R.T.: 10.966 min
Delta R.T.: 0.000 min
Response: 404427
Conc: 30.17 ng/ml

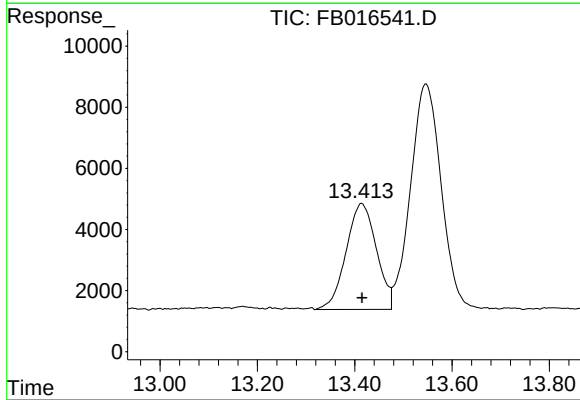


#7 Ethylbenzene

R.T.: 13.415 min
Delta R.T.: 0.000 min
Response: 149598
Conc: 10.25 ng/ml

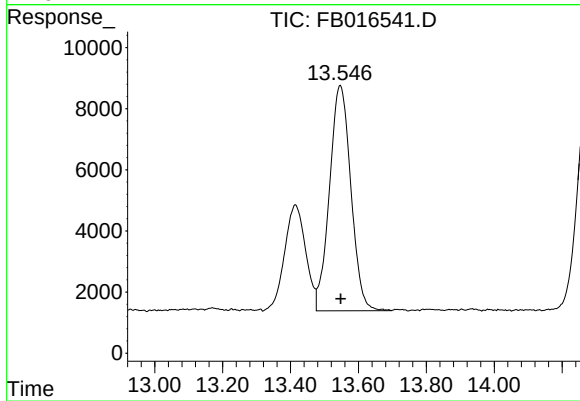


#8 m-Xylene

R.T.: 13.547 min
Delta R.T.: 0.000 min
Response: 323198
Conc: 20.35 ng/ml

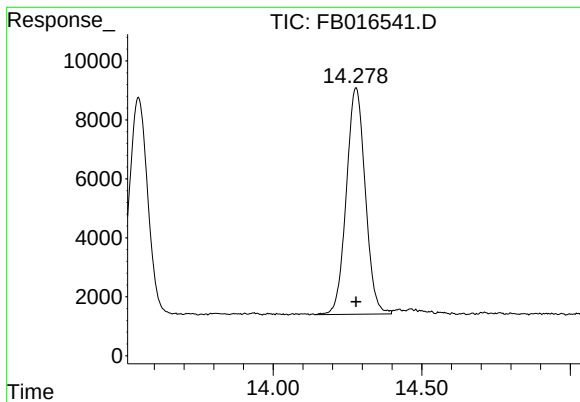

#9 O-Xylene

R.T.: 14.279 min
Delta R.T.: 0.000 min
Response: 340047
Conc: 19.92 ng/ml

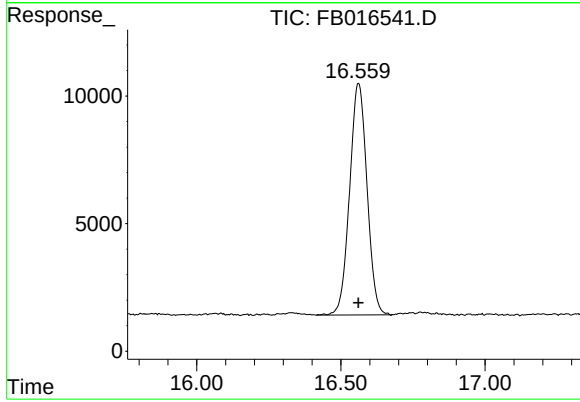

#10 1,2,4-Trimethylbenzene

R.T.: 16.561 min
Delta R.T.: 0.000 min
Response: 379731
Conc: 19.92 ng/ml