

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070919\
 Data File : FB021650.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jul 2019 11:40
 Operator : MJ/SJ
 Sample : BSF0709S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 10 01:01:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.990	269495	19.491 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.860	936398	27.430 ng/ml
2) t	2,2,4-Trimethylpentane	7.609	907654	29.371 ng/ml
3) t	n-Heptane	7.947	282963	9.668 ng/ml
4) t	Benzene	8.083	324315	9.662 ng/ml
6) t	Toluene	10.830	678234	29.692 ng/ml
7) t	Ethylbenzene	13.276	237280	10.023 ng/ml
8) t	m-Xylene	13.408	509892	20.117 ng/ml
9) t	O-Xylene	14.138	529404	20.186 ng/ml
10) t	1,2,4-Trimethylbenzene	16.417	540962	20.589 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070919\
Data File : FB021650.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2019 11:40
Operator : MJ/SJ
Sample : BSF0709S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 10 01:01:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

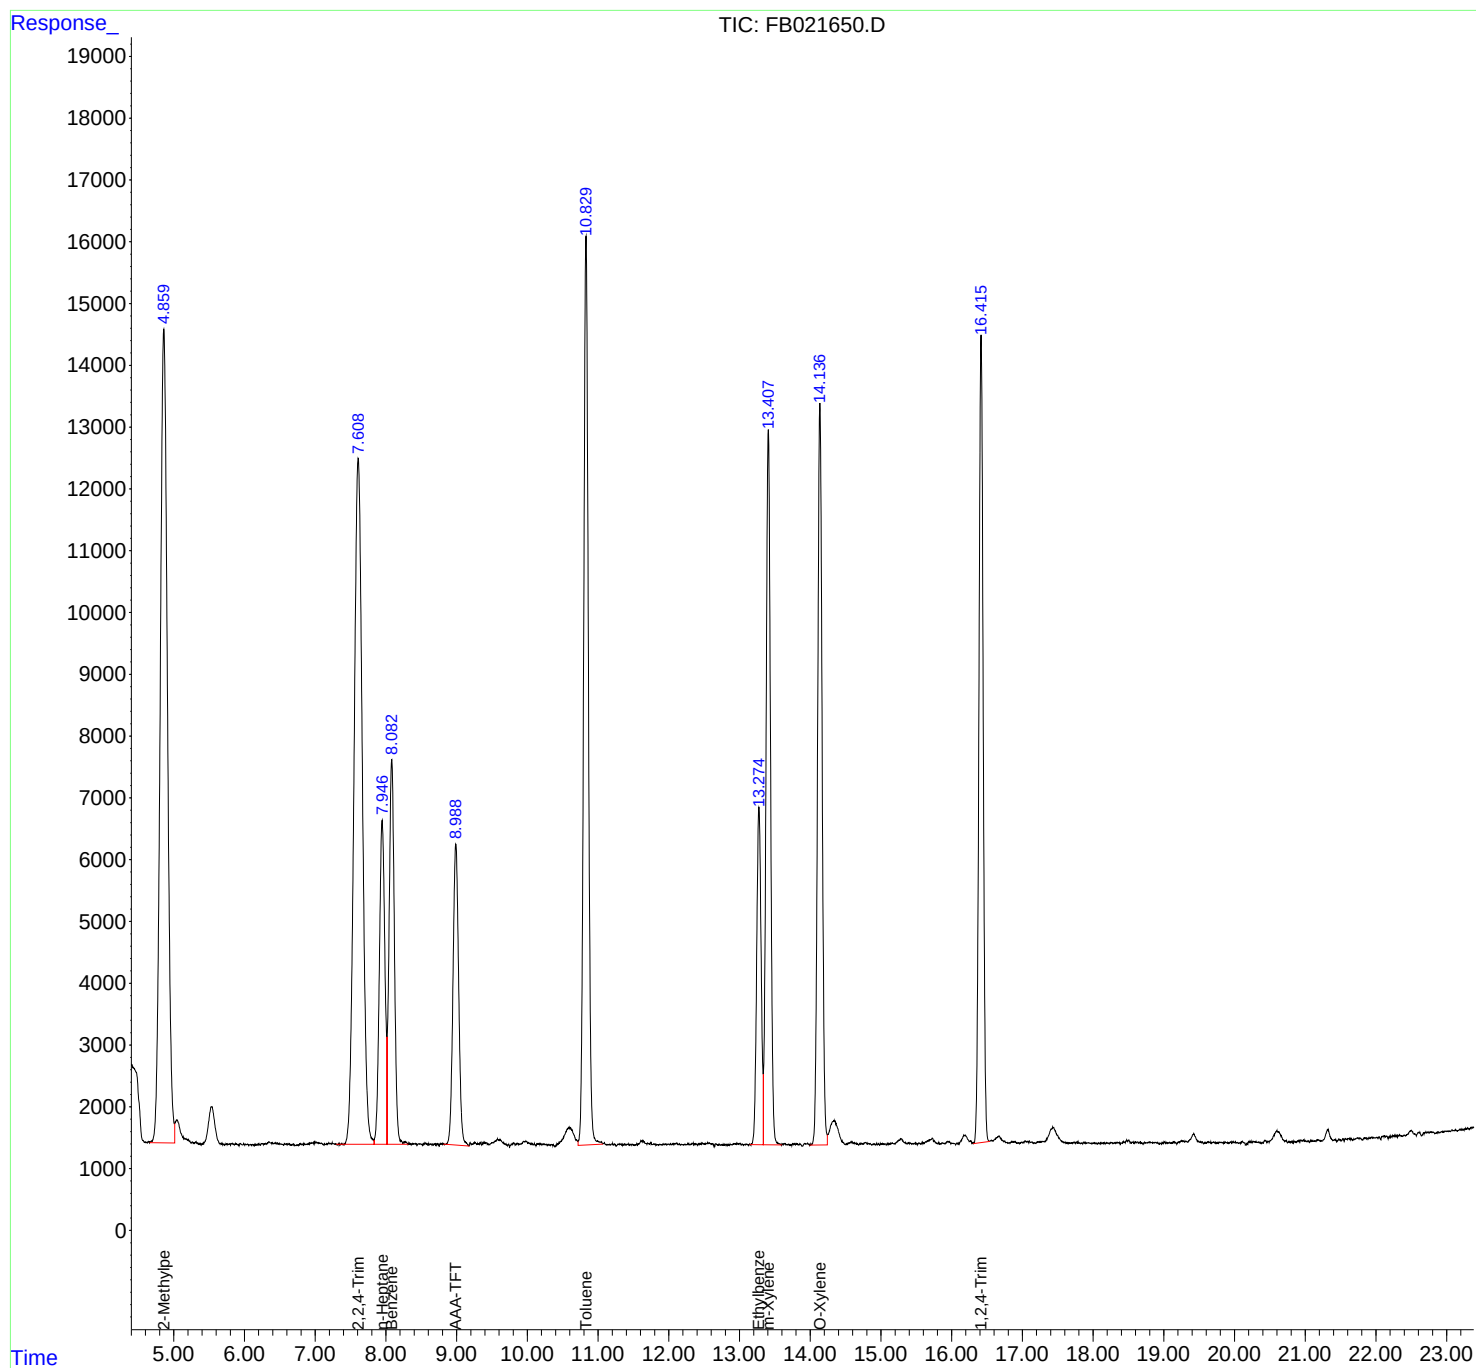

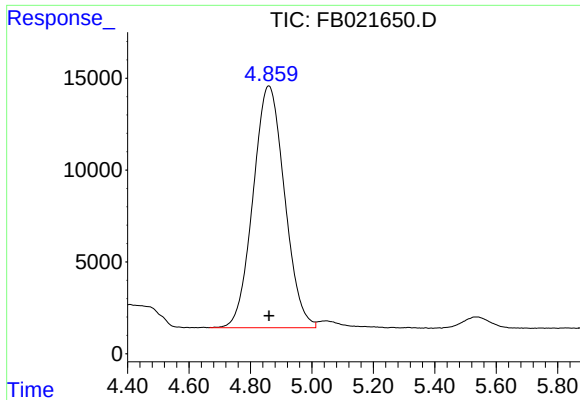


#1 2-Methylpentane

R.T.: 4.860 min
Delta R.T.: 0.000 min
Response: 936398
Conc: 27.43 ng/ml

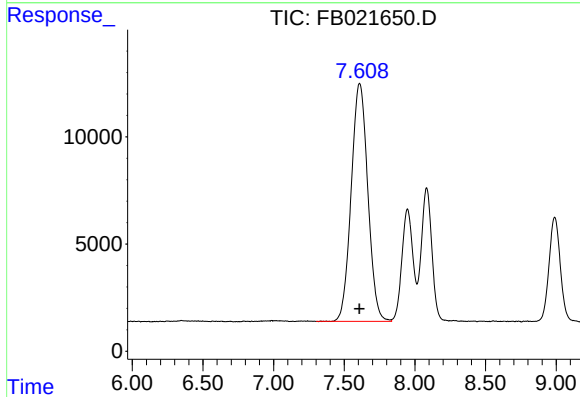


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: 0.001 min
Response: 907654
Conc: 29.37 ng/ml

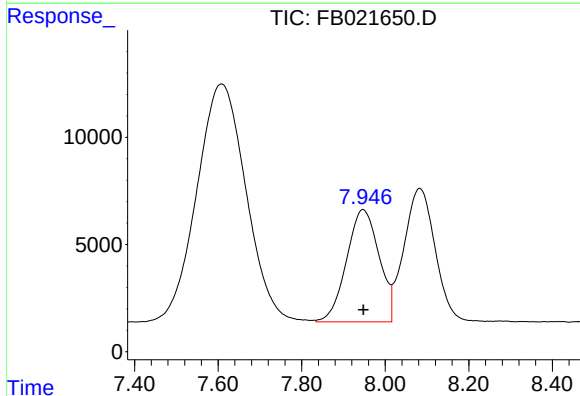


#3 n-Heptane

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 282963
Conc: 9.67 ng/ml

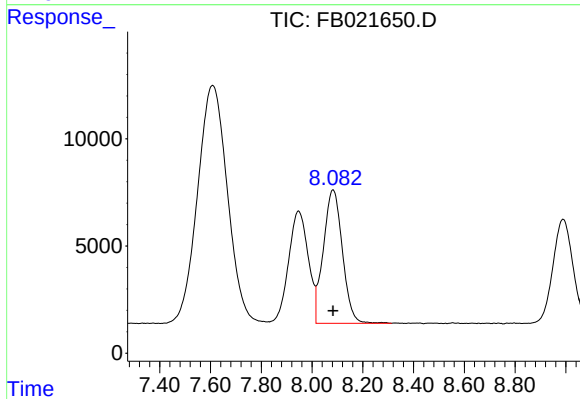


#4 Benzene

R.T.: 8.083 min
Delta R.T.: 0.001 min
Response: 324315
Conc: 9.66 ng/ml

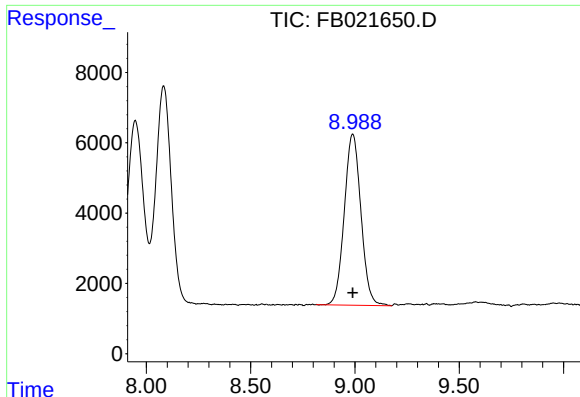


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 269495
Conc: 19.49 ng/ml

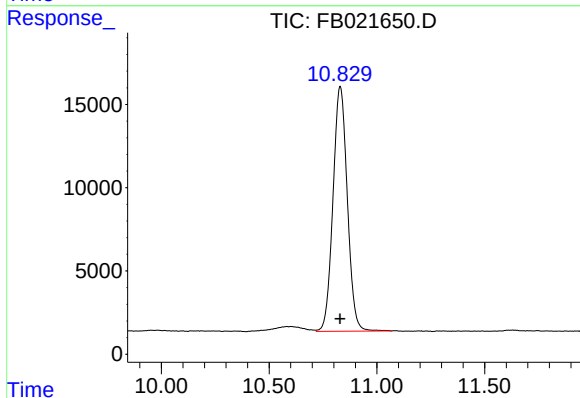


#6 Toluene

R.T.: 10.830 min
Delta R.T.: 0.000 min
Response: 678234
Conc: 29.69 ng/ml

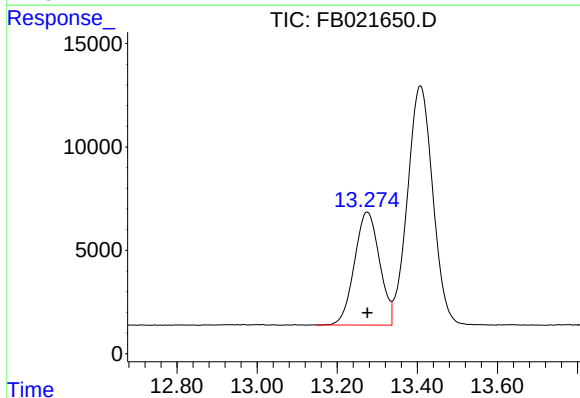


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: 0.000 min
Response: 237280
Conc: 10.02 ng/ml

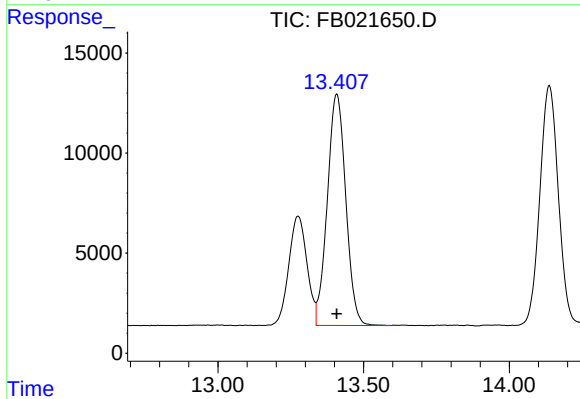


#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: 0.000 min
Response: 509892
Conc: 20.12 ng/ml

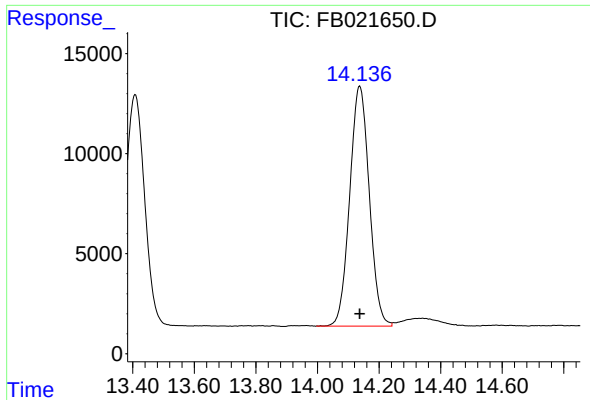

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: 0.000 min
Response: 529404
Conc: 20.19 ng/ml

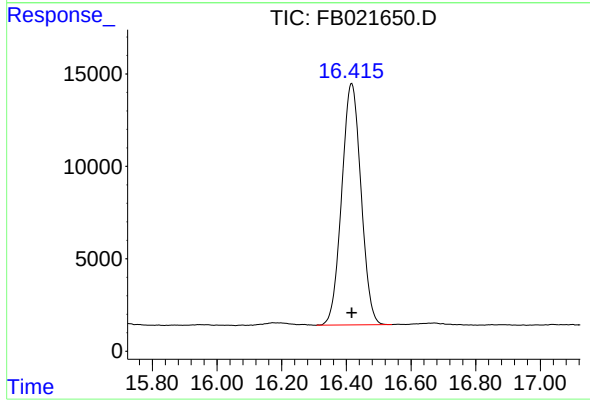

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: 0.000 min
Response: 540962
Conc: 20.59 ng/ml