

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070919\
 Data File : FB021654.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jul 2019 13:42
 Operator : MJ/SJ
 Sample : K3697-02MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 10 01:02:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	288181	20.843 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.860	776064	22.734 ng/ml
2) t 2,2,4-Trimethylpentane	7.608	654129	21.167 ng/ml
3) t n-Heptane	7.948	202875	6.932 ng/ml
4) t Benzene	8.082	305071	9.089 ng/ml
6) t Toluene	10.830	632519	27.690 ng/ml
7) t Ethylbenzene	13.276	209955	8.869 ng/ml
8) t m-Xylene	13.408	447601	17.660 ng/ml
9) t O-Xylene	14.137	468894	17.878 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	447946	17.049 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070919\
Data File : FB021654.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2019 13:42
Operator : MJ/SJ
Sample : K3697-02MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 10 01:02:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

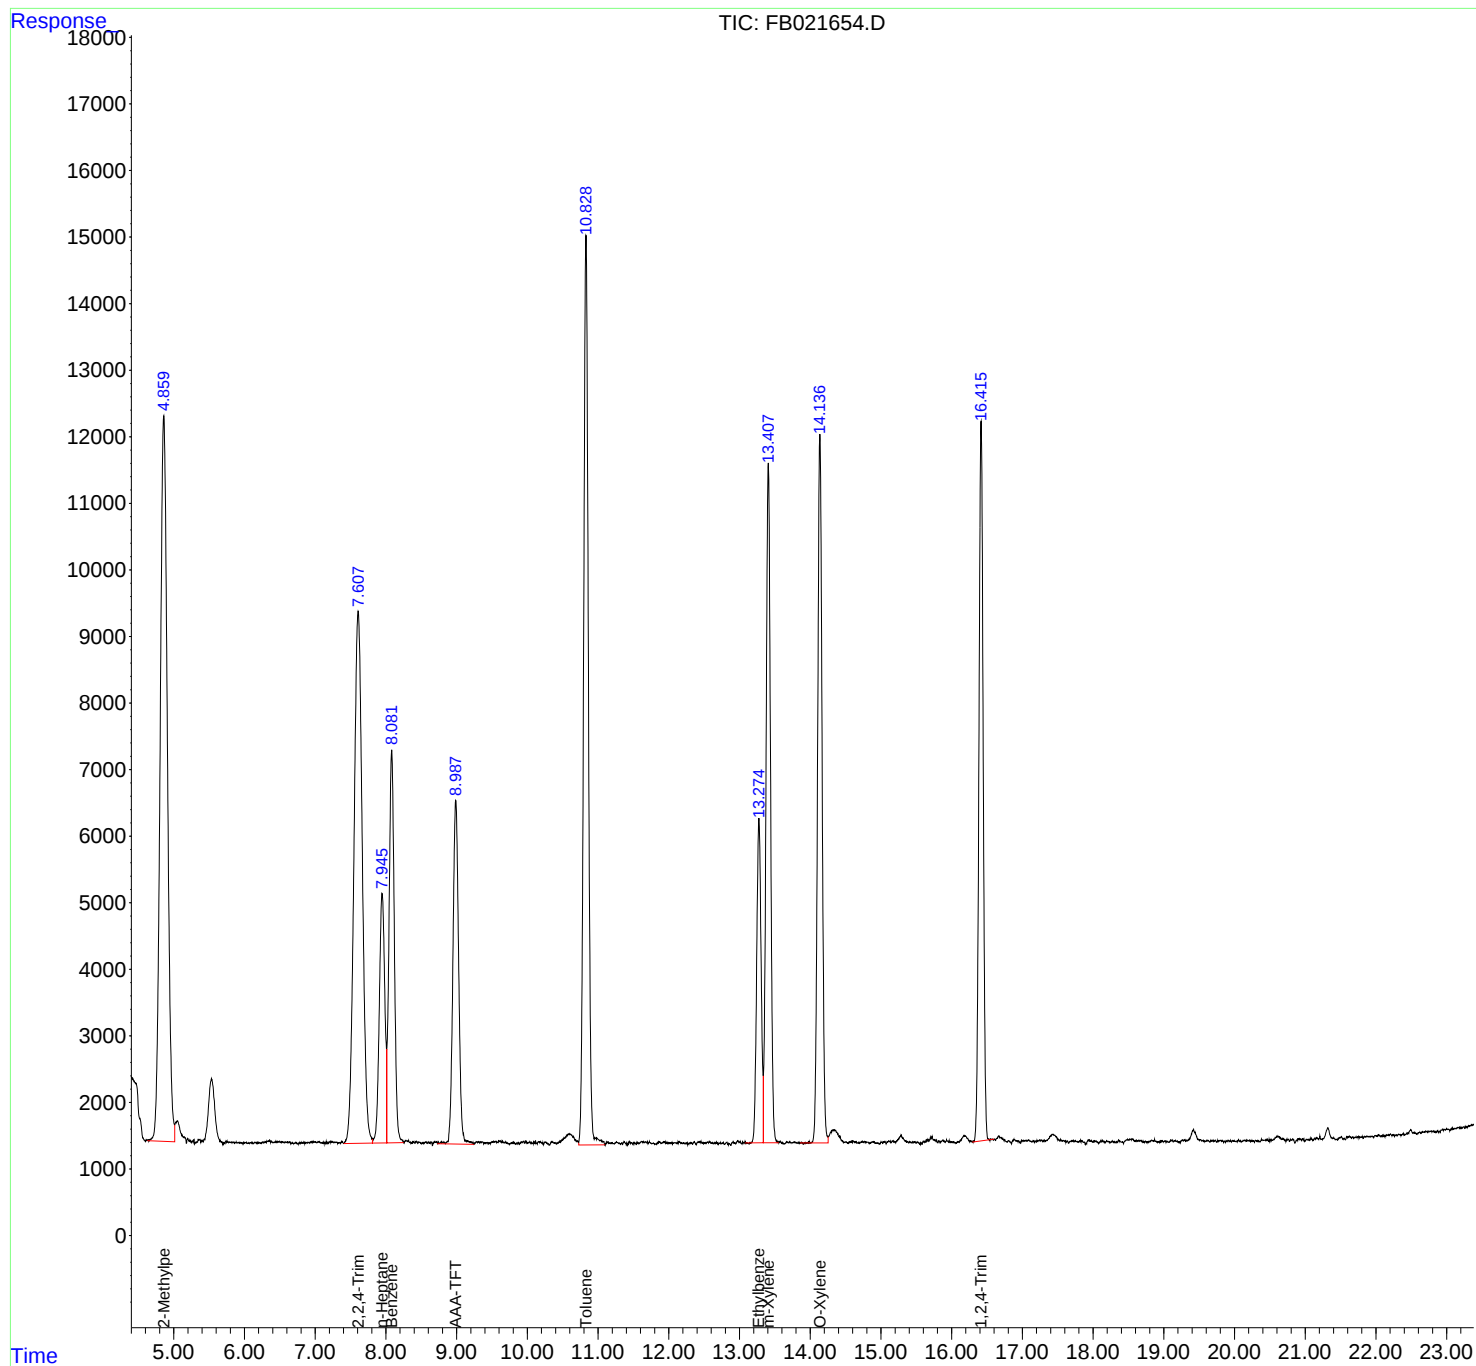

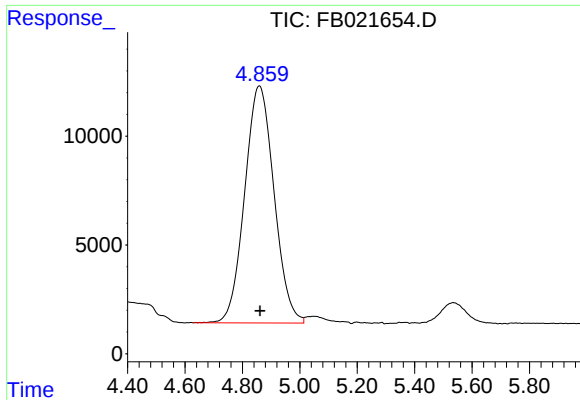


#1 2-Methylpentane

R.T.: 4.860 min
Delta R.T.: -0.001 min
Response: 776064
Conc: 22.73 ng/ml

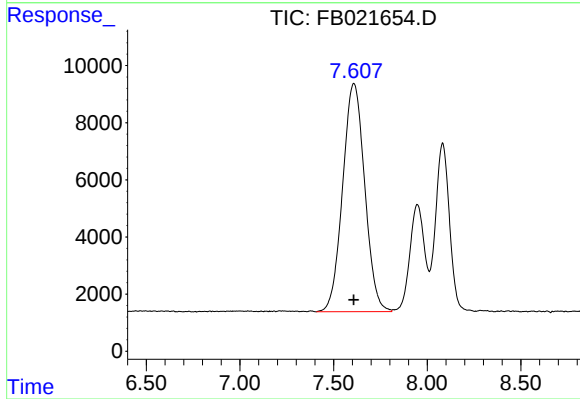


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 654129
Conc: 21.17 ng/ml

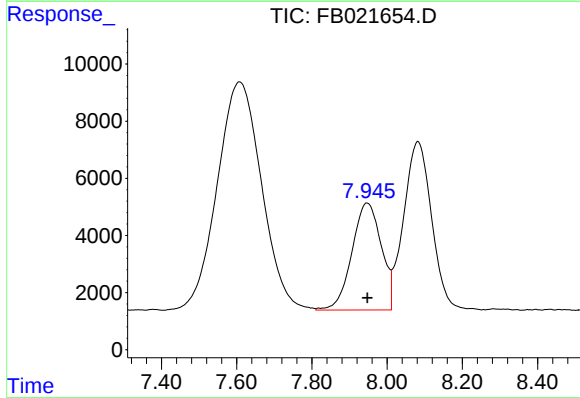


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: 0.000 min
Response: 202875
Conc: 6.93 ng/ml

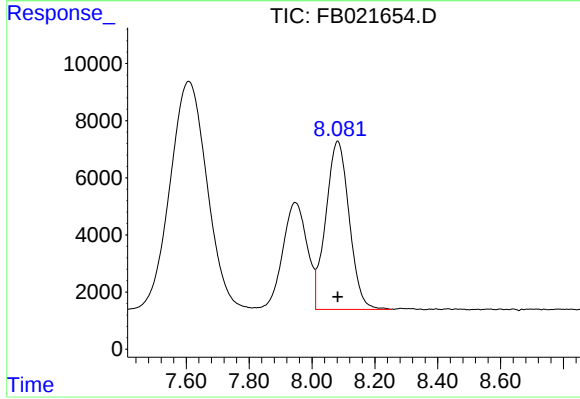


#4 Benzene

R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 305071
Conc: 9.09 ng/ml

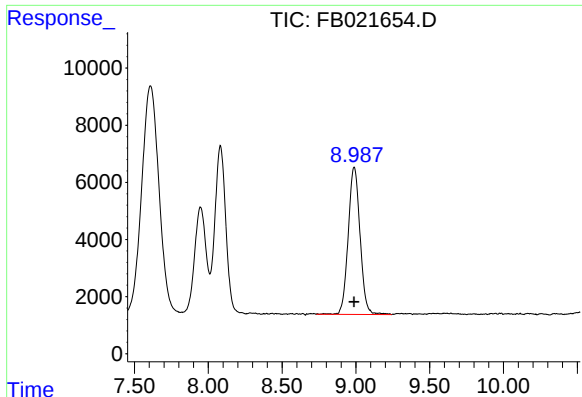


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 288181
Conc: 20.84 ng/ml

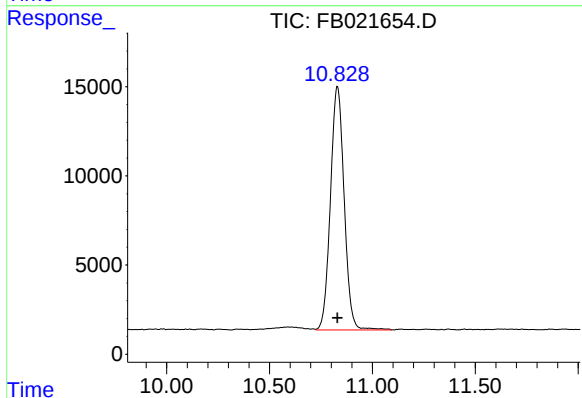


#6 Toluene

R.T.: 10.830 min
Delta R.T.: 0.000 min
Response: 632519
Conc: 27.69 ng/ml

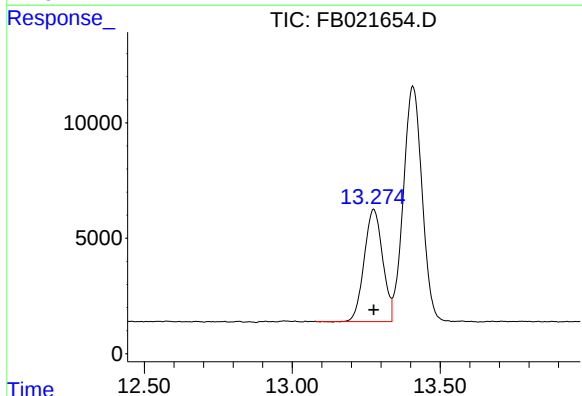


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: 0.000 min
Response: 209955
Conc: 8.87 ng/ml

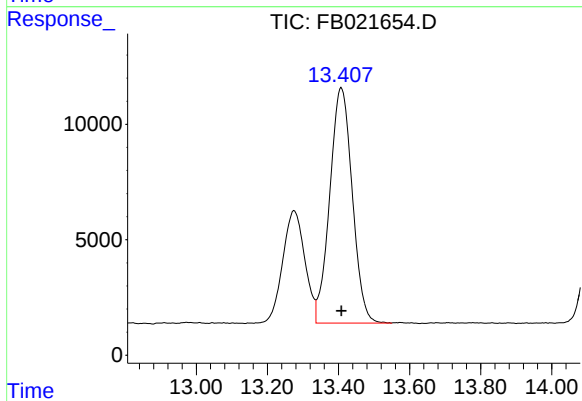


#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: 0.000 min
Response: 447601
Conc: 17.66 ng/ml

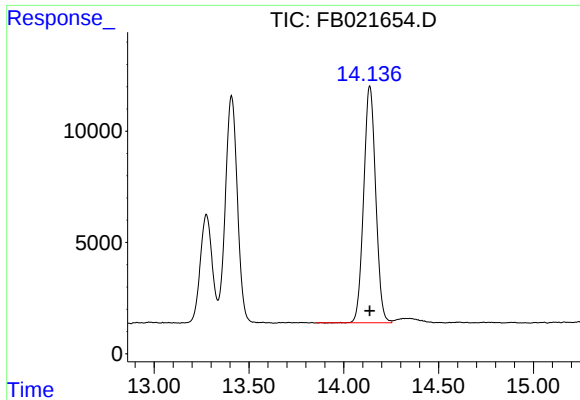

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: 0.000 min
Response: 468894
Conc: 17.88 ng/ml

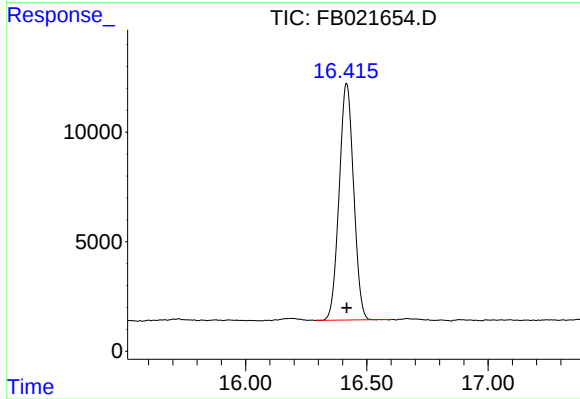

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: 0.000 min
Response: 447946
Conc: 17.05 ng/ml