

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070919\
 Data File : FB021653.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jul 2019 13:12
 Operator : MJ/SJ
 Sample : K3697-02MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 10 01:02:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.990	280373	20.278 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.862	851187	24.934 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	770098	24.920 ng/ml
3) t n-Heptane	7.949	237745	8.123 ng/ml
4) t Benzene	8.084	308825	9.201 ng/ml
6) t Toluene	10.830	650636	28.484 ng/ml
7) t Ethylbenzene	13.276	219118	9.256 ng/ml
8) t m-Xylene	13.408	469323	18.517 ng/ml
9) t O-Xylene	14.137	488582	18.629 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	482352	18.359 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070919\
Data File : FB021653.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2019 13:12
Operator : MJ/SJ
Sample : K3697-02MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 10 01:02:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

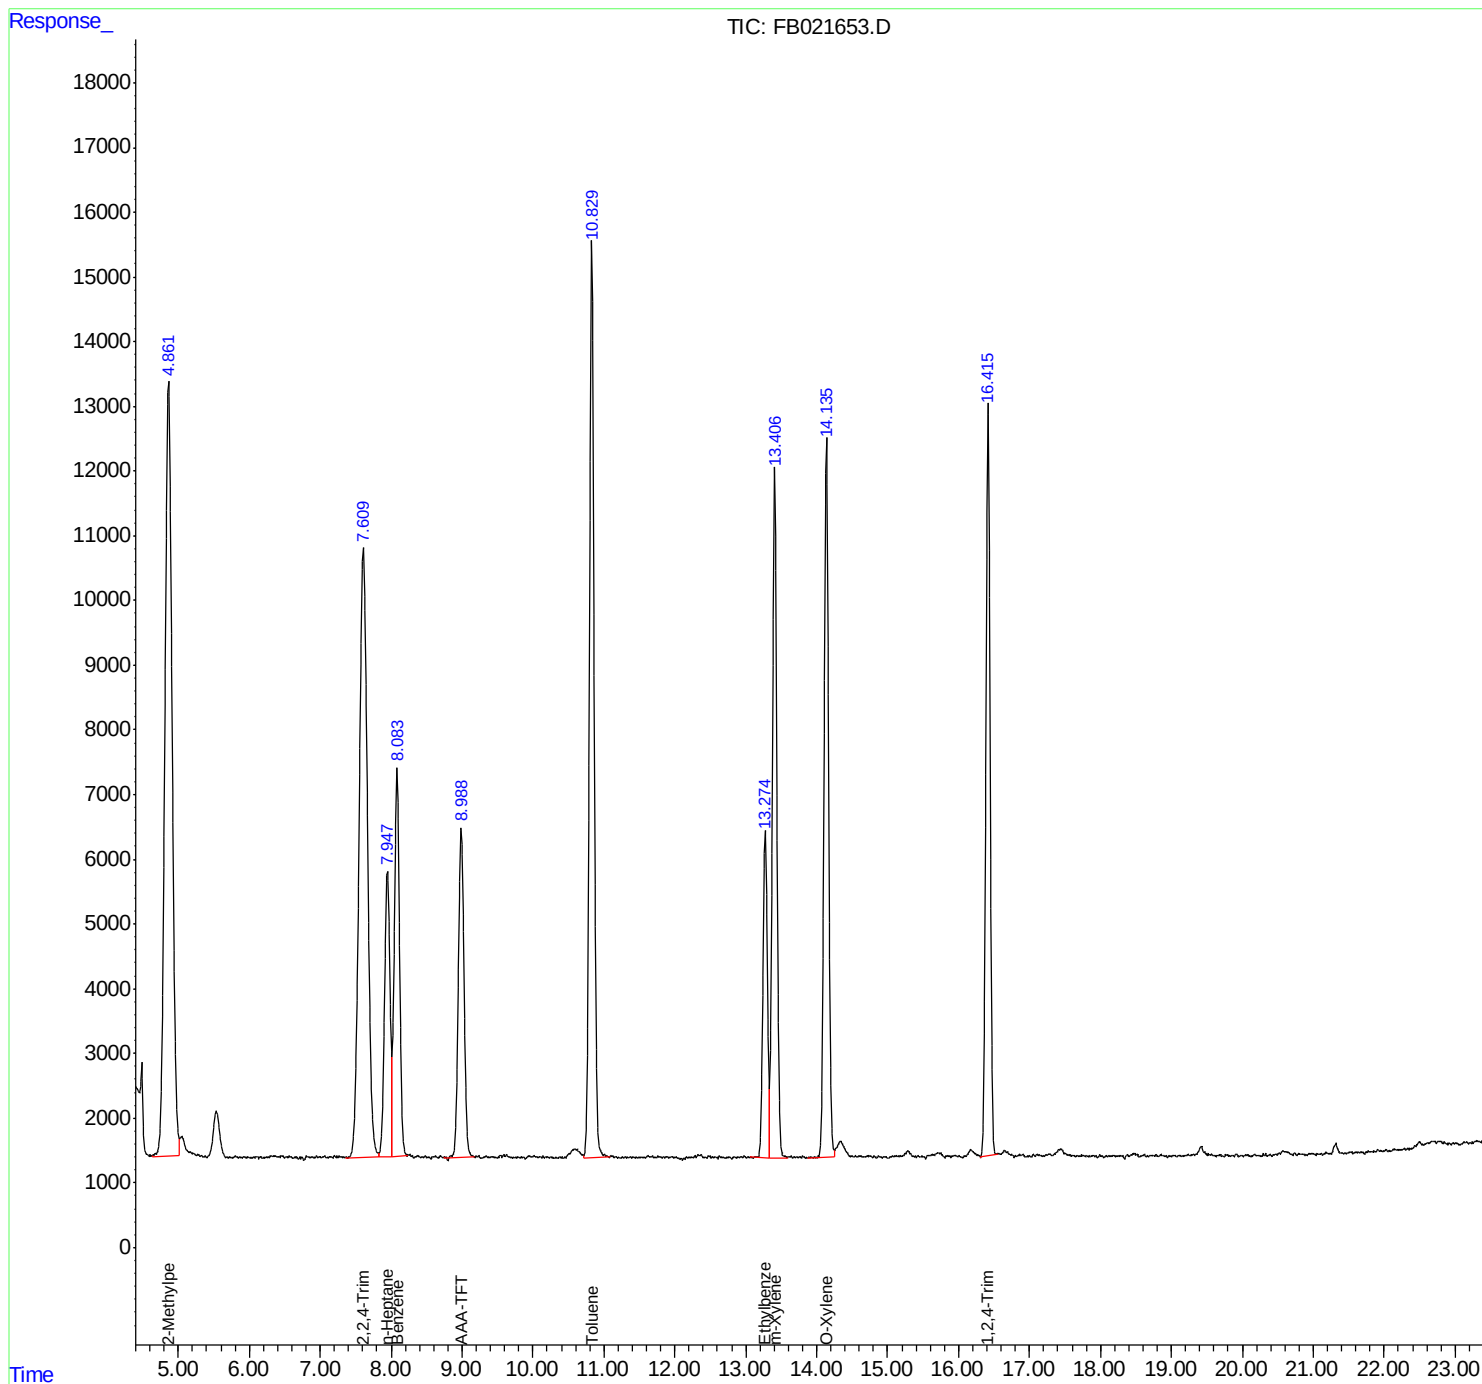

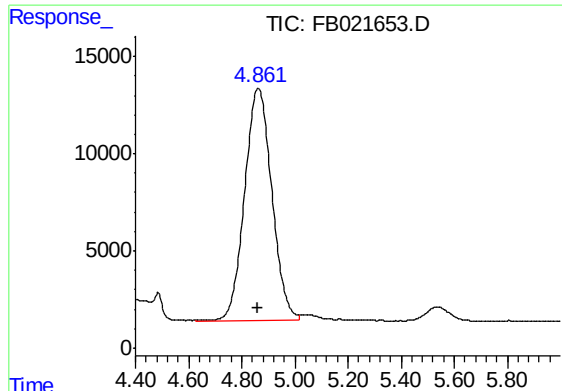


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: 0.001 min
Response: 851187
Conc: 24.93 ng/ml

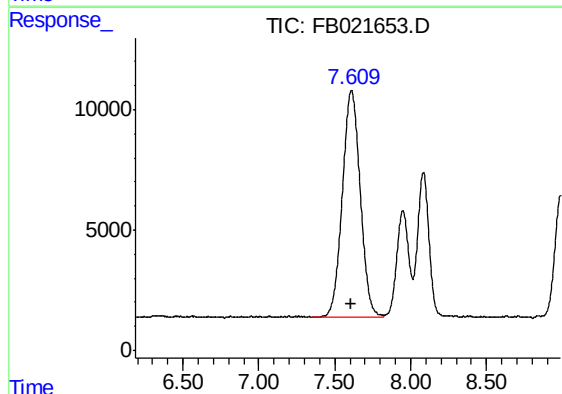


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: 0.002 min
Response: 770098
Conc: 24.92 ng/ml

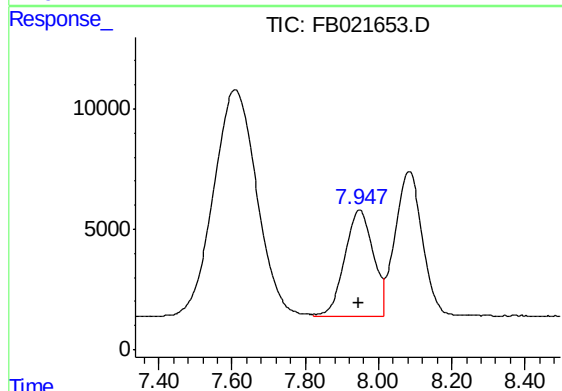


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 237745
Conc: 8.12 ng/ml

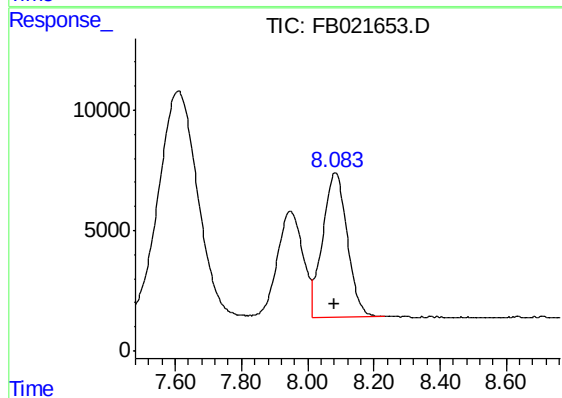


#4 Benzene

R.T.: 8.084 min
Delta R.T.: 0.002 min
Response: 308825
Conc: 9.20 ng/ml

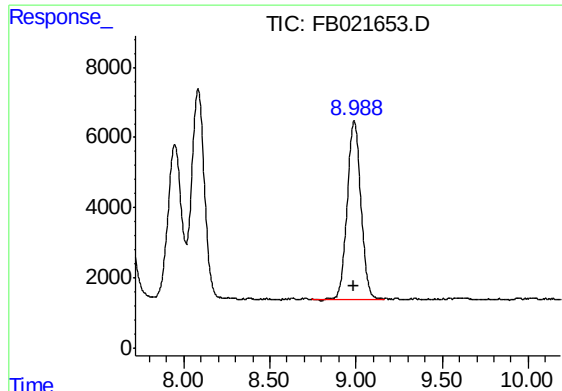


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 280373
Conc: 20.28 ng/ml

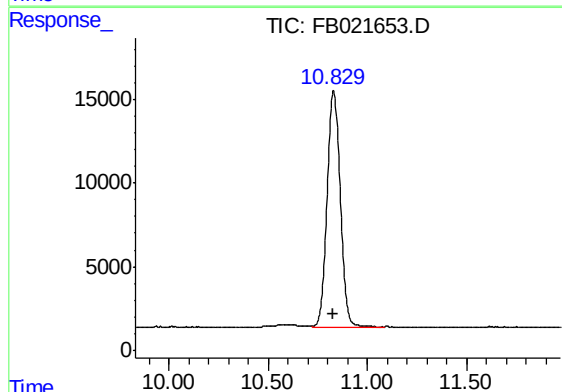


#6 Toluene

R.T.: 10.830 min
Delta R.T.: 0.000 min
Response: 650636
Conc: 28.48 ng/ml

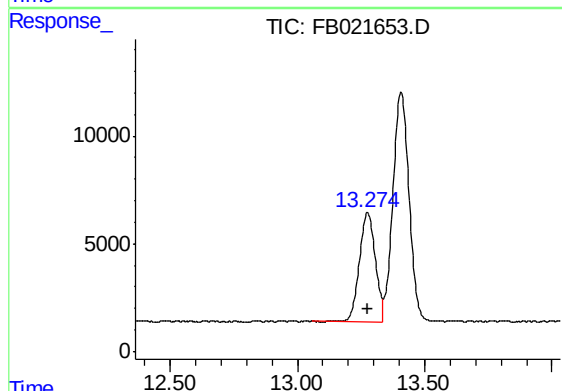


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: 0.000 min
Response: 219118
Conc: 9.26 ng/ml

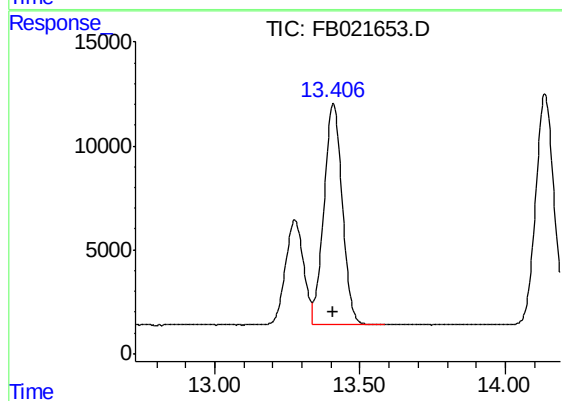


#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: 0.000 min
Response: 469323
Conc: 18.52 ng/ml

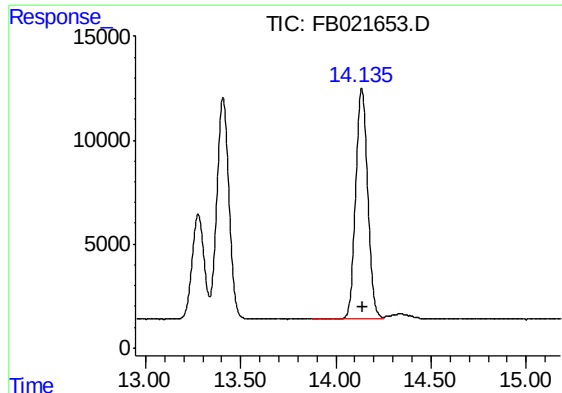

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: 0.000 min
Response: 488582
Conc: 18.63 ng/ml

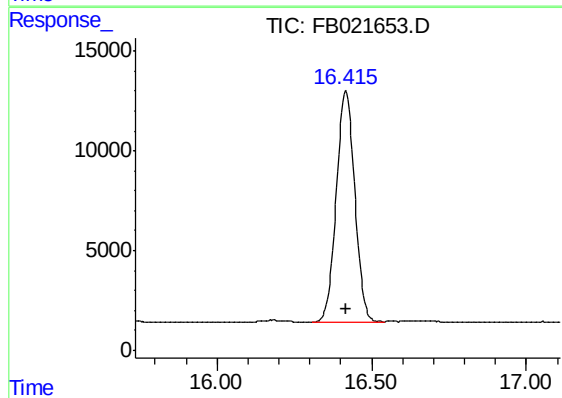

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: 0.000 min
Response: 482352
Conc: 18.36 ng/ml