

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071618\
 Data File : FB016777.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jul 2018 1:41
 Operator : MJ/SJ
 Sample : J3832-03
 Misc : 5.00g/5.00ml DI water
 ALS Vial : 30 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Jul 17 09:03:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
 Quant Title :
 QLast Update : Mon Jul 09 13:06:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.115	145762	16.719 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.956	2428	0.167 ng/ml
2) t	2,2,4-Trimethylpentane	7.719	618	0.044 ng/ml
3) t	n-Heptane	8.056	189	0.014 ng/ml
4) t	Benzene	8.200	1561	0.084 ng/ml
6) t	Toluene	10.961	3132	0.214 ng/ml
7) t	Ethylbenzene	13.412	893	0.061 ng/ml
8) t	m-Xylene	13.546	1747	0.112 ng/ml
9) t	O-Xylene	14.255	410	0.025 ng/ml
10) t	1,2,4-Trimethylbenzene	16.581	809	0.041 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071618\
Data File : FB016777.D
Signal(s) : FID2B.CH
Acq On : 17 Jul 2018 1:41
Operator : MJ/SJ
Sample : J3832-03
Misc : 5.00g/5.00ml DI water
ALS Vial : 30 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Jul 17 09:03:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
Quant Title :
QLast Update : Mon Jul 09 13:06:15 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

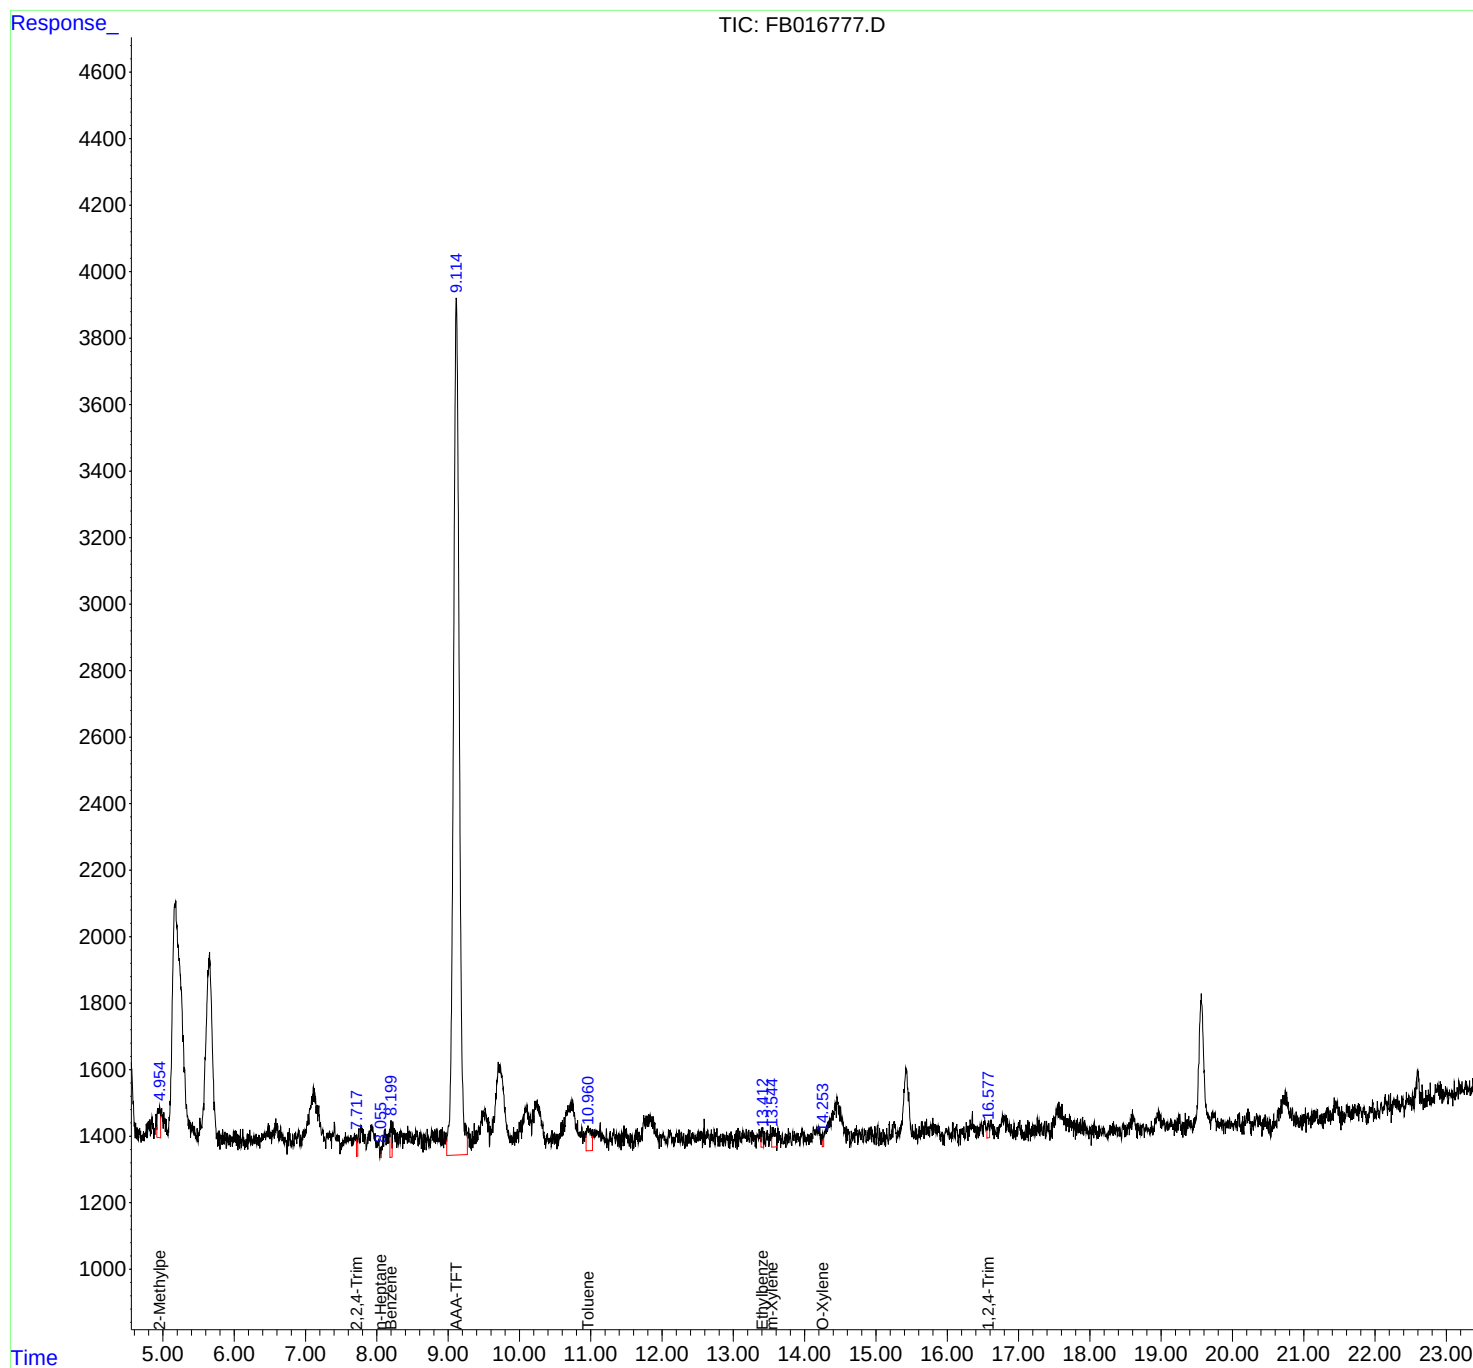

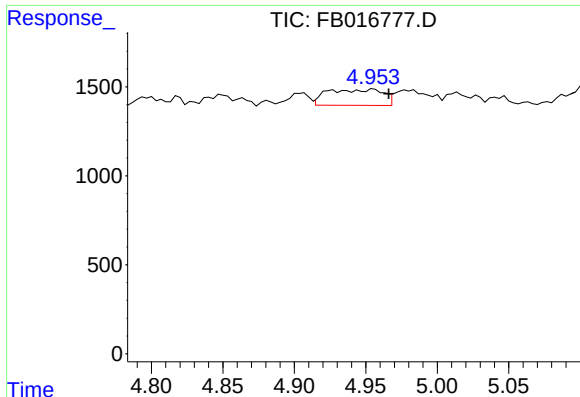


#1 2-Methylpentane

R.T.: 4.956 min
Delta R.T.: -0.010 min
Response: 2428
Conc: 0.17 ng/ml

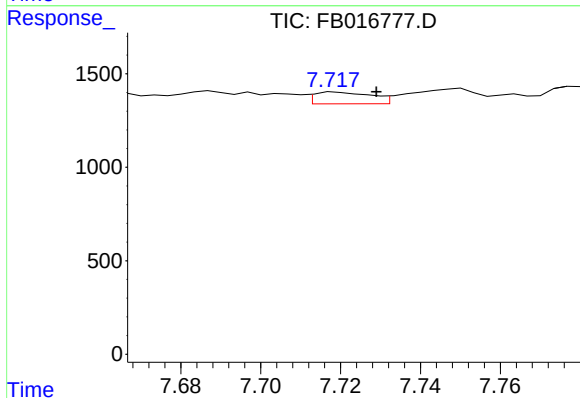


#2 2,2,4-Trimethylpentane

R.T.: 7.719 min
Delta R.T.: -0.010 min
Response: 618
Conc: 0.04 ng/ml

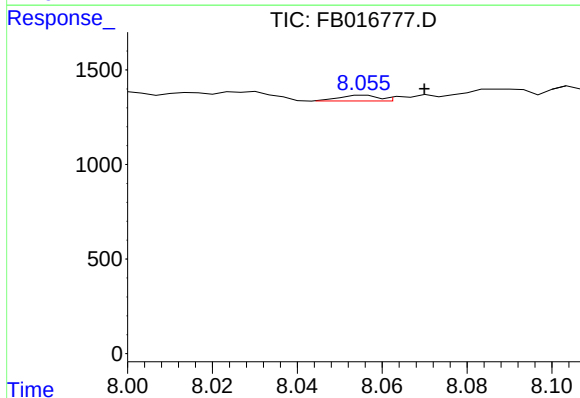


#3 n-Heptane

R.T.: 8.056 min
Delta R.T.: -0.014 min
Response: 189
Conc: 0.01 ng/ml

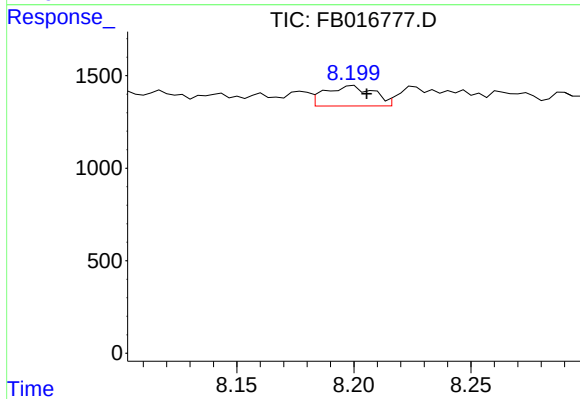


#4 Benzene

R.T.: 8.200 min
Delta R.T.: -0.006 min
Response: 1561
Conc: 0.08 ng/ml

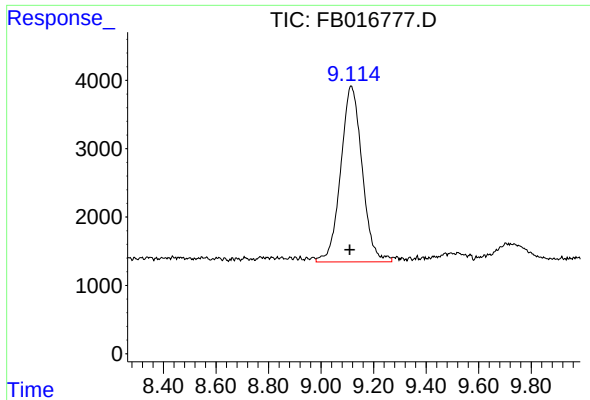


#5 AAA-TFT

R.T.: 9.115 min
Delta R.T.: 0.005 min
Response: 145762
Conc: 16.72 ng/ml

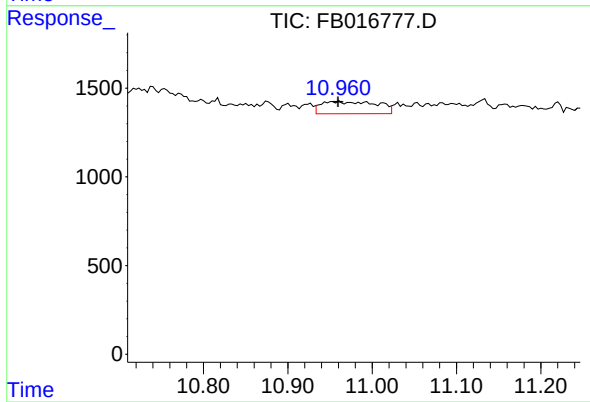


#6 Toluene

R.T.: 10.961 min
Delta R.T.: 0.001 min
Response: 3132
Conc: 0.21 ng/ml

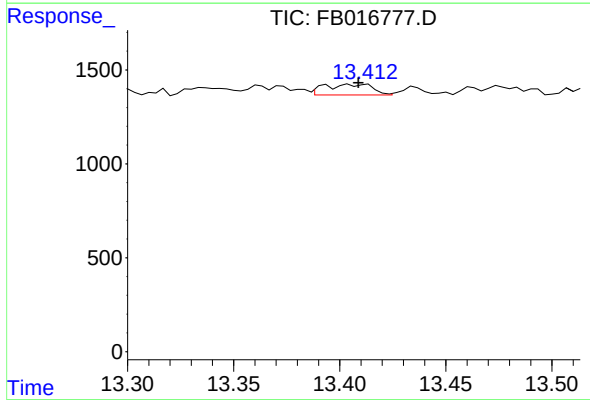


#7 Ethylbenzene

R.T.: 13.412 min
Delta R.T.: 0.003 min
Response: 893
Conc: 0.06 ng/ml

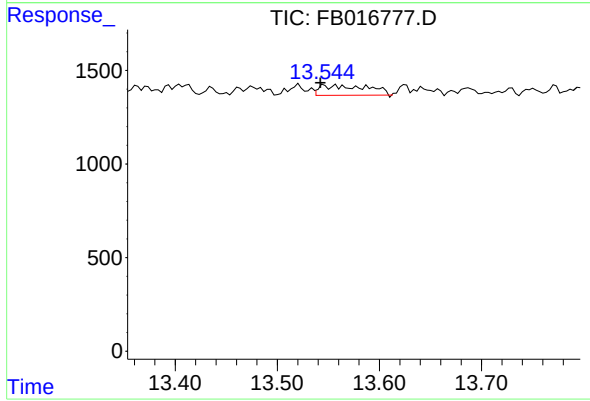


#8 m-Xylene

R.T.: 13.546 min
Delta R.T.: 0.004 min
Response: 1747
Conc: 0.11 ng/ml

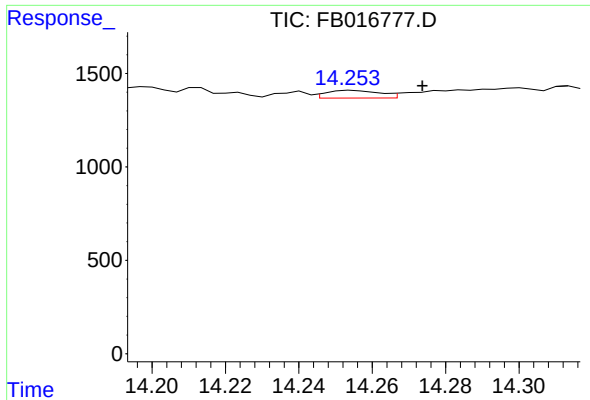

#9 O-Xylene

R.T.: 14.255 min
Delta R.T.: -0.019 min
Response: 410
Conc: 0.02 ng/ml

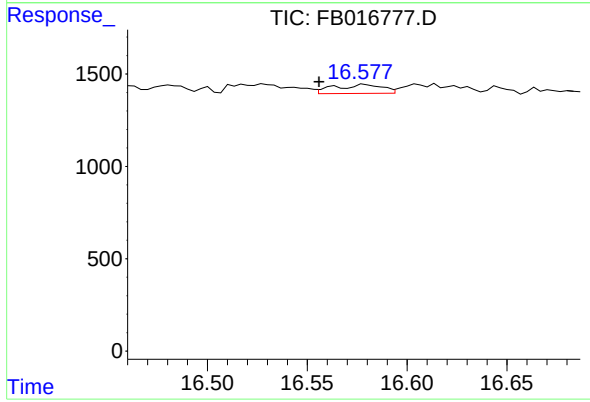

#10 1,2,4-Trimethylbenzene

R.T.: 16.581 min
Delta R.T.: 0.025 min
Response: 809
Conc: 0.04 ng/ml