

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071618\
 Data File : FB016779.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jul 2018 2:42
 Operator : MJ/SJ
 Sample : J4013-03
 Misc : 5.05g/5.00ml DI water
 ALS Vial : 32 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Jul 17 09:03:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
 Quant Title :
 QLast Update : Mon Jul 09 13:06:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.115	154876	17.764 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.954	2386	0.164 ng/ml
2) t	2,2,4-Trimethylpentane	7.721	1175	0.085 ng/ml
3) t	n-Heptane	8.077	530	0.039 ng/ml
4) t	Benzene	8.205	1918	0.103 ng/ml
6) t	Toluene	10.958	2835	0.194 ng/ml
7) t	Ethylbenzene	13.407	2165	0.147 ng/ml
8) t	m-Xylene	13.548	1042	0.067 ng/ml
9) t	O-Xylene	14.284	659	0.040 ng/ml
10) t	1,2,4-Trimethylbenzene	16.560	708	0.036 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071618\
Data File : FB016779.D
Signal(s) : FID2B.CH
Acq On : 17 Jul 2018 2:42
Operator : MJ/SJ
Sample : J4013-03
Misc : 5.05g/5.00ml DI water
ALS Vial : 32 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Jul 17 09:03:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
Quant Title :
QLast Update : Mon Jul 09 13:06:15 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

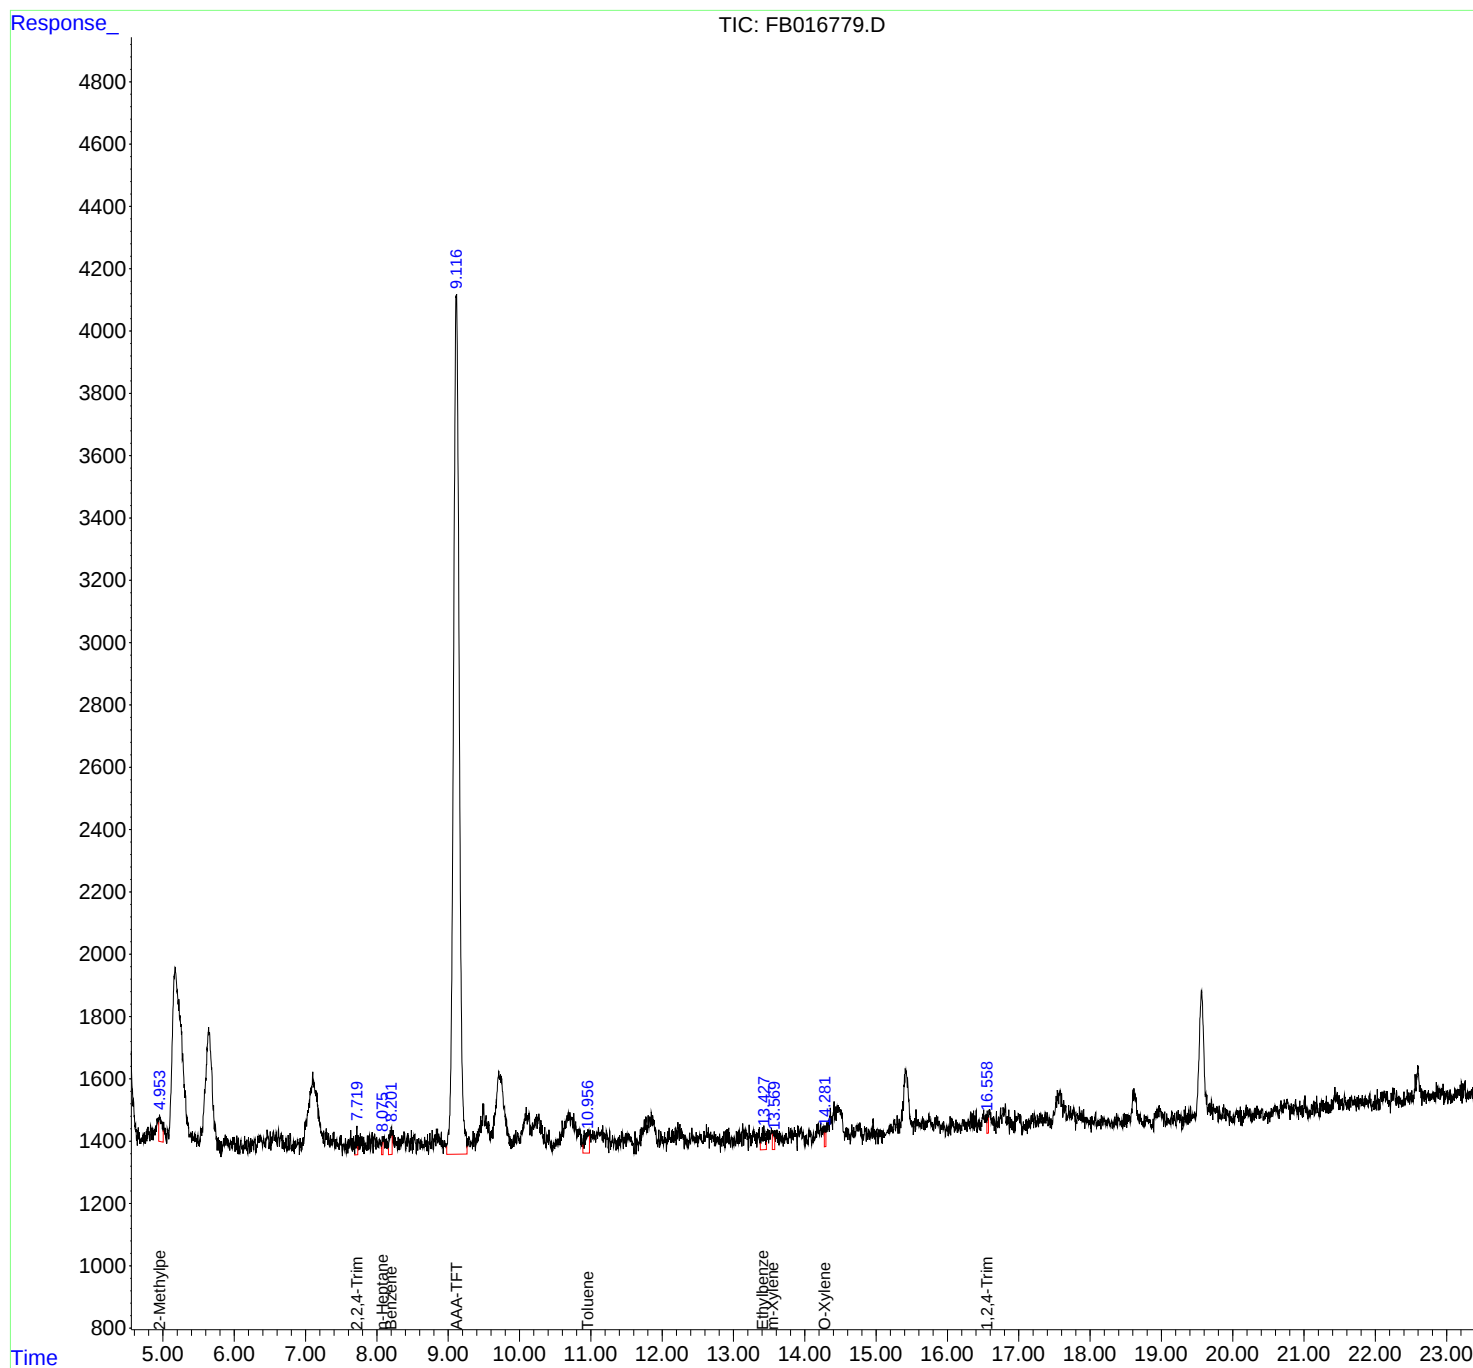

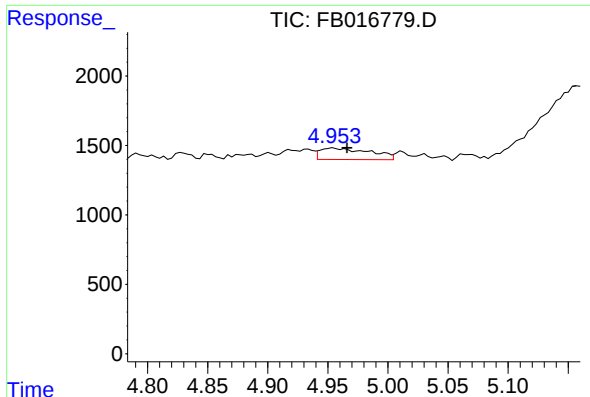


#1 2-Methylpentane

R.T.: 4.954 min
Delta R.T.: -0.012 min
Response: 2386
Conc: 0.16 ng/ml

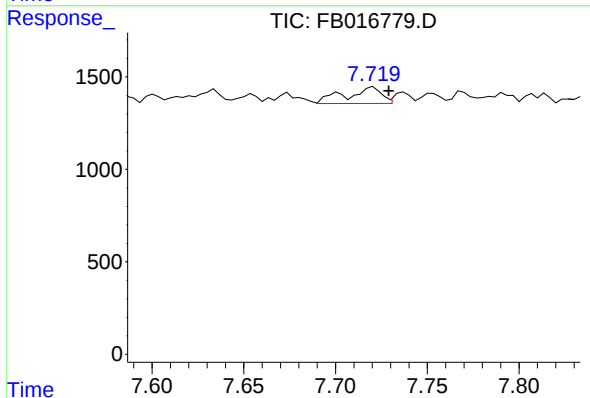


#2 2,2,4-Trimethylpentane

R.T.: 7.721 min
Delta R.T.: -0.008 min
Response: 1175
Conc: 0.08 ng/ml

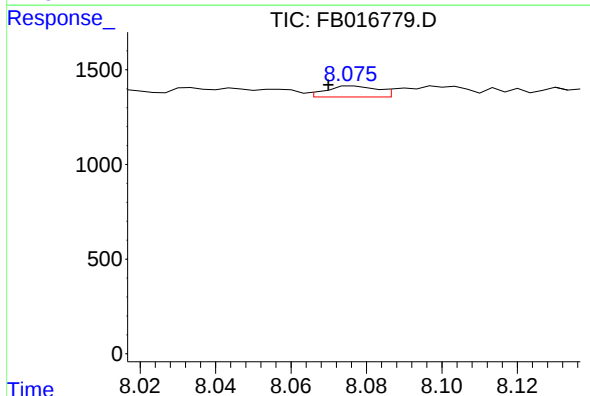


#3 n-Heptane

R.T.: 8.077 min
Delta R.T.: 0.008 min
Response: 530
Conc: 0.04 ng/ml

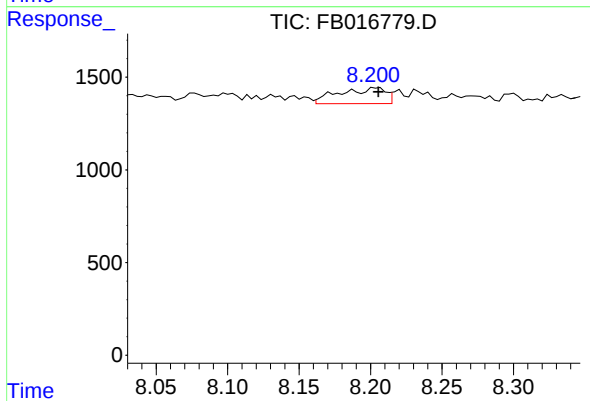


#4 Benzene

R.T.: 8.205 min
Delta R.T.: 0.000 min
Response: 1918
Conc: 0.10 ng/ml

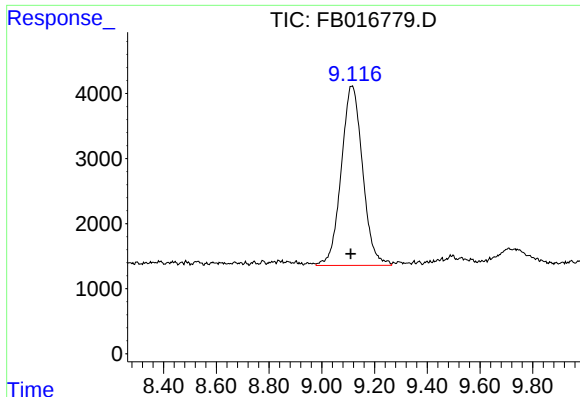


#5 AAA-TFT

R.T.: 9.115 min
Delta R.T.: 0.005 min
Response: 154876
Conc: 17.76 ng/ml

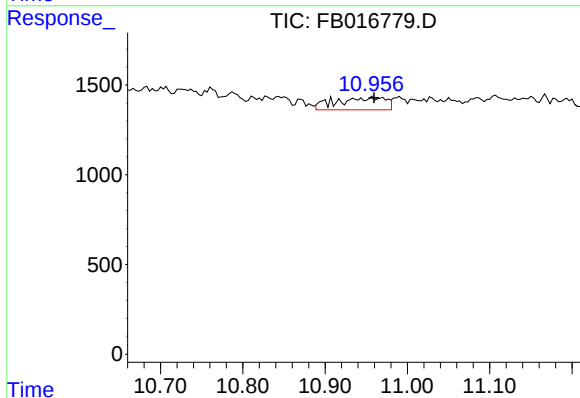


#6 Toluene

R.T.: 10.958 min
Delta R.T.: -0.002 min
Response: 2835
Conc: 0.19 ng/ml

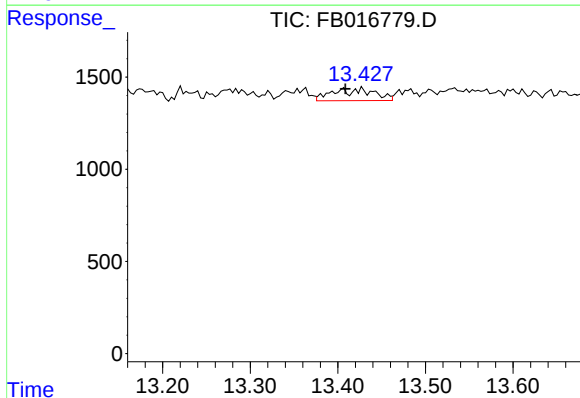


#7 Ethylbenzene

R.T.: 13.407 min
Delta R.T.: -0.002 min
Response: 2165
Conc: 0.15 ng/ml

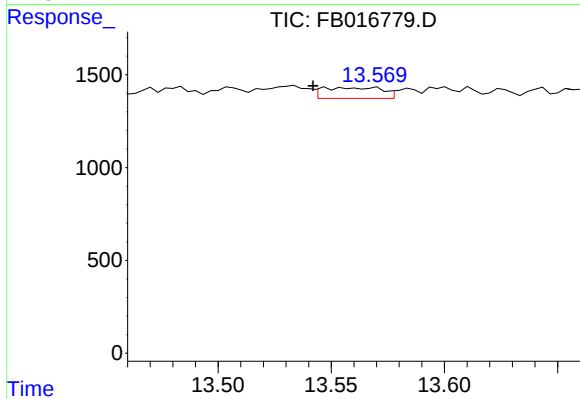


#8 m-Xylene

R.T.: 13.548 min
Delta R.T.: 0.006 min
Response: 1042
Conc: 0.07 ng/ml

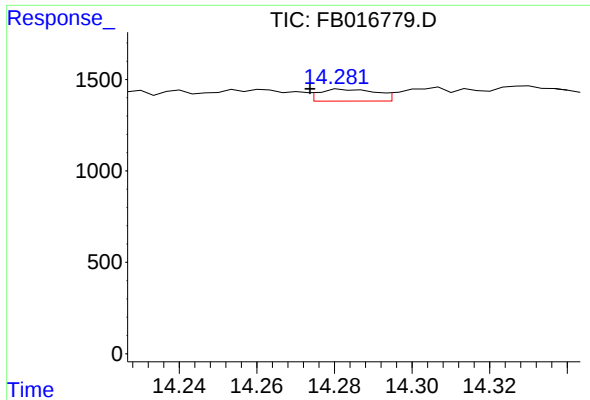

#9 O-Xylene

R.T.: 14.284 min
Delta R.T.: 0.010 min
Response: 659
Conc: 0.04 ng/ml

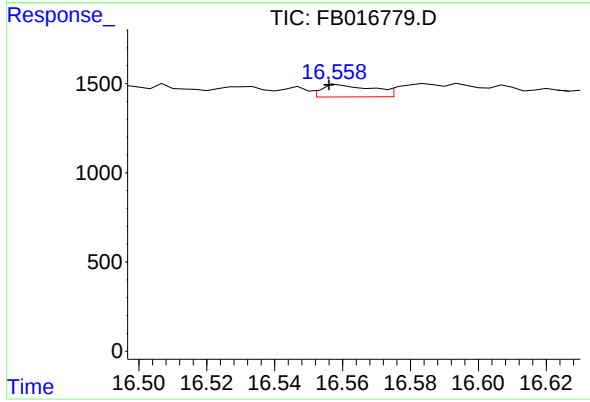

#10 1,2,4-Trimethylbenzene

R.T.: 16.560 min
Delta R.T.: 0.004 min
Response: 708
Conc: 0.04 ng/ml