

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072718\
 Data File : FB016977.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jul 2018 17:39
 Operator : MJ/SJ
 Sample : J4086-09 250X
 Misc : 5.00g/5.00ml DI water
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 30 08:55:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.183	1111250	139.675 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.956	4429267	311.350 ng/ml
2) t 2,2,4-Trimethylpentane	7.720	3731342	272.014 ng/ml
3) t n-Heptane	8.069	1939489	138.883 ng/ml
4) t Benzene	8.209	1046043	59.718 ng/ml
6) t Toluene	10.966	6112593	450.583 ng/ml
7) t Ethylbenzene	13.416	1459075	106.322 ng/ml
8) t m-Xylene	13.547	4943243	340.755 ng/ml
9) t O-Xylene	14.281	2166194	140.796 ng/ml
10) t 1,2,4-Trimethylbenzene	16.564	2815000	150.927 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072718\
Data File : FB016977.D
Signal(s) : FID2B.CH
Acq On : 27 Jul 2018 17:39
Operator : MJ/SJ
Sample : J4086-09 250X
Misc : 5.00g/5.00ml DI water
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 30 08:55:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

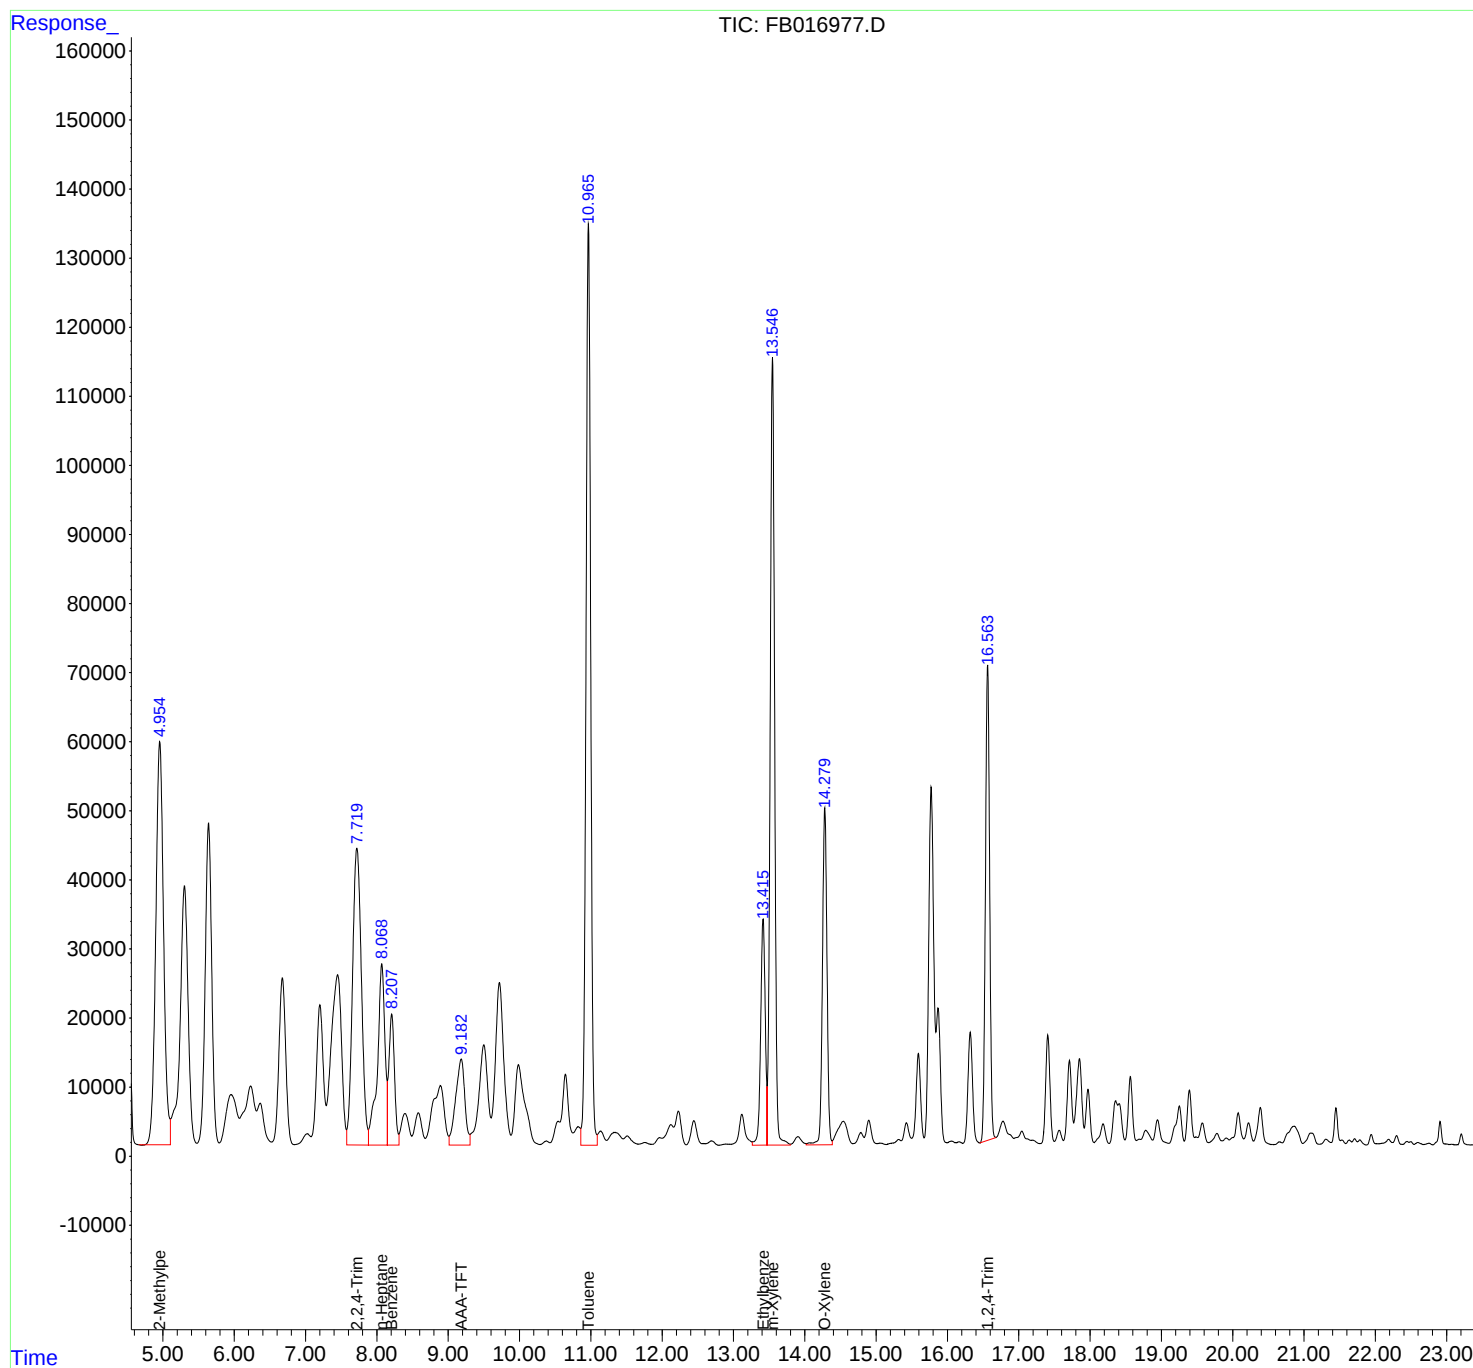

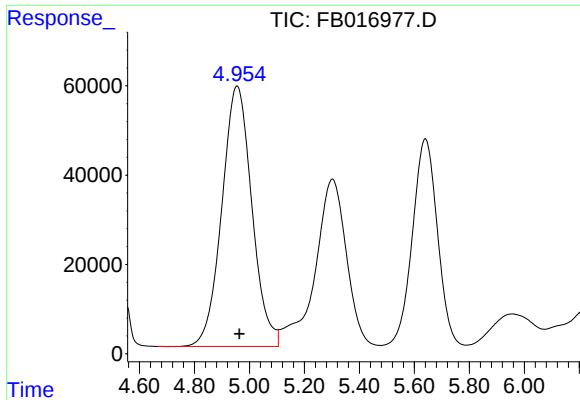


#1 2-Methylpentane

R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 4429267
Conc: 311.35 ng/ml

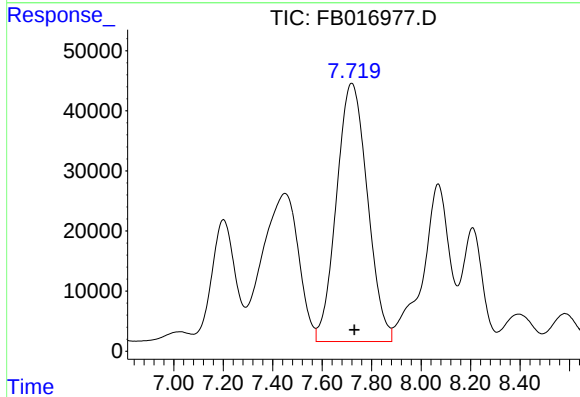


#2 2,2,4-Trimethylpentane

R.T.: 7.720 min
Delta R.T.: -0.010 min
Response: 3731342
Conc: 272.01 ng/ml

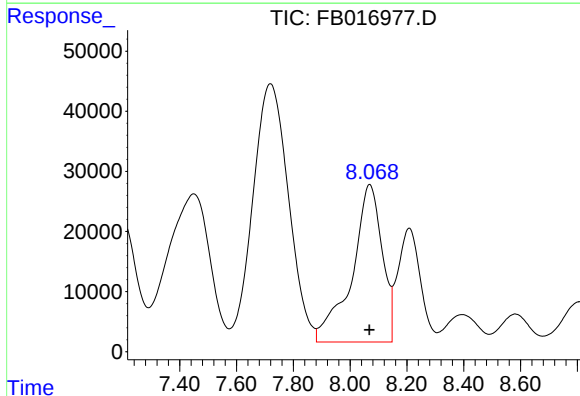


#3 n-Heptane

R.T.: 8.069 min
Delta R.T.: 0.000 min
Response: 1939489
Conc: 138.88 ng/ml

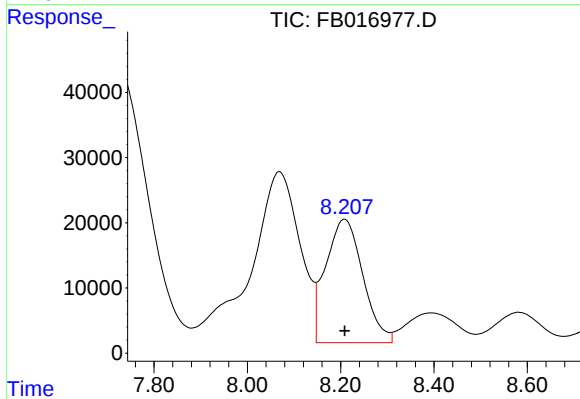


#4 Benzene

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 1046043
Conc: 59.72 ng/ml

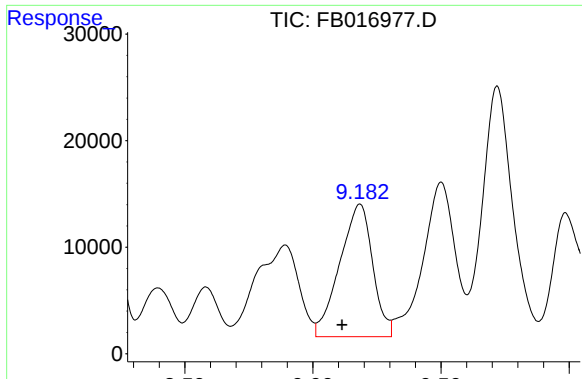


#5 AAA-TFT

R.T.: 9.183 min
Delta R.T.: 0.069 min
Response: 1111250
Conc: 139.68 ng/ml

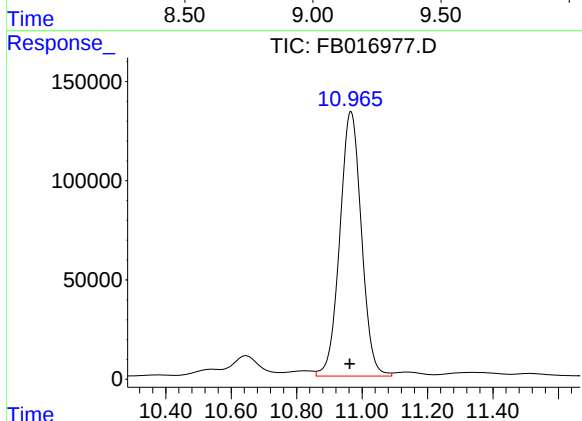


#6 Toluene

R.T.: 10.966 min
Delta R.T.: 0.004 min
Response: 6112593
Conc: 450.58 ng/ml

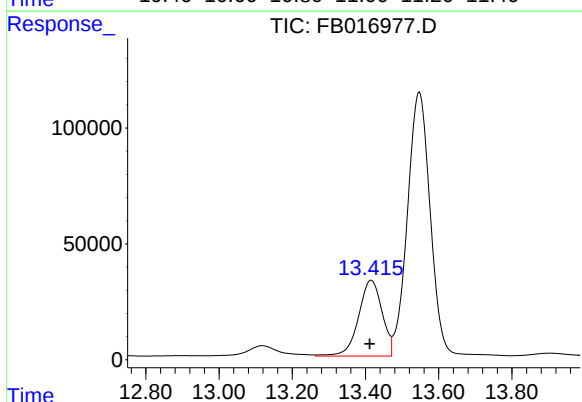


#7 Ethylbenzene

R.T.: 13.416 min
Delta R.T.: 0.004 min
Response: 1459075
Conc: 106.32 ng/ml

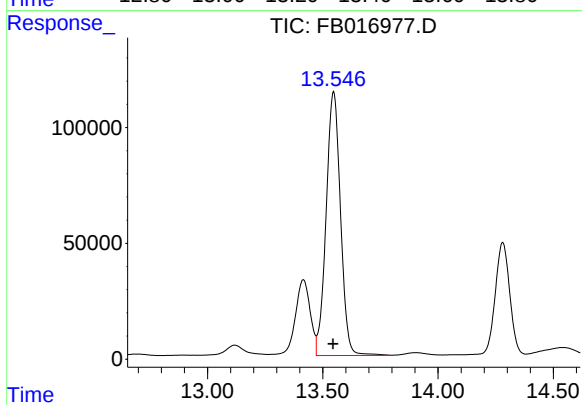

#8 m-Xylene

R.T.: 13.547 min
Delta R.T.: 0.003 min
Response: 4943243
Conc: 340.75 ng/ml

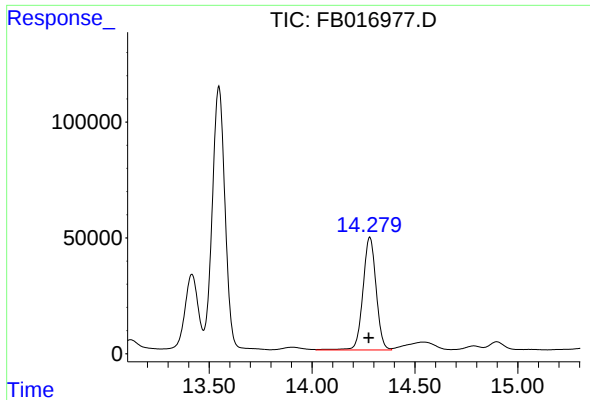


#9 O-Xylene

R.T.: 14.281 min

Delta R.T.: 0.005 min

Response: 2166194

Conc: 140.80 ng/ml

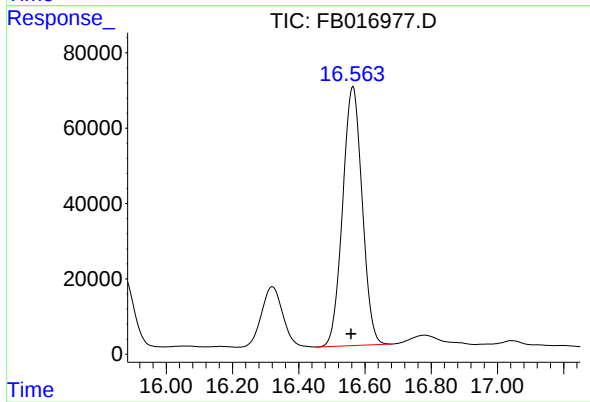

#10 1,2,4-Trimethylbenzene

R.T.: 16.564 min

Delta R.T.: 0.005 min

Response: 2815000

Conc: 150.93 ng/ml