

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072718\
 Data File : FB016979.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jul 2018 19:29
 Operator : MJ/SJ
 Sample : J4086-09 1250X
 Misc : 5.00g/5.00ml DI water
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 30 08:55:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.127	307555	38.657 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.961	760696	53.472 ng/ml
2) t 2,2,4-Trimethylpentane	7.722	654961	47.747 ng/ml
3) t n-Heptane	8.071	342048	24.493 ng/ml
4) t Benzene	8.209	191756	10.947 ng/ml
6) t Toluene	10.965	1117412	82.369 ng/ml
7) t Ethylbenzene	13.414	253394	18.465 ng/ml
8) t m-Xylene	13.545	863944	59.555 ng/ml
9) t O-Xylene	14.279	376932	24.499 ng/ml
10) t 1,2,4-Trimethylbenzene	16.562	528495	28.335 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072718\
Data File : FB016979.D
Signal(s) : FID2B.CH
Acq On : 27 Jul 2018 19:29
Operator : MJ/SJ
Sample : J4086-09 1250X
Misc : 5.00g/5.00ml DI water
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 30 08:55:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

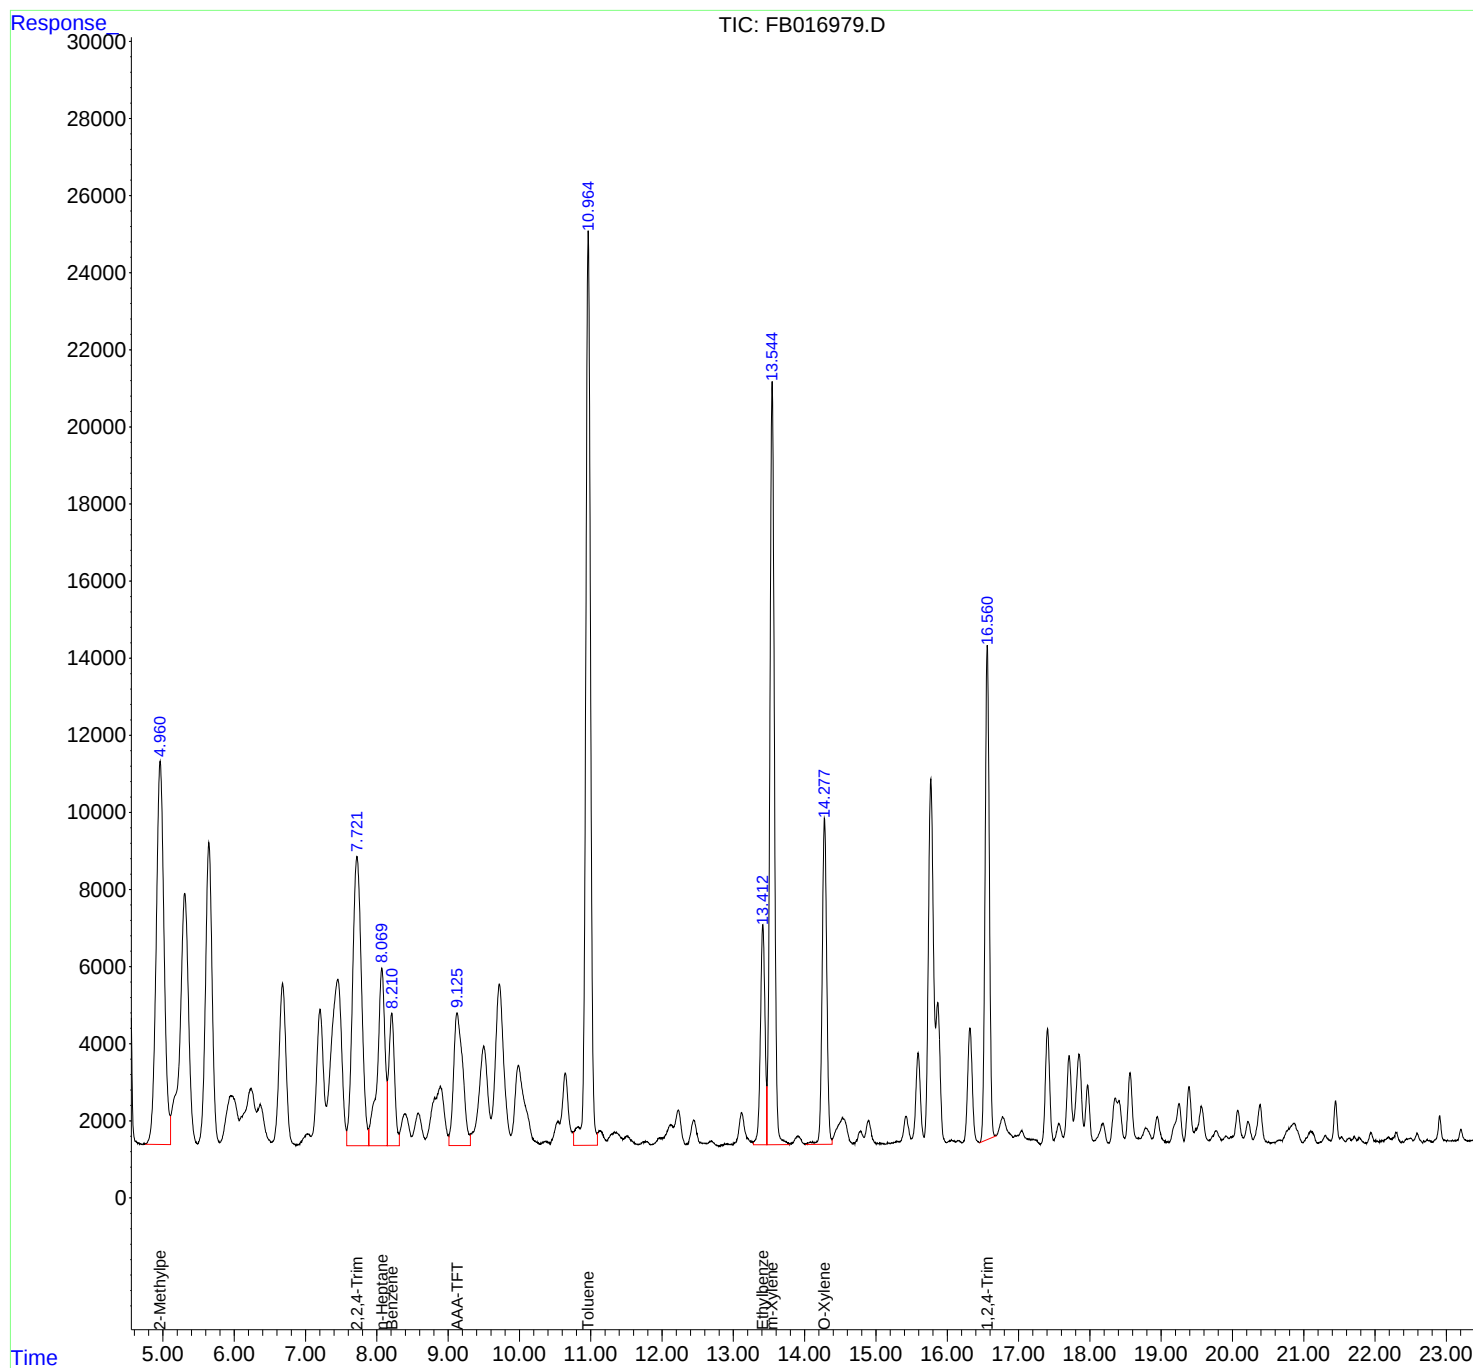

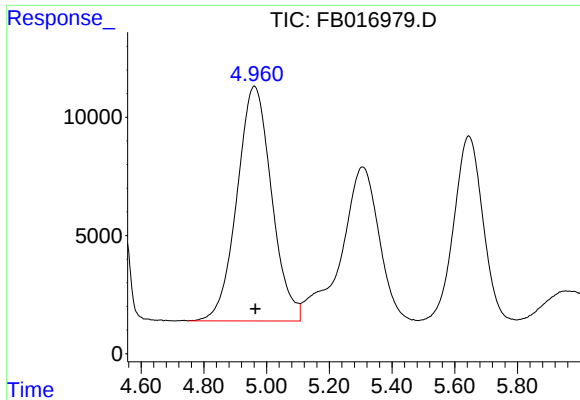


#1 2-Methylpentane

R.T.: 4.961 min
Delta R.T.: -0.003 min
Response: 760696
Conc: 53.47 ng/ml

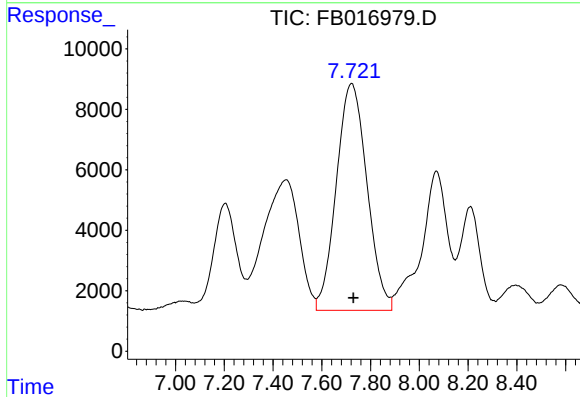


#2 2,2,4-Trimethylpentane

R.T.: 7.722 min
Delta R.T.: -0.008 min
Response: 654961
Conc: 47.75 ng/ml

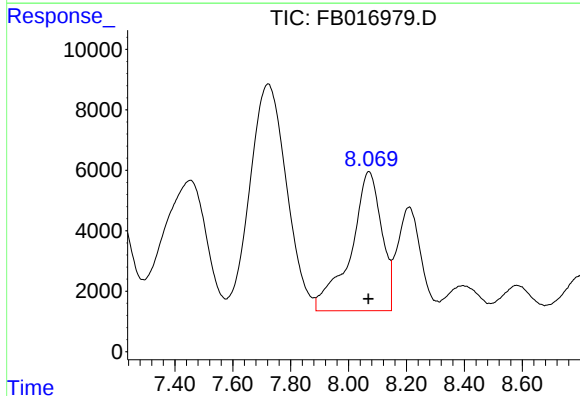


#3 n-Heptane

R.T.: 8.071 min
Delta R.T.: 0.002 min
Response: 342048
Conc: 24.49 ng/ml

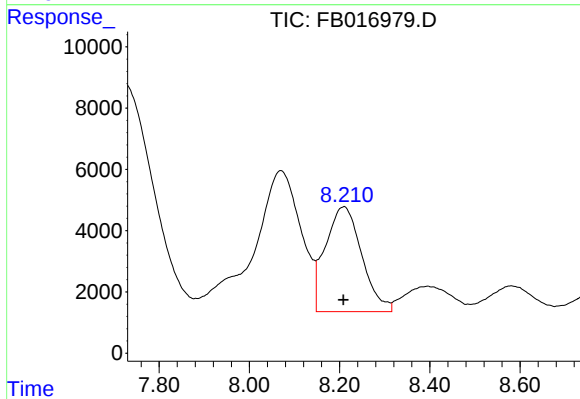


#4 Benzene

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 191756
Conc: 10.95 ng/ml

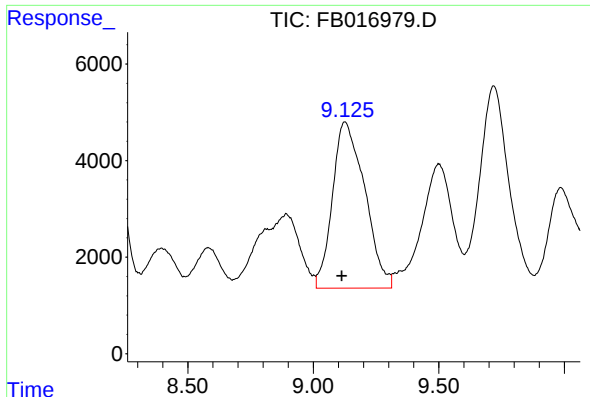


#5 AAA-TFT

R.T.: 9.127 min
Delta R.T.: 0.013 min
Response: 307555
Conc: 38.66 ng/ml

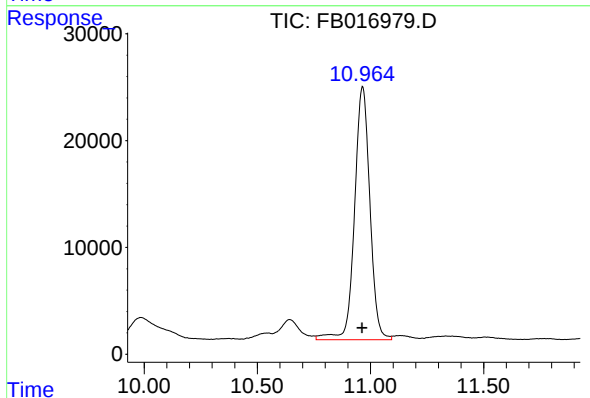


#6 Toluene

R.T.: 10.965 min
Delta R.T.: 0.003 min
Response: 1117412
Conc: 82.37 ng/ml

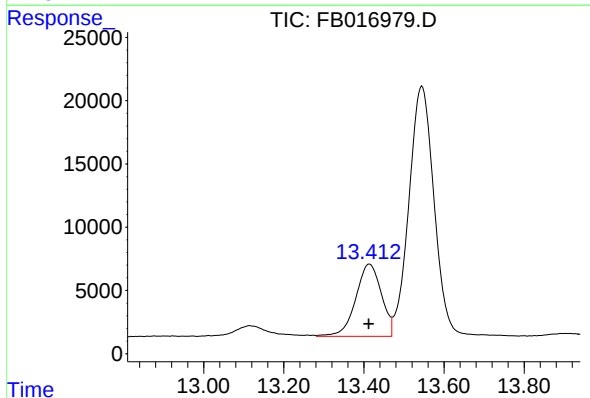


#7 Ethylbenzene

R.T.: 13.414 min
Delta R.T.: 0.003 min
Response: 253394
Conc: 18.46 ng/ml

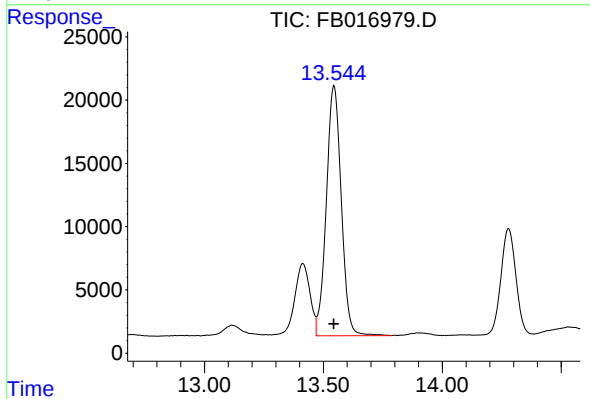


#8 m-Xylene

R.T.: 13.545 min
Delta R.T.: 0.000 min
Response: 863944
Conc: 59.55 ng/ml

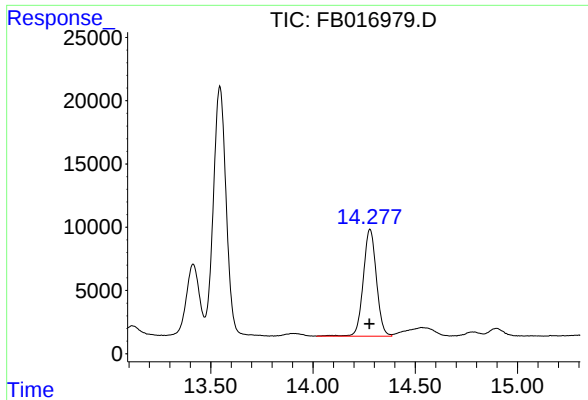

#9 O-Xylene

R.T.: 14.279 min
Delta R.T.: 0.003 min
Response: 376932
Conc: 24.50 ng/ml

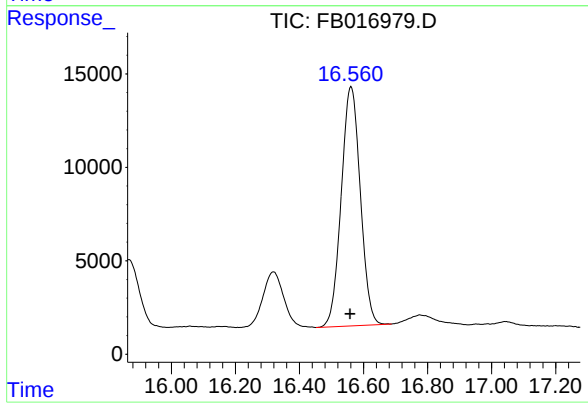

#10 1,2,4-Trimethylbenzene

R.T.: 16.562 min
Delta R.T.: 0.003 min
Response: 528495
Conc: 28.34 ng/ml