

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080418\
 Data File : FB017148.D
 Signal(s) : FID2B.CH
 Acq On : 4 Aug 2018 11:03
 Operator : MJ/SJ
 Sample : BSF0804S1
 Misc : 5.03g/5.00ml DI water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 06 08:03:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	162051	20.476 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.964	429528	29.756 ng/ml
2) t 2,2,4-Trimethylpentane	7.729	417417	29.839 ng/ml
3) t n-Heptane	8.068	131760	9.370 ng/ml
4) t Benzene	8.208	164452	9.361 ng/ml
6) t Toluene	10.961	418952	30.508 ng/ml
7) t Ethylbenzene	13.411	141384	10.368 ng/ml
8) t m-Xylene	13.544	299019	20.783 ng/ml
9) t O-Xylene	14.276	321590	21.087 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	366487	19.856 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080418\
Data File : FB017148.D
Signal(s) : FID2B.CH
Acq On : 4 Aug 2018 11:03
Operator : MJ/SJ
Sample : BSF0804S1
Misc : 5.03g/5.00ml DI water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 06 08:03:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

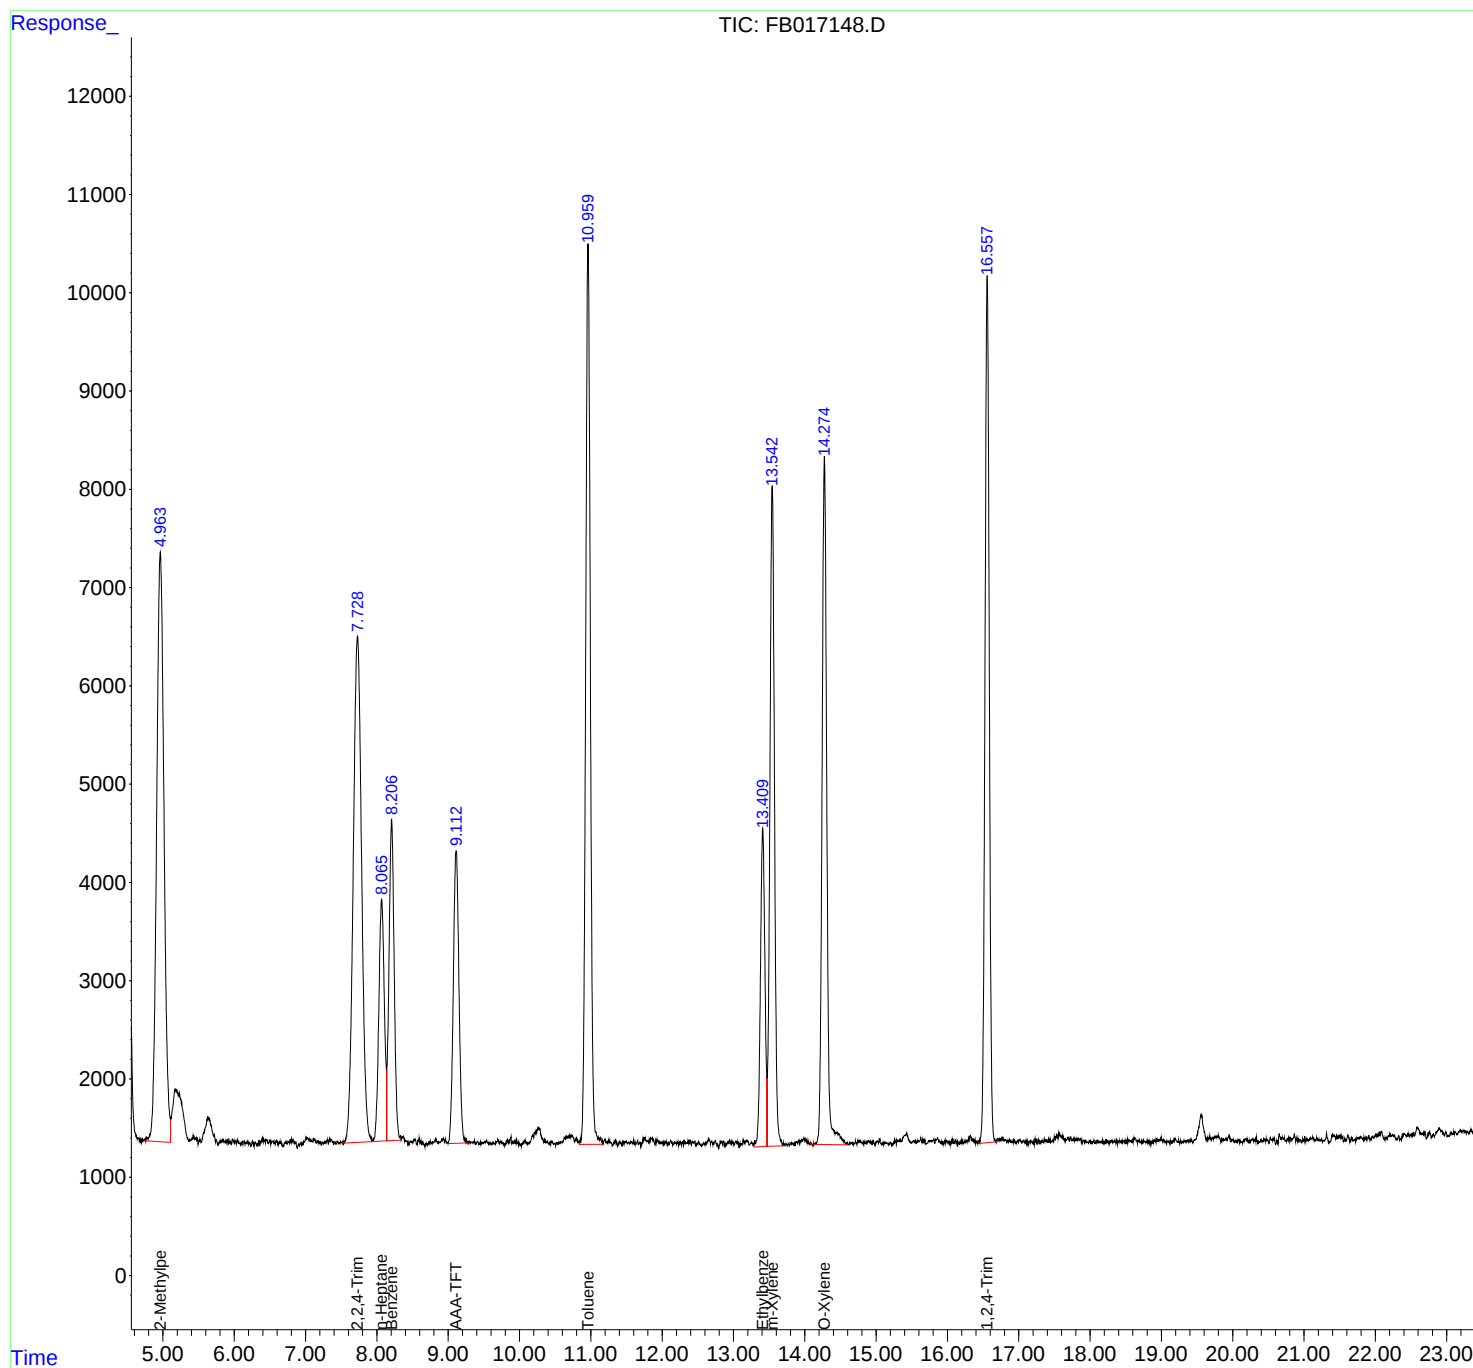

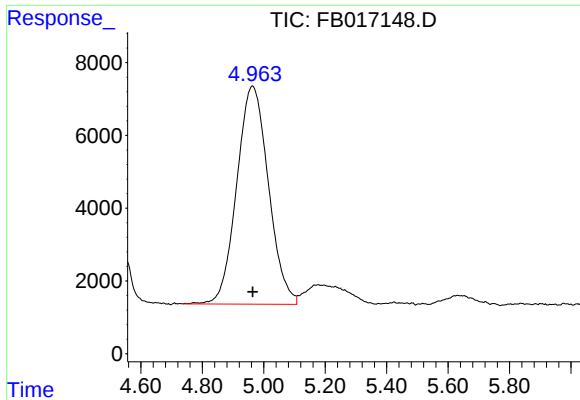


#1 2-Methylpentane

R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 429528
Conc: 29.76 ng/ml

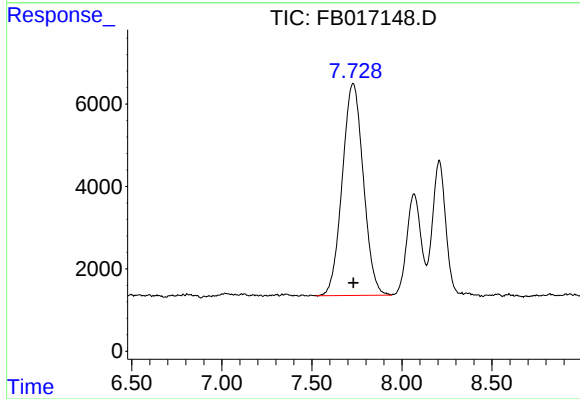


#2 2,2,4-Trimethylpentane

R.T.: 7.729 min
Delta R.T.: -0.001 min
Response: 417417
Conc: 29.84 ng/ml

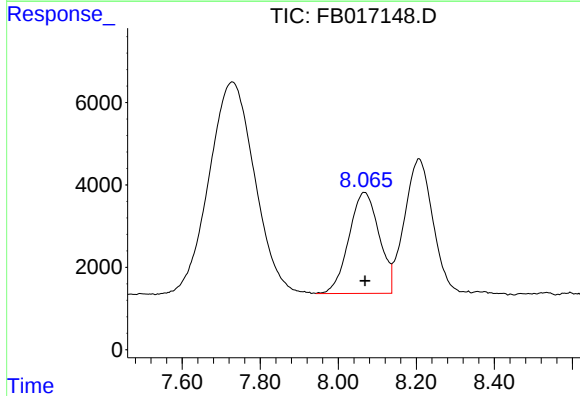


#3 n-Heptane

R.T.: 8.068 min
Delta R.T.: -0.001 min
Response: 131760
Conc: 9.37 ng/ml

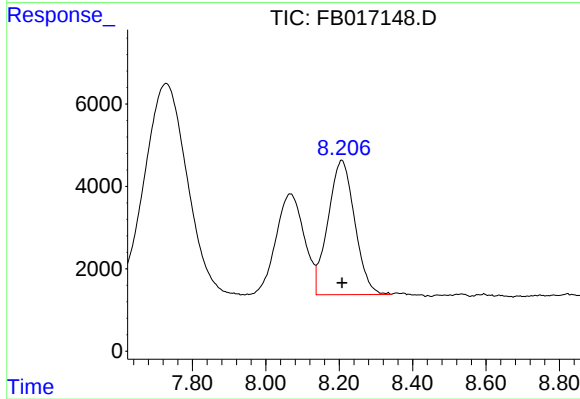


#4 Benzene

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 164452
Conc: 9.36 ng/ml

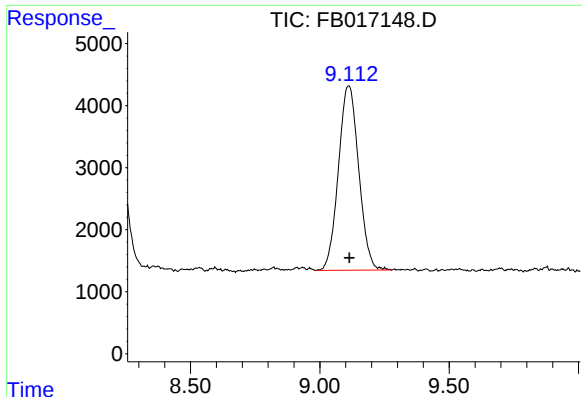


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: -0.001 min
Response: 162051
Conc: 20.48 ng/ml

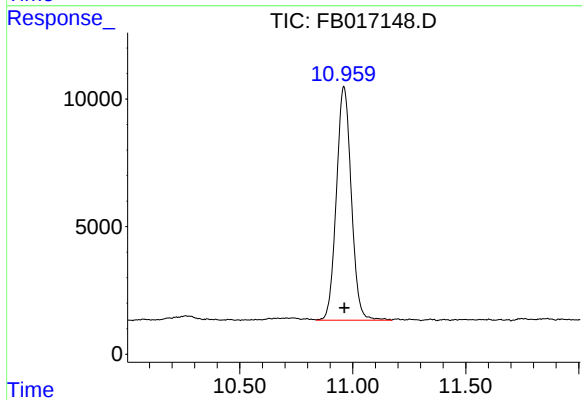


#6 Toluene

R.T.: 10.961 min
Delta R.T.: -0.002 min
Response: 418952
Conc: 30.51 ng/ml

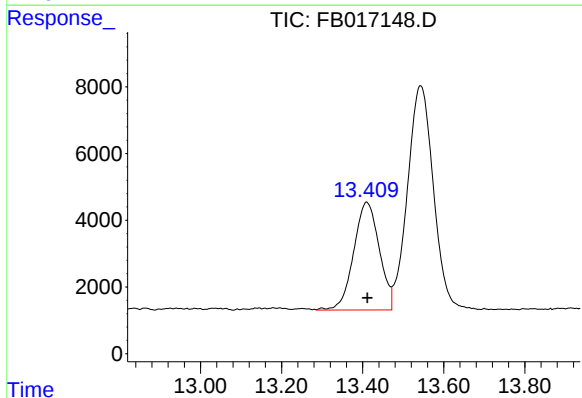


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 141384
Conc: 10.37 ng/ml

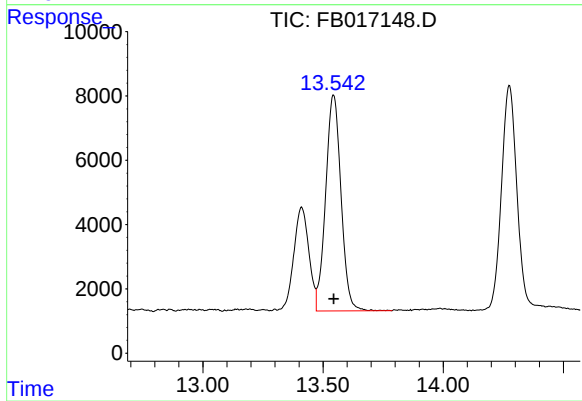


#8 m-Xylene

R.T.: 13.544 min
Delta R.T.: 0.000 min
Response: 299019
Conc: 20.78 ng/ml

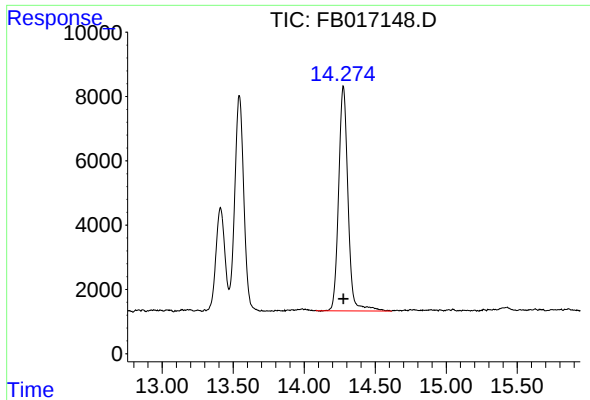

#9 O-Xylene

R.T.: 14.276 min
Delta R.T.: 0.000 min
Response: 321590
Conc: 21.09 ng/ml

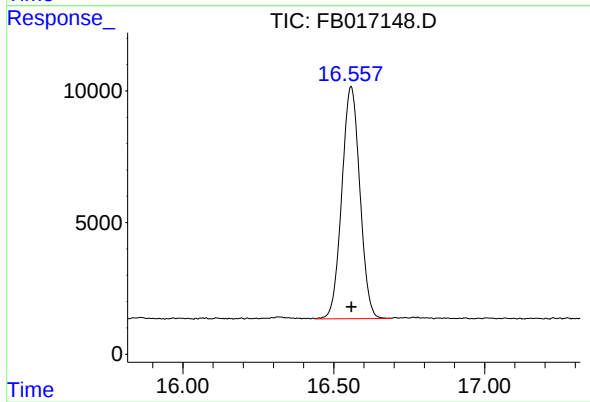

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.000 min
Response: 366487
Conc: 19.86 ng/ml