

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080418\
 Data File : FB017151.D
 Signal(s) : FID2B.CH
 Acq On : 4 Aug 2018 13:36
 Operator : MJ/SJ
 Sample : J4316-06MS
 Misc : 5.00g/5.00ml DI water
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 06 08:03:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.113	164924	20.839 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.965	407359	28.220 ng/ml
2) t 2,2,4-Trimethylpentane	7.730	388605	27.779 ng/ml
3) t n-Heptane	8.070	124740	8.871 ng/ml
4) t Benzene	8.207	157554	8.968 ng/ml
6) t Toluene	10.962	387045	28.184 ng/ml
7) t Ethylbenzene	13.412	134980	9.899 ng/ml
8) t m-Xylene	13.544	283063	19.674 ng/ml
9) t O-Xylene	14.276	295895	19.402 ng/ml
10) t 1,2,4-Trimethylbenzene	16.559	350944	19.014 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080418\
Data File : FB017151.D
Signal(s) : FID2B.CH
Acq On : 4 Aug 2018 13:36
Operator : MJ/SJ
Sample : J4316-06MS
Misc : 5.00g/5.00ml DI water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 06 08:03:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

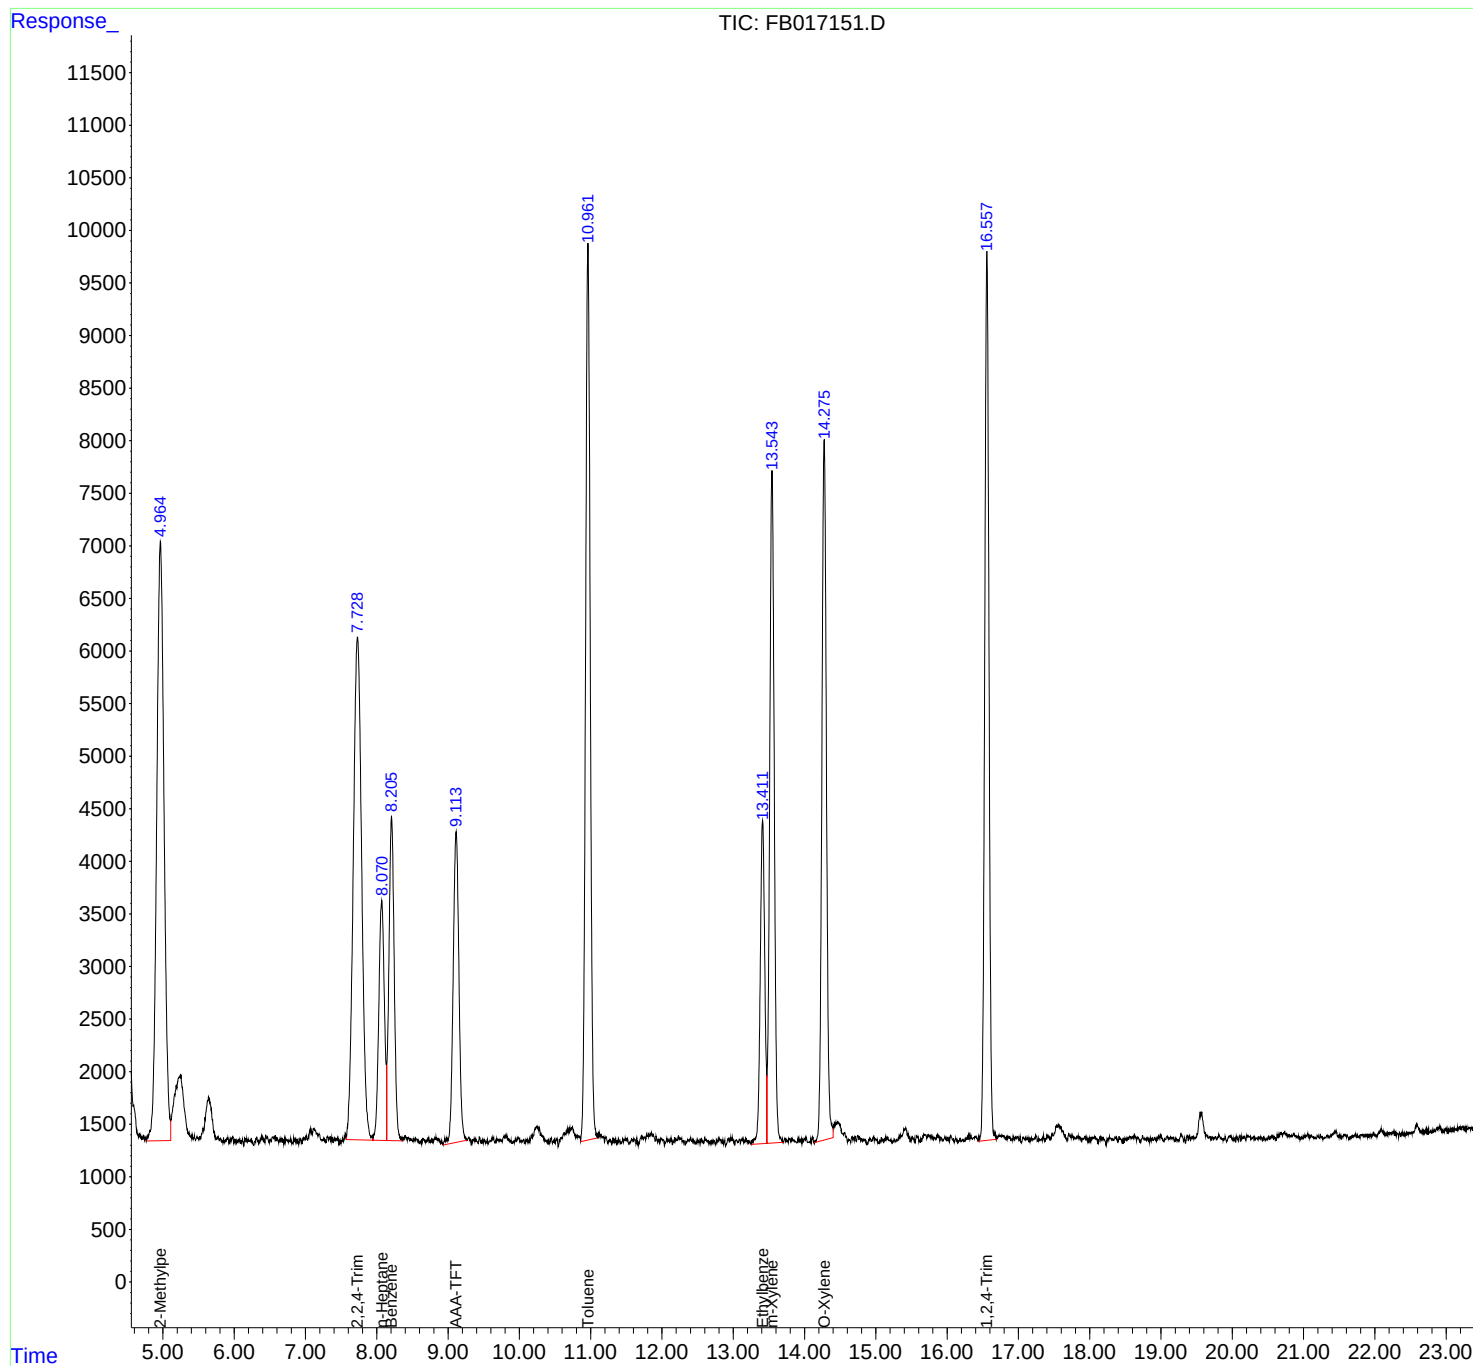

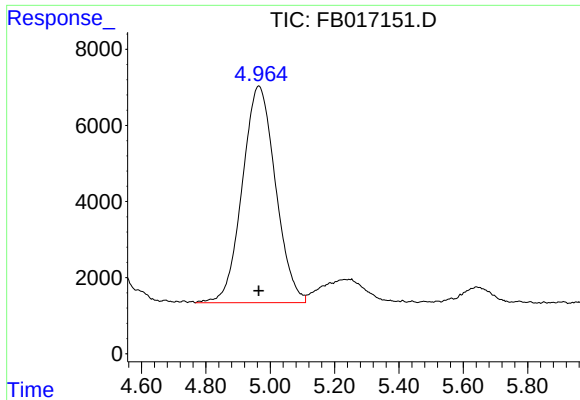


#1 2-Methylpentane

R.T.: 4.965 min
Delta R.T.: 0.001 min
Response: 407359
Conc: 28.22 ng/ml

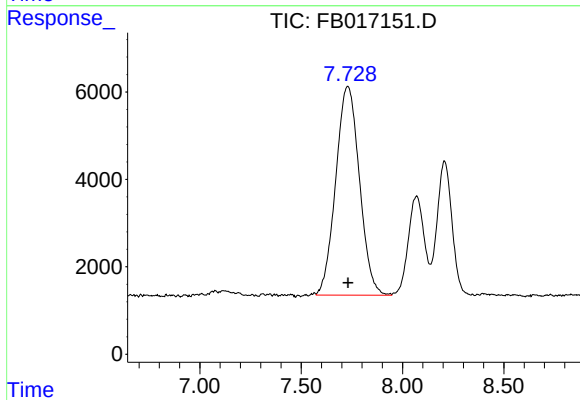


#2 2,2,4-Trimethylpentane

R.T.: 7.730 min
Delta R.T.: 0.000 min
Response: 388605
Conc: 27.78 ng/ml

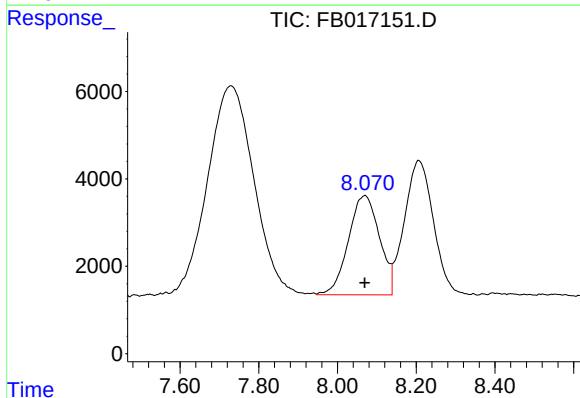


#3 n-Heptane

R.T.: 8.070 min
Delta R.T.: 0.001 min
Response: 124740
Conc: 8.87 ng/ml

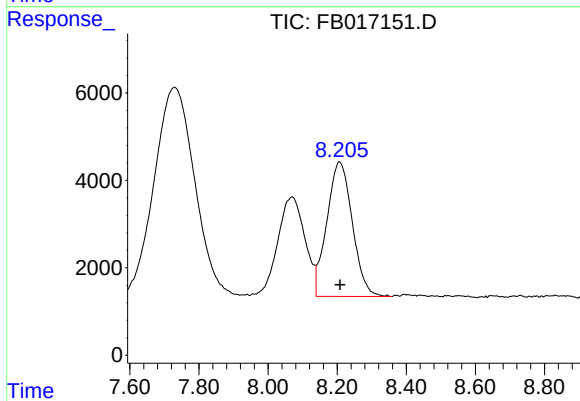


#4 Benzene

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 157554
Conc: 8.97 ng/ml

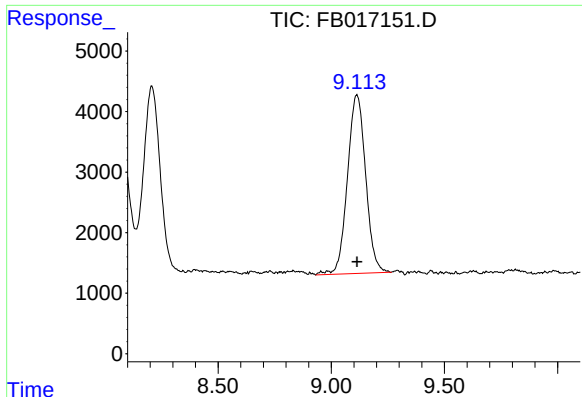


#5 AAA-TFT

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 164924
Conc: 20.84 ng/ml

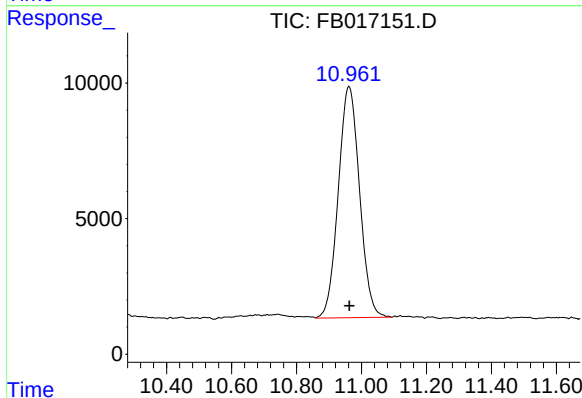


#6 Toluene

R.T.: 10.962 min
Delta R.T.: 0.000 min
Response: 387045
Conc: 28.18 ng/ml

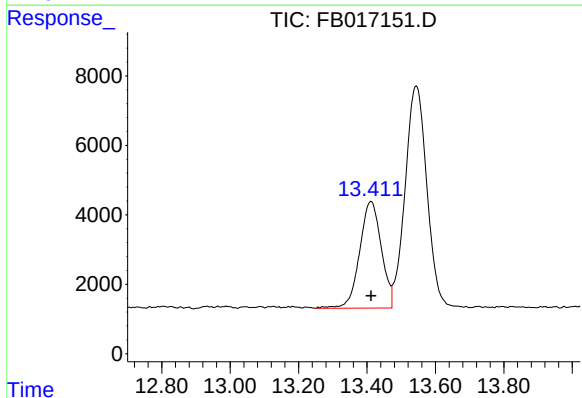


#7 Ethylbenzene

R.T.: 13.412 min
Delta R.T.: 0.000 min
Response: 134980
Conc: 9.90 ng/ml

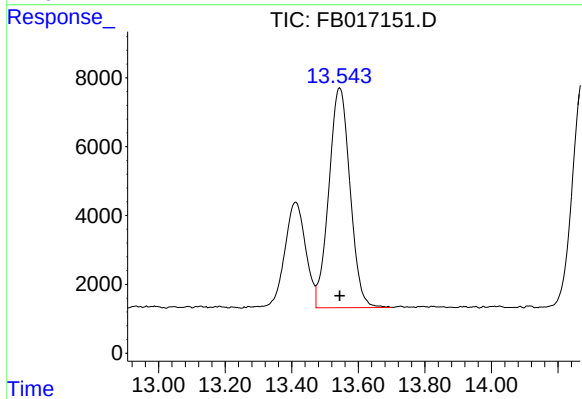


#8 m-Xylene

R.T.: 13.544 min
Delta R.T.: 0.000 min
Response: 283063
Conc: 19.67 ng/ml

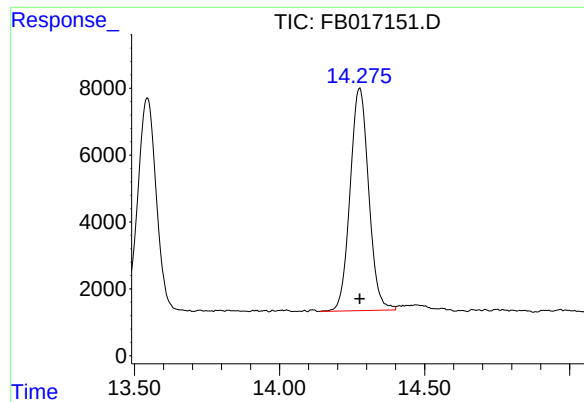

#9 O-Xylene

R.T.: 14.276 min
Delta R.T.: 0.000 min
Response: 295895
Conc: 19.40 ng/ml

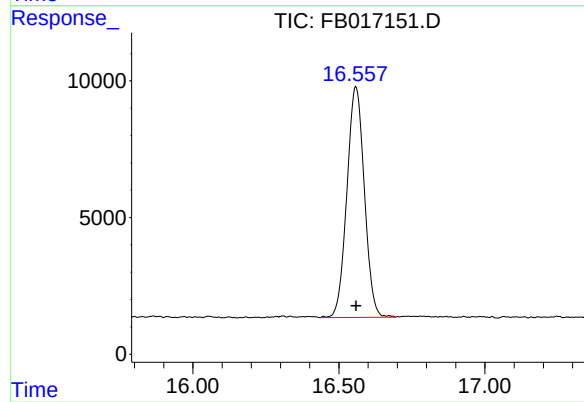

#10 1,2,4-Trimethylbenzene

R.T.: 16.559 min
Delta R.T.: 0.000 min
Response: 350944
Conc: 19.01 ng/ml