

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081318\
 Data File : FB017301.D
 Signal(s) : FID2B.CH
 Acq On : 13 Aug 2018 9:11
 Operator : MJ/SJ
 Sample : BSF0813S1
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 13 12:57:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080818.M
 Quant Title :
 QLast Update : Wed Aug 08 11:39:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	167032	17.827 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.963	421195	24.632 ng/ml
2) t 2,2,4-Trimethylpentane	7.727	425660	25.193 ng/ml
3) t n-Heptane	8.068	135383	8.404 ng/ml
4) t Benzene	8.207	176297	8.699 ng/ml
6) t Toluene	10.961	428871	26.018 ng/ml
7) t Ethylbenzene	13.411	147880	8.864 ng/ml
8) t m-Xylene	13.544	312546	16.672 ng/ml
9) t O-Xylene	14.275	326961	16.088 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	389515	17.392 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081318\
Data File : FB017301.D
Signal(s) : FID2B.CH
Acq On : 13 Aug 2018 9:11
Operator : MJ/SJ
Sample : BSF0813S1
Misc : 5.00g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 13 12:57:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080818.M
Quant Title :
QLast Update : Wed Aug 08 11:39:03 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

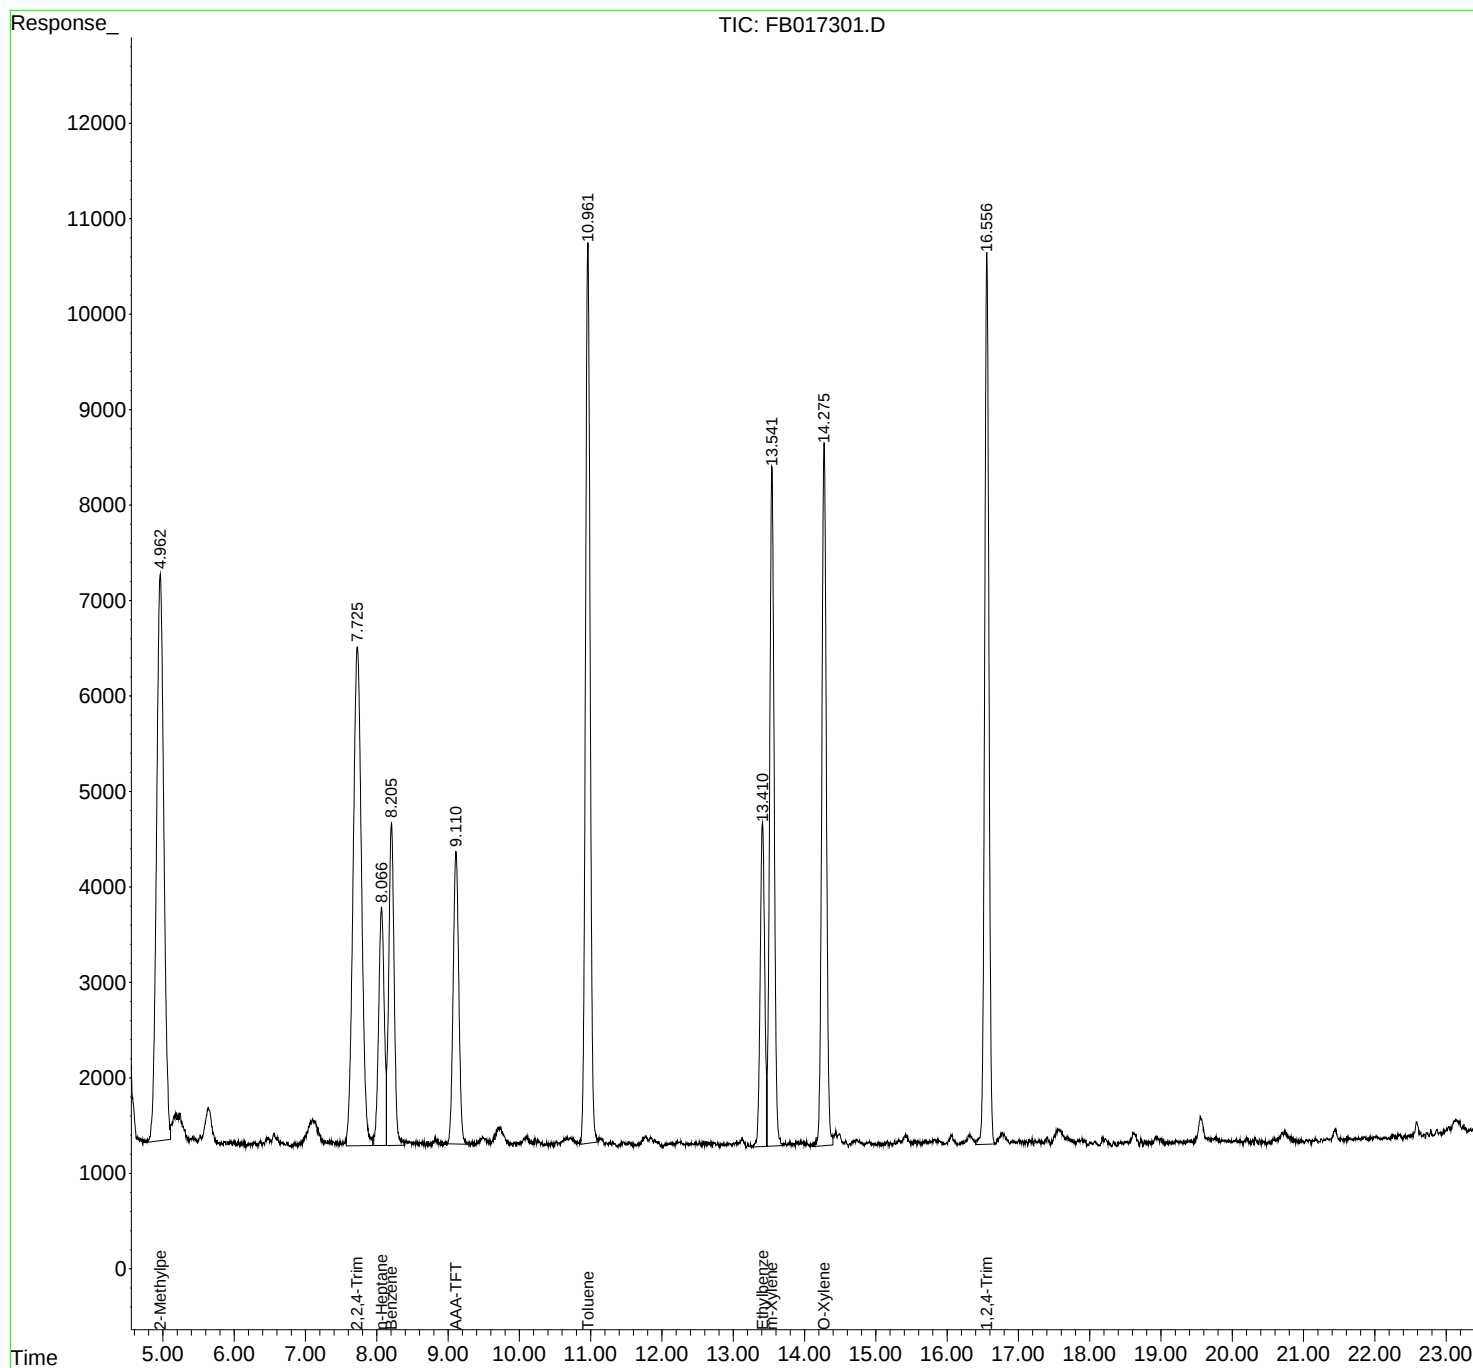

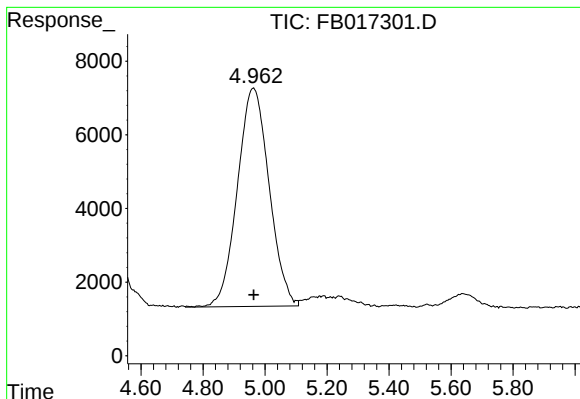


#1 2-Methylpentane

R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 421195
Conc: 24.63 ng/ml

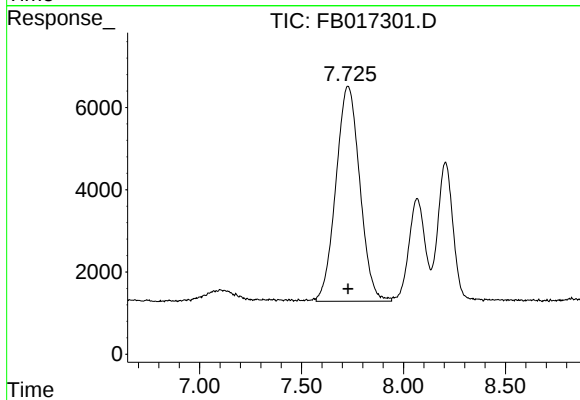


#2 2,2,4-Trimethylpentane

R.T.: 7.727 min
Delta R.T.: -0.001 min
Response: 425660
Conc: 25.19 ng/ml

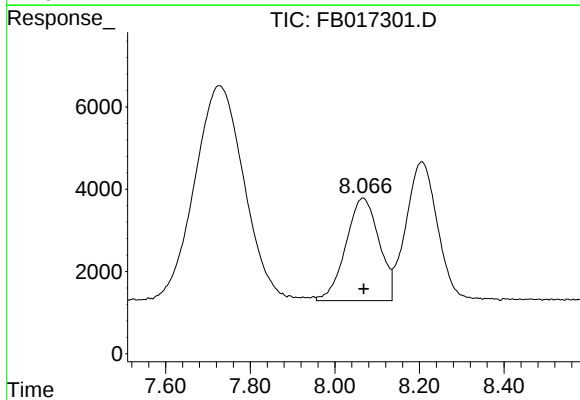


#3 n-Heptane

R.T.: 8.068 min
Delta R.T.: 0.000 min
Response: 135383
Conc: 8.40 ng/ml

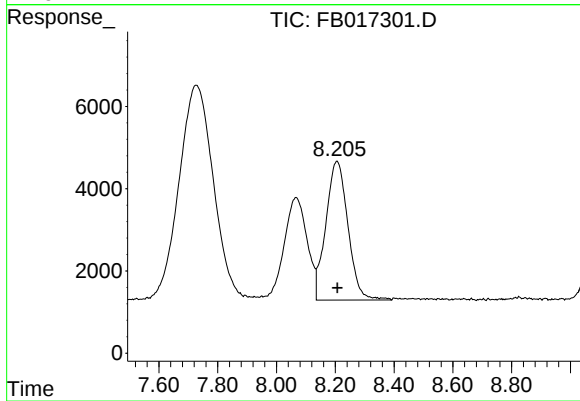


#4 Benzene


R.T.: 8.207 min
Delta R.T.: -0.001 min
Response: 176297
Conc: 8.70 ng/ml

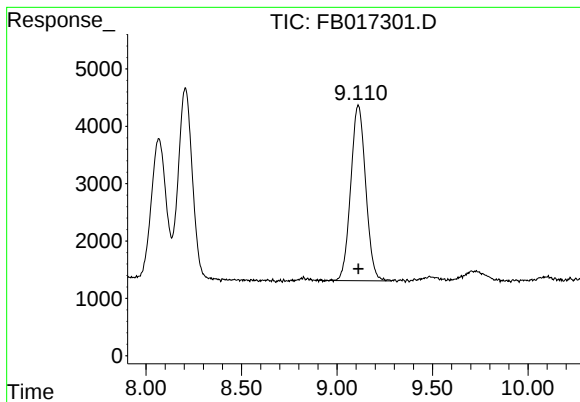


#5 AAA-TFT
 R.T.: 9.112 min
 Delta R.T.: 0.000 min
 Response: 167032
 Conc: 17.83 ng/ml

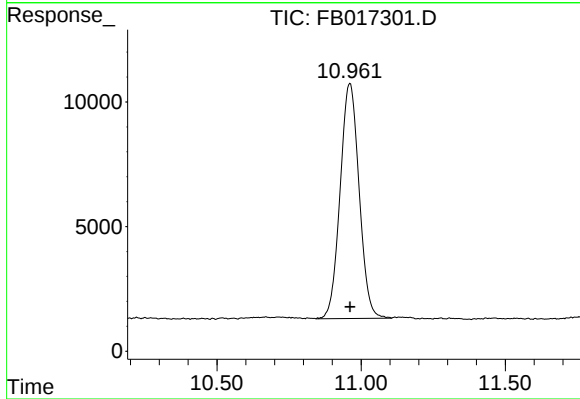


#6 Toluene
 R.T.: 10.961 min
 Delta R.T.: 0.000 min
 Response: 428871
 Conc: 26.02 ng/ml

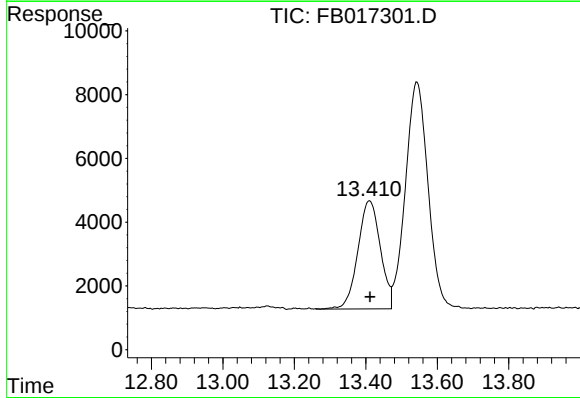

#7 Ethylbenzene
 R.T.: 13.411 min
 Delta R.T.: -0.001 min
 Response: 147880
 Conc: 8.86 ng/ml

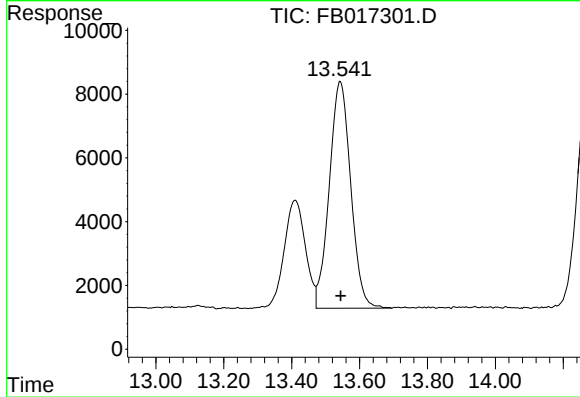


#8 m-Xylene
 R.T.: 13.544 min
 Delta R.T.: 0.000 min
 Response: 312546
 Conc: 16.67 ng/ml

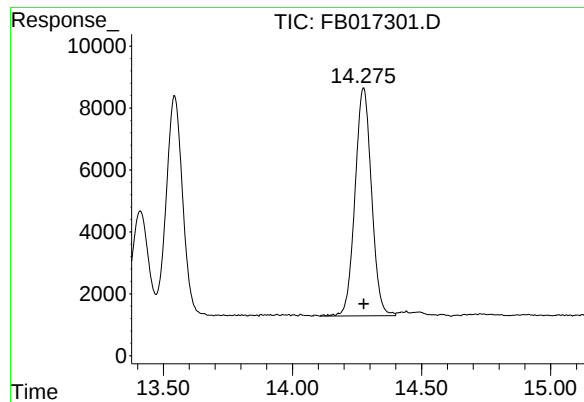

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: -0.001 min
Response: 326961
Conc: 16.09 ng/ml

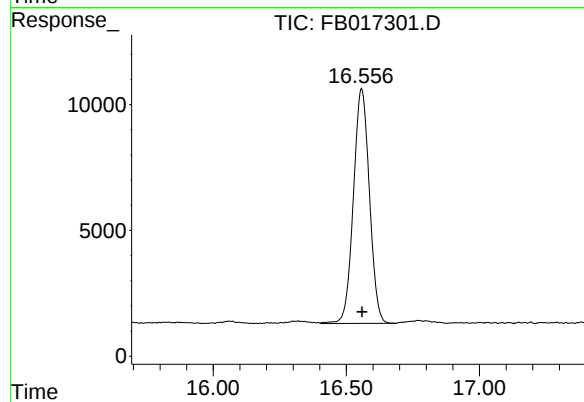

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: -0.001 min
Response: 389515
Conc: 17.39 ng/ml