

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081418\
 Data File : FB017343.D
 Signal(s) : FID2B.CH
 Acq On : 14 Aug 2018 10:20
 Operator : MJ/SJ
 Sample : BSF0814S1
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 15 07:51:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080818.M
 Quant Title :
 QLast Update : Wed Aug 08 11:39:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.114	169919	18.135 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.963	465697	27.234 ng/ml
2) t 2,2,4-Trimethylpentane	7.729	459843	27.216 ng/ml
3) t n-Heptane	8.069	146853	9.116 ng/ml
4) t Benzene	8.209	183789	9.069 ng/ml
6) t Toluene	10.964	450079	27.305 ng/ml
7) t Ethylbenzene	13.413	151960	9.108 ng/ml
8) t m-Xylene	13.546	321939	17.173 ng/ml
9) t O-Xylene	14.278	339664	16.713 ng/ml
10) t 1,2,4-Trimethylbenzene	16.560	405430	18.103 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081418\
Data File : FB017343.D
Signal(s) : FID2B.CH
Acq On : 14 Aug 2018 10:20
Operator : MJ/SJ
Sample : BSF0814S1
Misc : 5.00g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 15 07:51:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080818.M
Quant Title :
QLast Update : Wed Aug 08 11:39:03 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

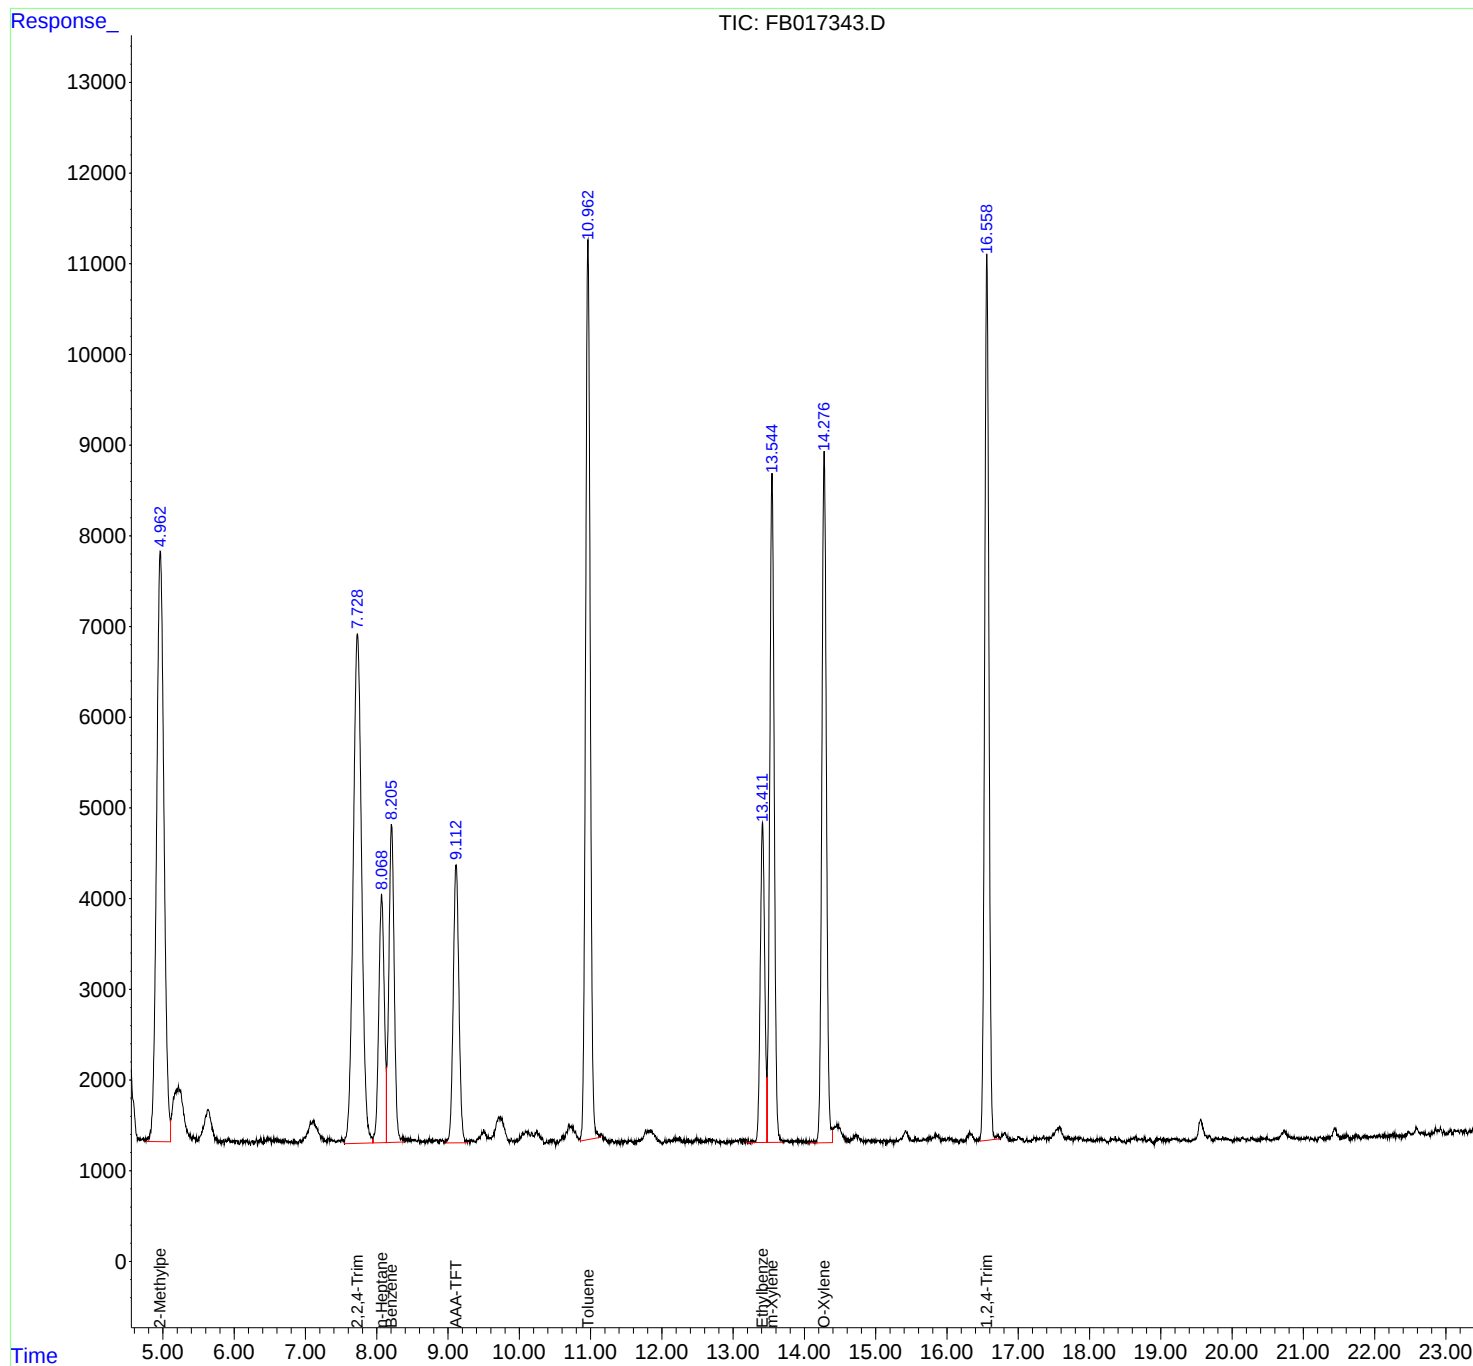

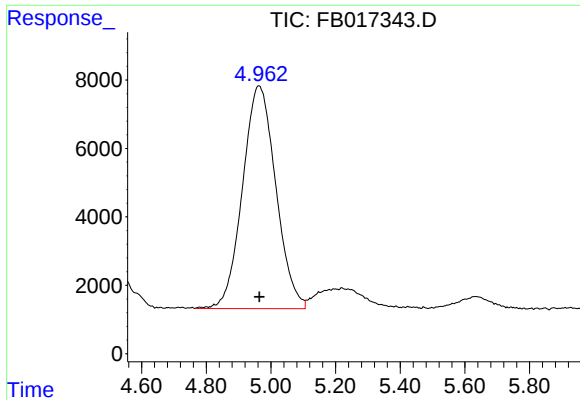


#1 2-Methylpentane

R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 465697
Conc: 27.23 ng/ml

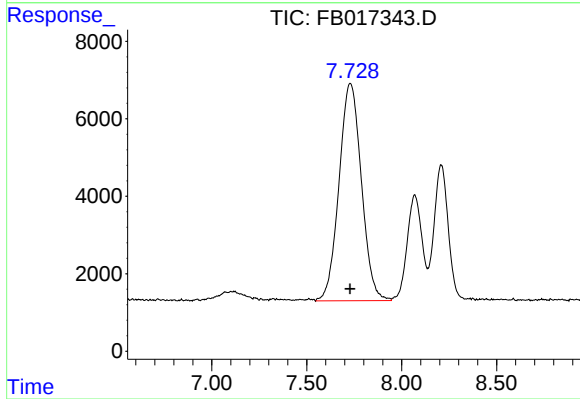


#2 2,2,4-Trimethylpentane

R.T.: 7.729 min
Delta R.T.: 0.000 min
Response: 459843
Conc: 27.22 ng/ml

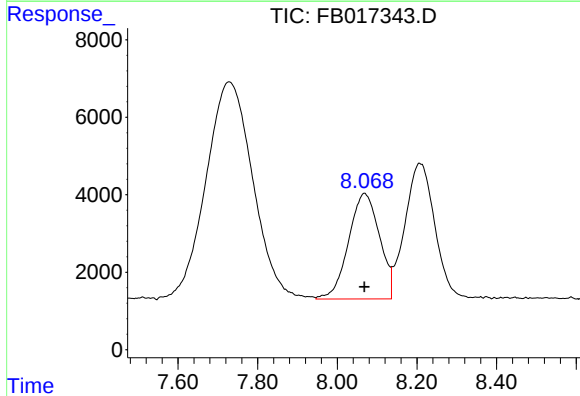


#3 n-Heptane

R.T.: 8.069 min
Delta R.T.: 0.000 min
Response: 146853
Conc: 9.12 ng/ml

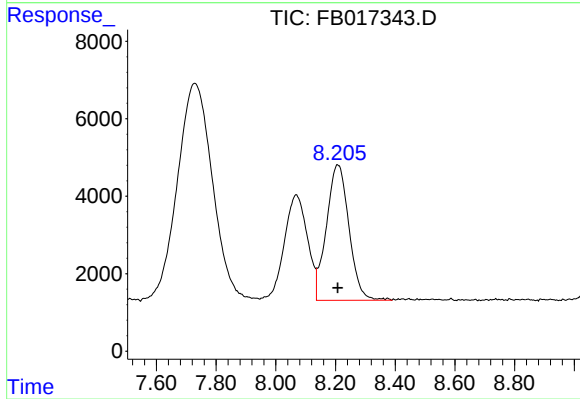


#4 Benzene

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 183789
Conc: 9.07 ng/ml

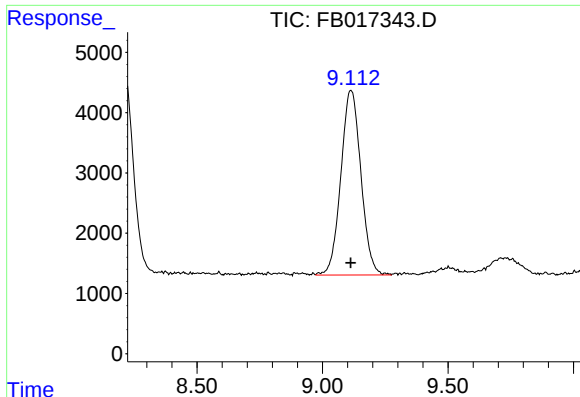


#5 AAA-TFT

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 169919
Conc: 18.14 ng/ml

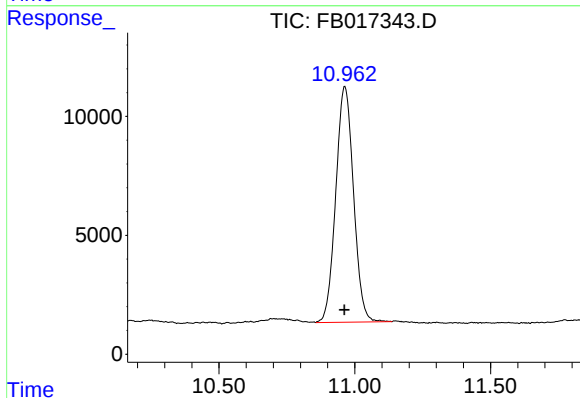


#6 Toluene

R.T.: 10.964 min
Delta R.T.: 0.002 min
Response: 450079
Conc: 27.30 ng/ml

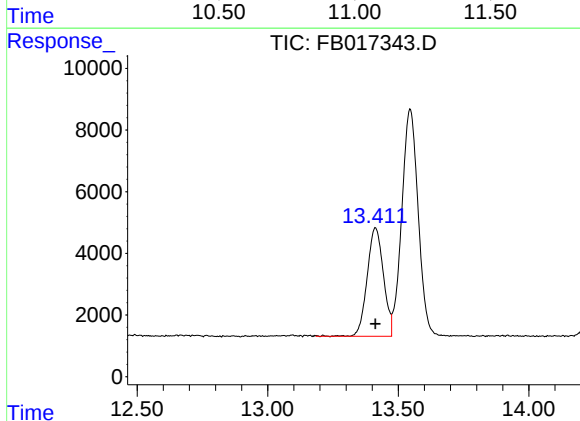


#7 Ethylbenzene

R.T.: 13.413 min
Delta R.T.: 0.000 min
Response: 151960
Conc: 9.11 ng/ml

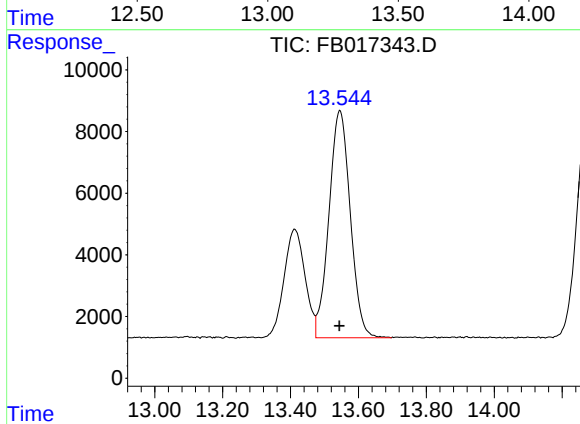


#8 m-Xylene

R.T.: 13.546 min
Delta R.T.: 0.001 min
Response: 321939
Conc: 17.17 ng/ml

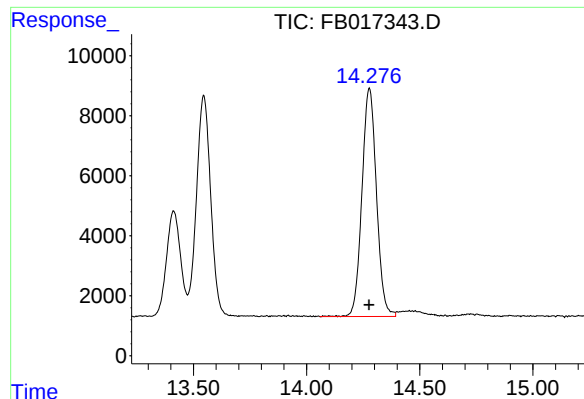

#9 O-Xylene

R.T.: 14.278 min
Delta R.T.: 0.001 min
Response: 339664
Conc: 16.71 ng/ml

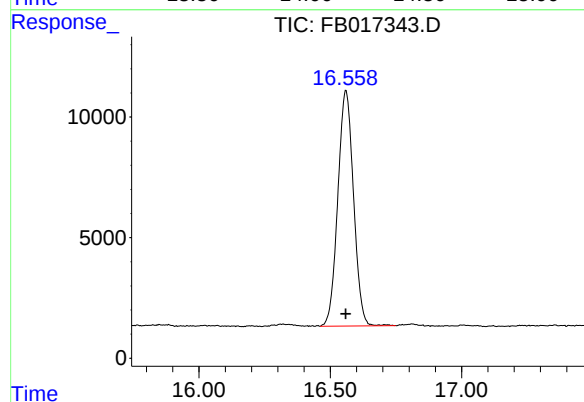

#10 1,2,4-Trimethylbenzene

R.T.: 16.560 min
Delta R.T.: 0.000 min
Response: 405430
Conc: 18.10 ng/ml