

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082725\
 Data File : FB032187.D
 Signal(s) : FID2B.CH
 Acq On : 27 Aug 2025 16:58
 Operator : YP/AJ
 Sample : BSF0827W1
 Misc : 5.00G/5.00ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0827W1

Integration File: Calibration.e
 Quant Time: Aug 28 02:38:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082125.M
 Quant Title :
 QLast Update : Thu Aug 21 10:58:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	333498	19.378 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	606500	26.492 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	728953	28.476 ng/ml
3) t n-Heptane	7.758	220905	8.975 ng/ml
4) t Benzene	7.897	282189	8.867 ng/ml
6) t Toluene	10.627	830232	25.313 ng/ml
7) t Ethylbenzene	13.063	239900	8.262 ng/ml
8) t m-Xylene	13.197	500637	16.722 ng/ml
9) t O-Xylene	13.924	480760	16.818 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	408634	15.720 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082725\
Data File : FB032187.D
Signal(s) : FID2B.CH
Acq On : 27 Aug 2025 16:58
Operator : YP/AJ
Sample : BSF0827W1
Misc : 5.00G/5.00ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0827W1

Integration File: Calibration.e
Quant Time: Aug 28 02:38:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082125.M
Quant Title :
QLast Update : Thu Aug 21 10:58:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

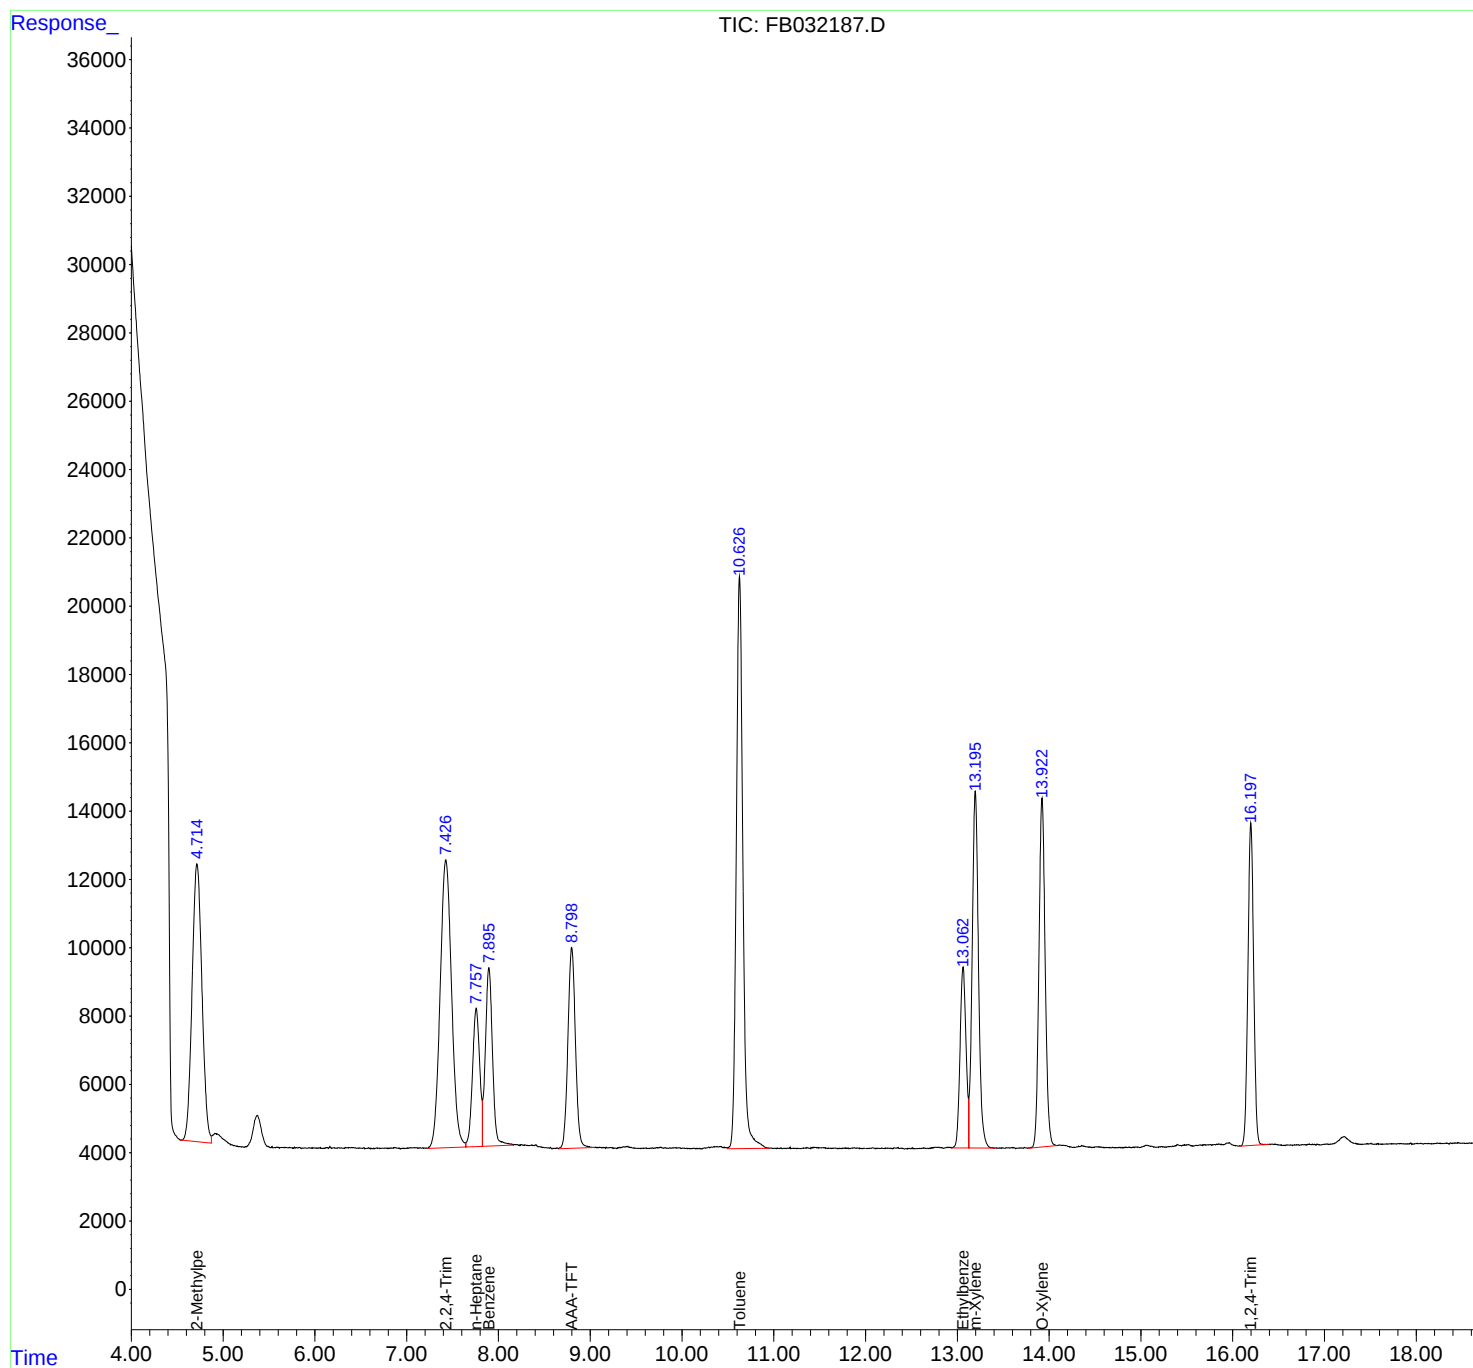


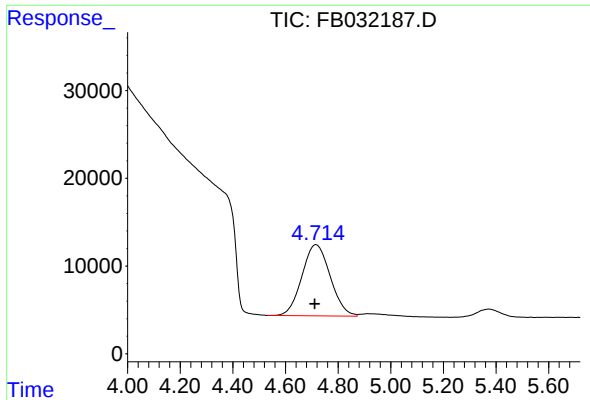

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: 0.005 min
Response: 606500
Conc: 26.49 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0827W1

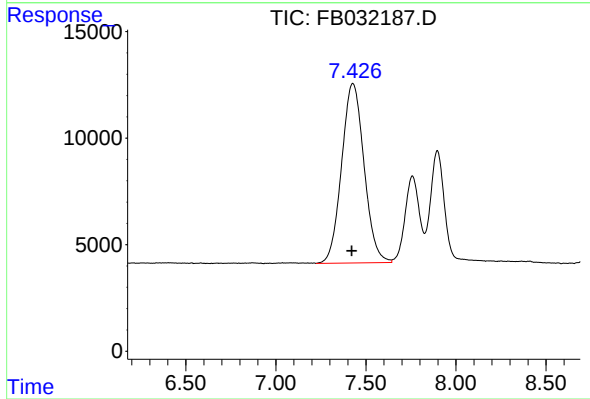


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.006 min
Response: 728953
Conc: 28.48 ng/ml

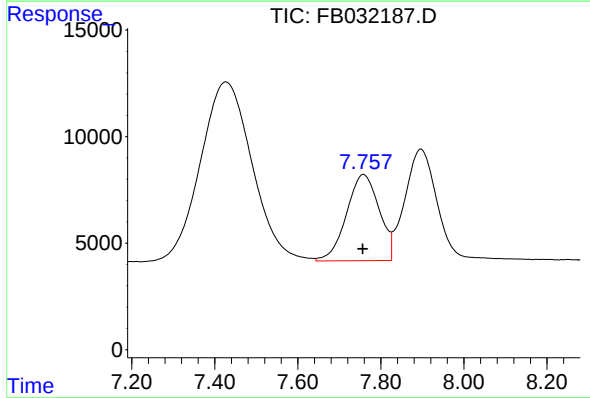


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.002 min
Response: 220905
Conc: 8.97 ng/ml

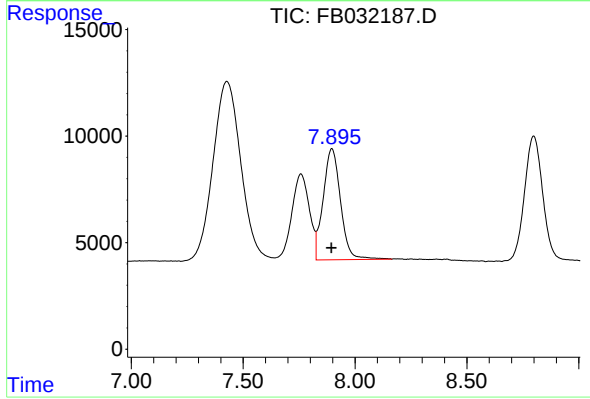

#4 Benzene


R.T.: 7.897 min
Delta R.T.: 0.002 min
Response: 282189
Conc: 8.87 ng/ml

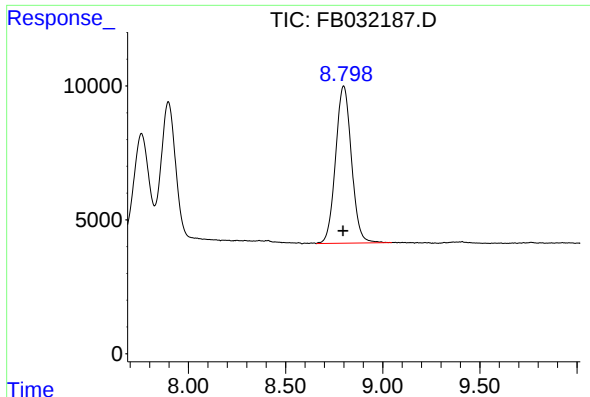

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.002 min
Response: 333498
Conc: 19.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0827W1

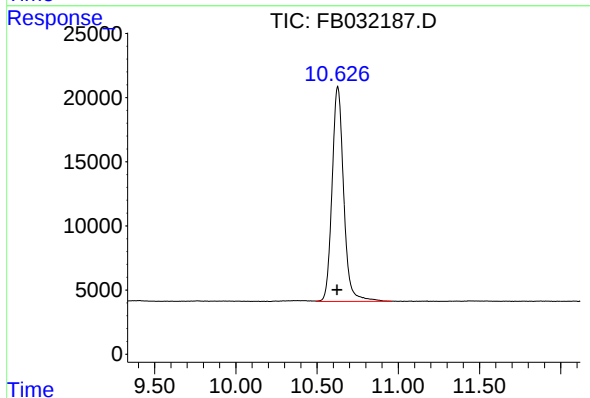


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.003 min
Response: 830232
Conc: 25.31 ng/ml

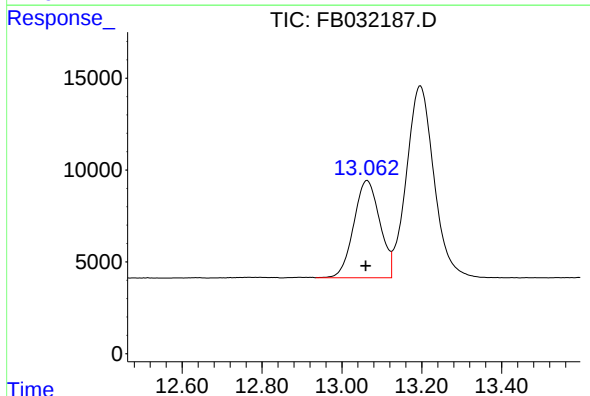


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.004 min
Response: 239900
Conc: 8.26 ng/ml

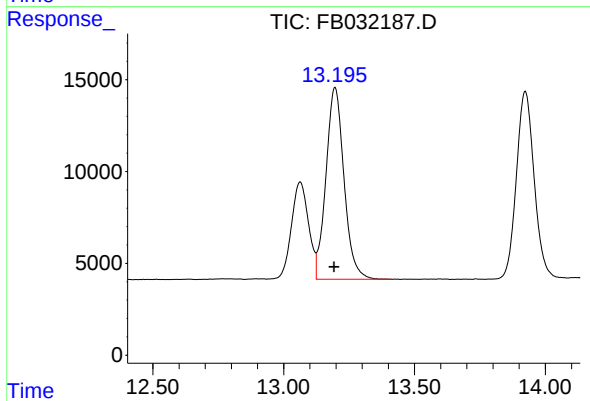

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.003 min
Response: 500637
Conc: 16.72 ng/ml

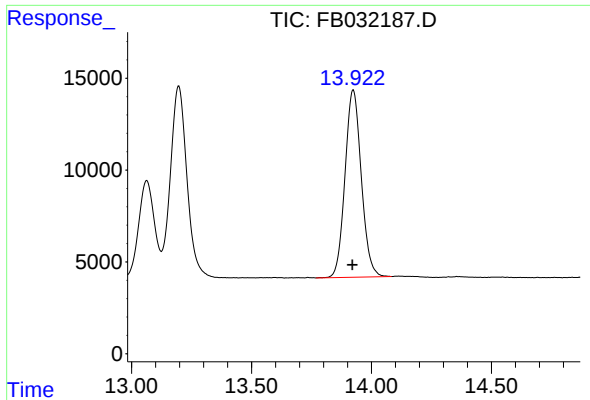

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.003 min
Response: 480760
Conc: 16.82 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0827W1

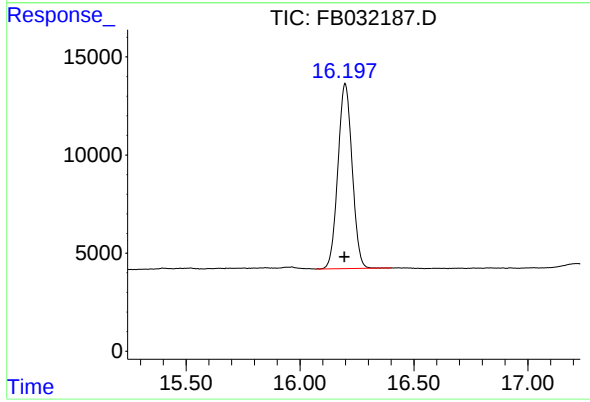

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.003 min
Response: 408634
Conc: 15.72 ng/ml