

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082919\
 Data File : FB022242.D
 Signal(s) : FID2B.CH
 Acq On : 29 Aug 2019 9:15
 Operator : DD/AJ
 Sample : BSF0829S1
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0829S1

Integration File: Calibration.e
 Quant Time: Aug 30 00:13:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.983	441333	20.778 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.851	1252010	31.283 ng/ml
2) t 2,2,4-Trimethylpentane	7.601	1278705	31.747 ng/ml
3) t n-Heptane	7.941	402684	10.542 ng/ml
4) t Benzene	8.076	457822	10.198 ng/ml
6) t Toluene	10.824	936153	30.452 ng/ml
7) t Ethylbenzene	13.270	219033	10.733 ng/ml
8) t m-Xylene	13.403	453812	21.548 ng/ml
9) t O-Xylene	14.132	474643	21.222 ng/ml
10) t 1,2,4-Trimethylbenzene	16.411	534268	20.832 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082919\
Data File : FB022242.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2019 9:15
Operator : DD/AJ
Sample : BSF0829S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0829S1

Integration File: Calibration.e
Quant Time: Aug 30 00:13:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

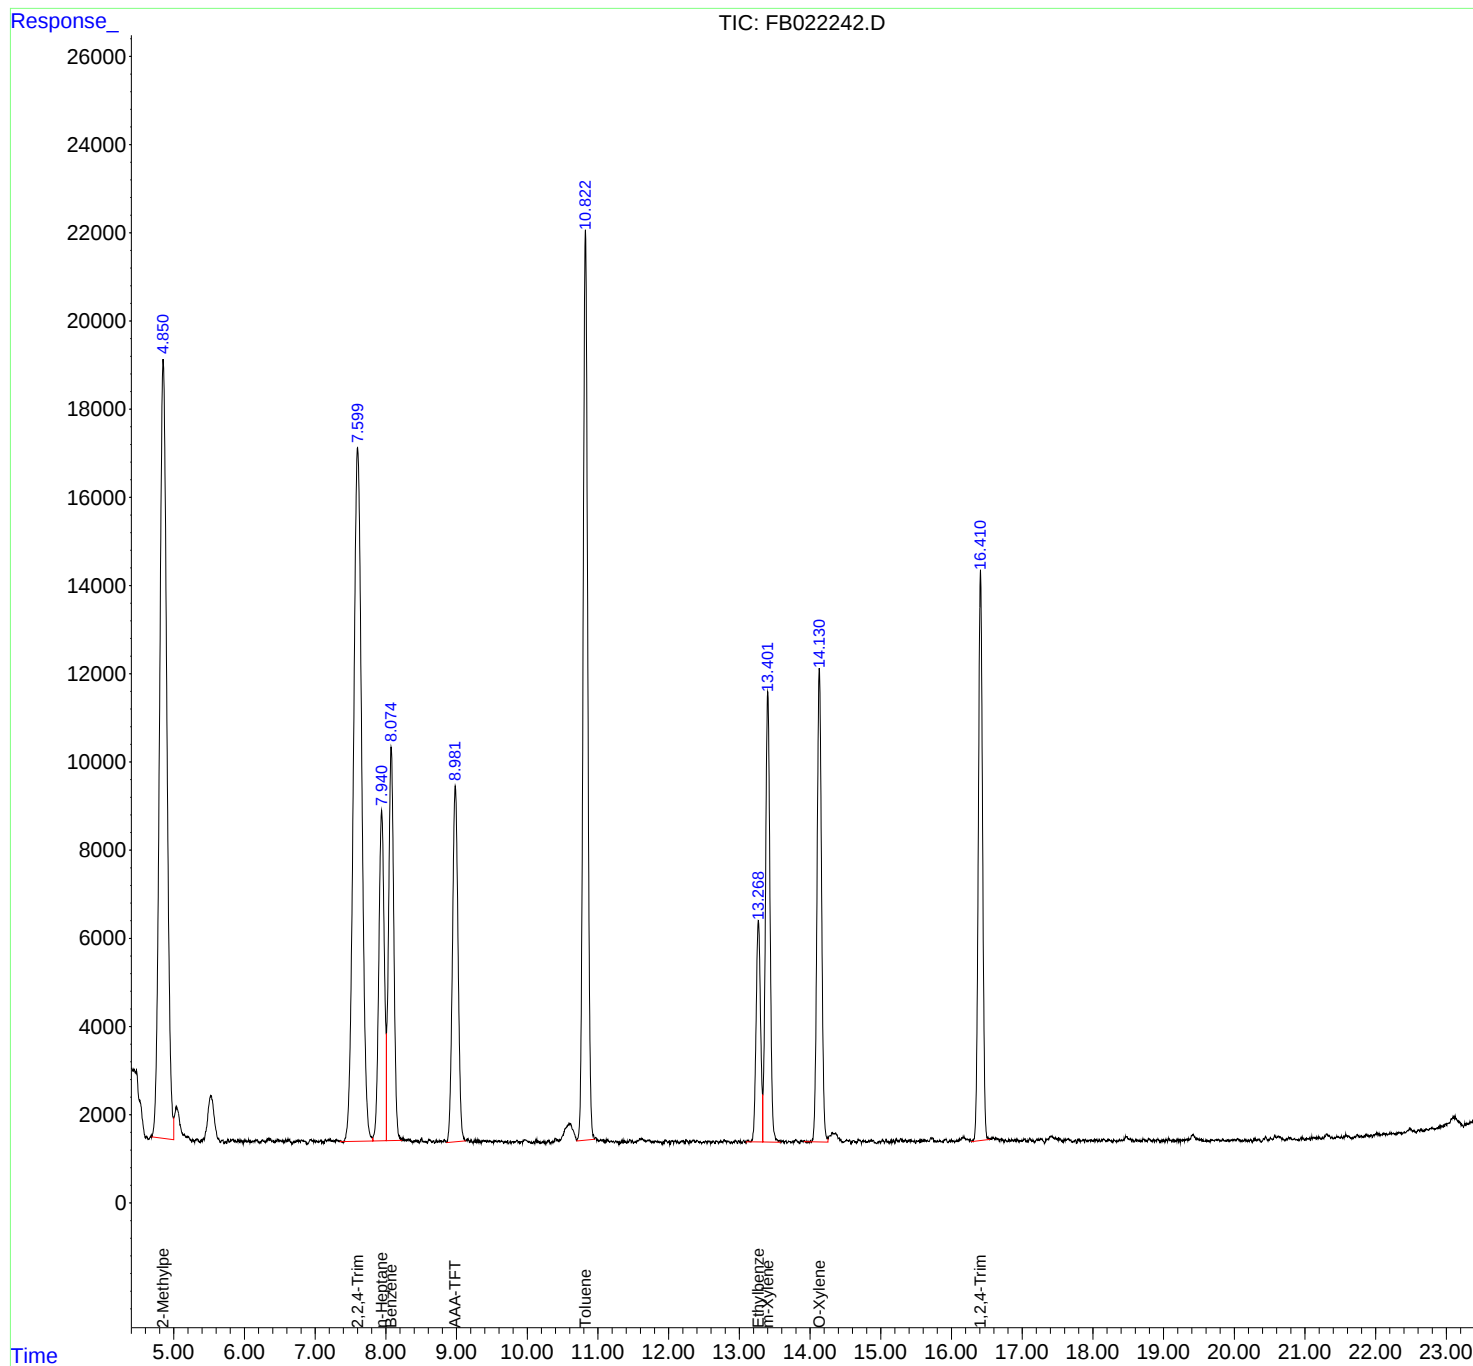


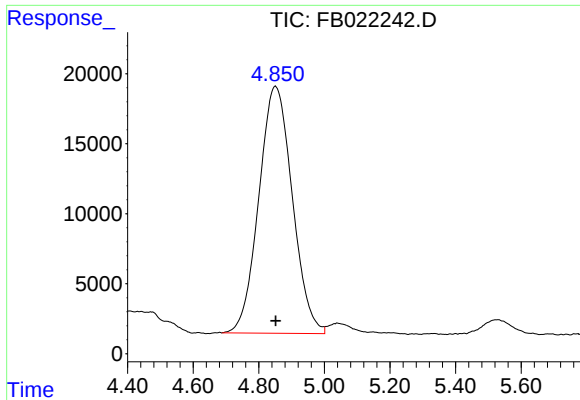

#1 2-Methylpentane


R.T.: 4.851 min
Delta R.T.: 0.000 min
Response: 1252010
Conc: 31.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0829S1

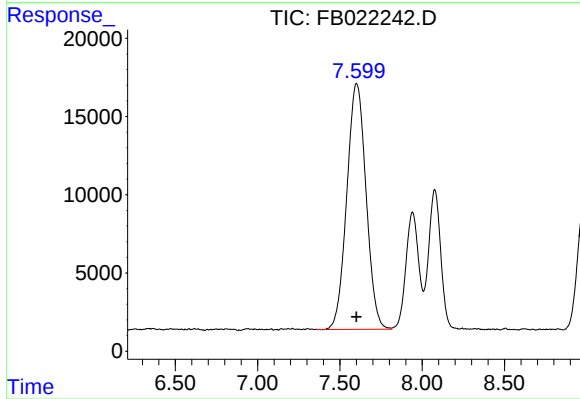


#2 2,2,4-Trimethylpentane

R.T.: 7.601 min
Delta R.T.: 0.001 min
Response: 1278705
Conc: 31.75 ng/ml

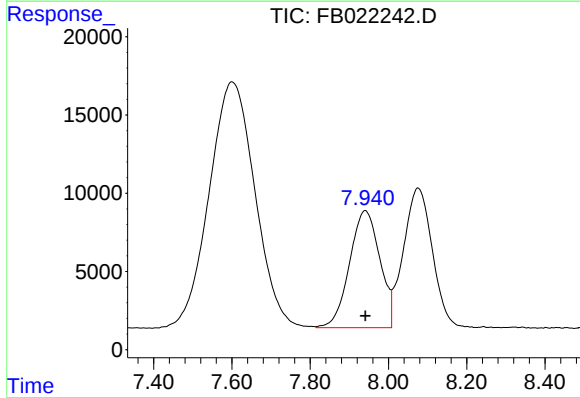


#3 n-Heptane

R.T.: 7.941 min
Delta R.T.: 0.000 min
Response: 402684
Conc: 10.54 ng/ml

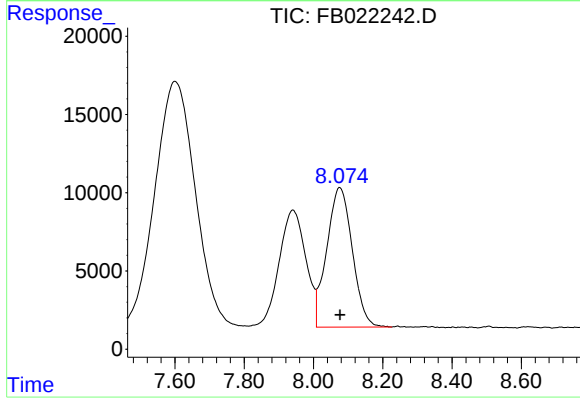

#4 Benzene


R.T.: 8.076 min
Delta R.T.: 0.000 min
Response: 457822
Conc: 10.20 ng/ml

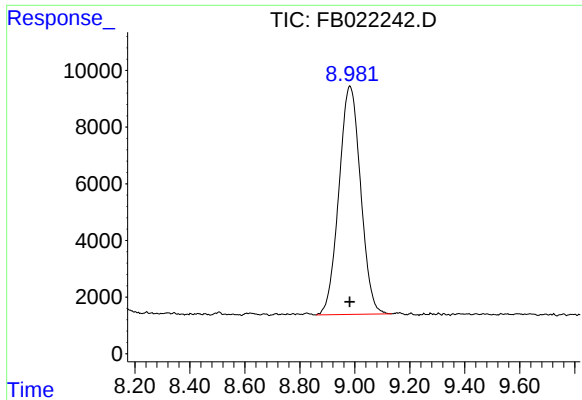

#5 AAA-TFT


R.T.: 8.983 min
Delta R.T.: 0.000 min
Response: 441333
Conc: 20.78 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0829S1

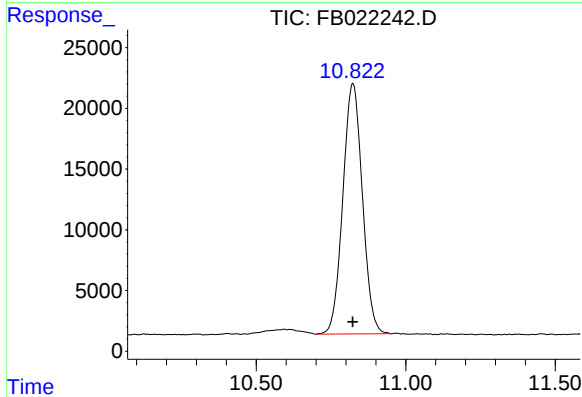


#6 Toluene

R.T.: 10.824 min
Delta R.T.: 0.000 min
Response: 936153
Conc: 30.45 ng/ml

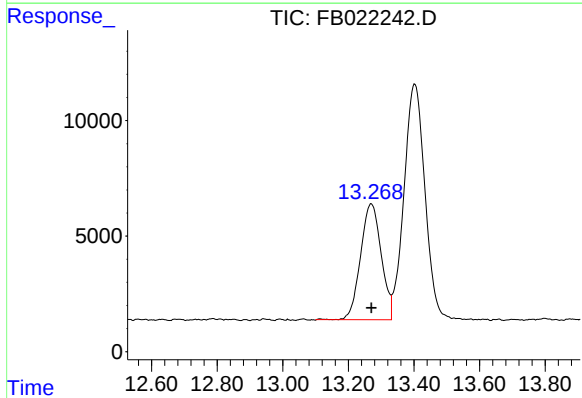


#7 Ethylbenzene

R.T.: 13.270 min
Delta R.T.: 0.000 min
Response: 219033
Conc: 10.73 ng/ml

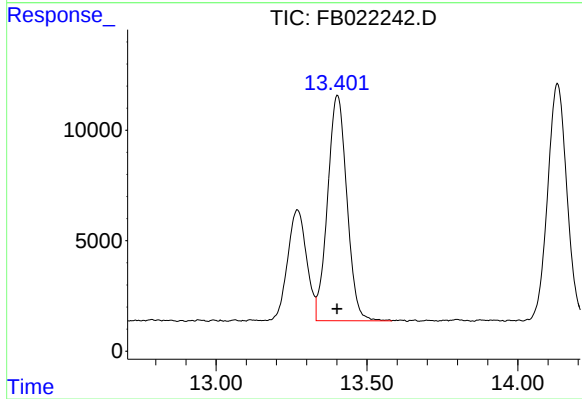

#8 m-Xylene


R.T.: 13.403 min
Delta R.T.: 0.000 min
Response: 453812
Conc: 21.55 ng/ml

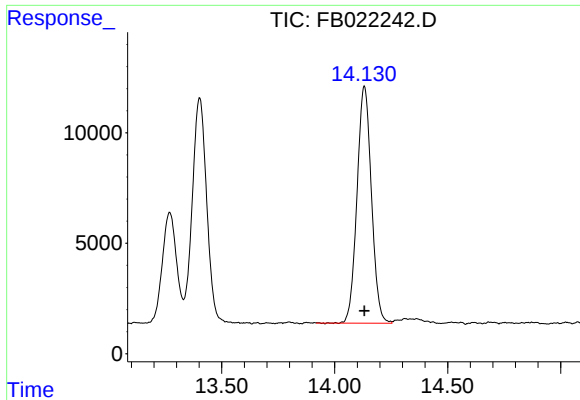

#9 O-Xylene

R.T.: 14.132 min
Delta R.T.: 0.000 min
Response: 474643
Conc: 21.22 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0829S1

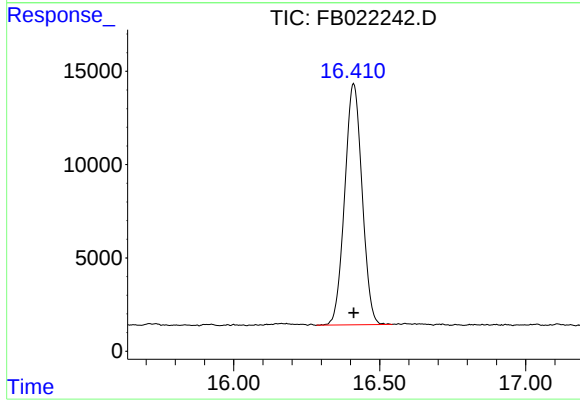

#10 1,2,4-Trimethylbenzene

R.T.: 16.411 min
Delta R.T.: 0.000 min
Response: 534268
Conc: 20.83 ng/ml