

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082919\
 Data File : FB022246.D
 Signal(s) : FID2B.CH
 Acq On : 29 Aug 2019 11:54
 Operator : DD/AJ
 Sample : K4554-01
 Misc : 5.06/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-13-(0-2)

Integration File: Calibration.e
 Quant Time: Aug 30 00:14:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.983	461431	21.724 ng/ml
Target Compounds			
3) t n-Heptane	7.927	792	0.021 ng/ml
8) t m-Xylene	13.408	1386	0.066 ng/ml
9) t O-Xylene	14.072	937	0.042 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082919\
Data File : FB022246.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2019 11:54
Operator : DD/AJ
Sample : K4554-01
Misc : 5.06/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-13-(0-2)

Integration File: Calibration.e
Quant Time: Aug 30 00:14:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

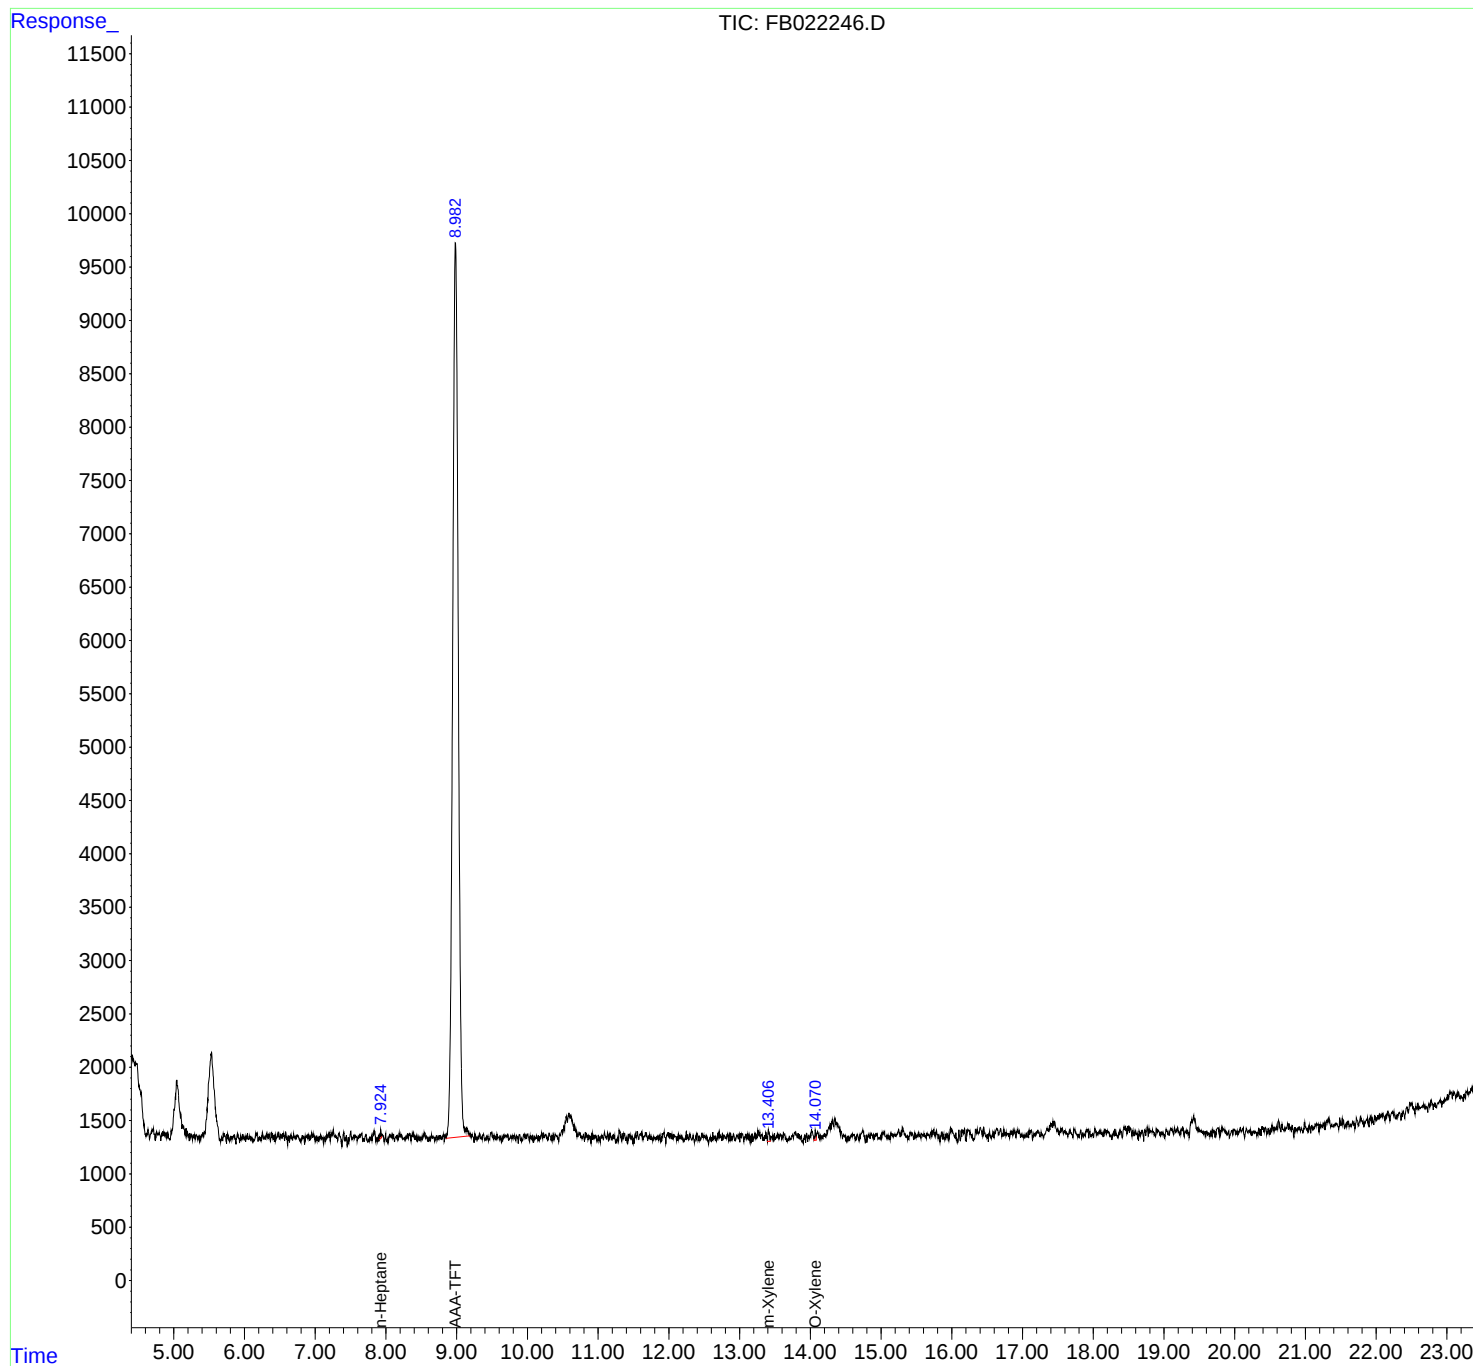


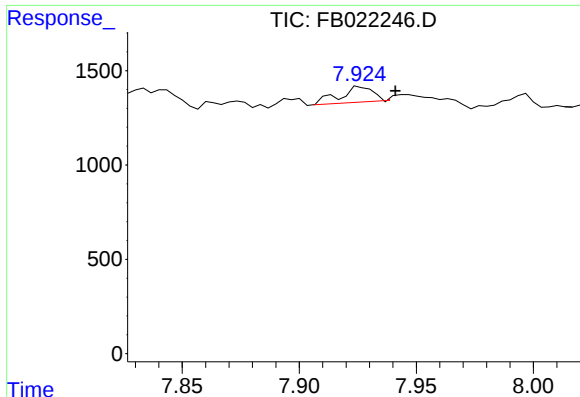

#3 n-Heptane


R.T.: 7.927 min
Delta R.T.: -0.014 min
Response: 792
Conc: 0.02 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-13-(0-2)

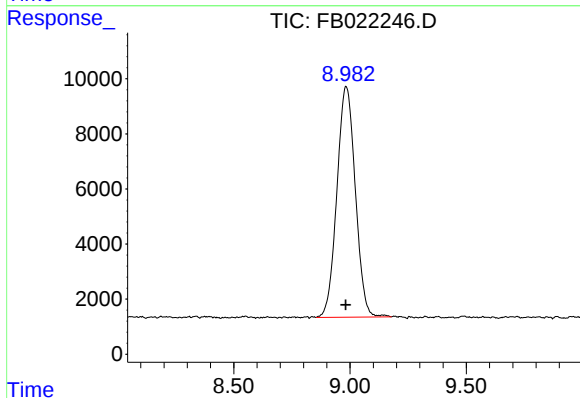


#5 AAA-TFT

R.T.: 8.983 min
Delta R.T.: 0.001 min
Response: 461431
Conc: 21.72 ng/ml

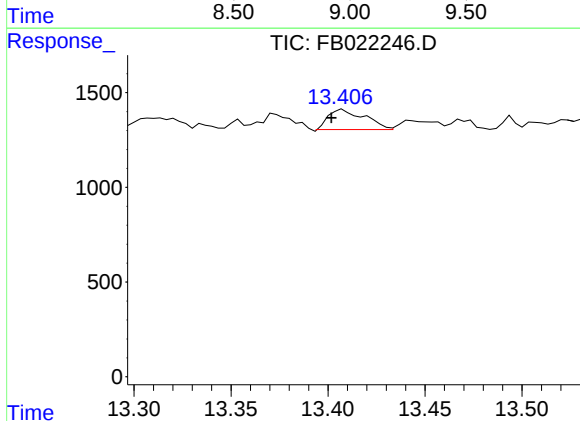

#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: 0.006 min
Response: 1386
Conc: 0.07 ng/ml

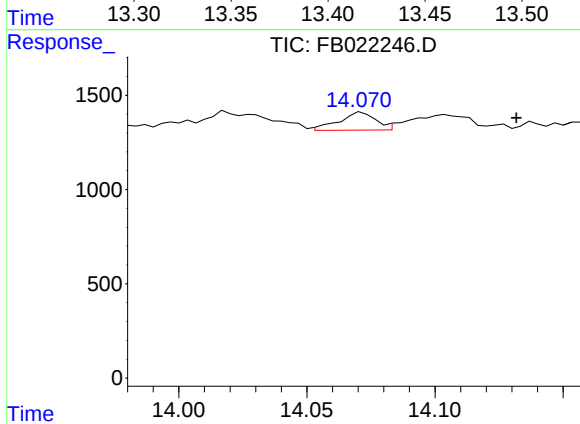

#9 O-Xylene

R.T.: 14.072 min
Delta R.T.: -0.060 min
Response: 937
Conc: 0.04 ng/ml