

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082919\
 Data File : FB022250.D
 Signal(s) : FID2B.CH
 Acq On : 29 Aug 2019 13:56
 Operator : DD/AJ
 Sample : K4439-03MS
 Misc : 5.07/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 S-2-(1-3)MS

Integration File: Calibration.e
 Quant Time: Aug 30 00:14:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.988	325732	15.336 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.858	717989	17.940 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	698945	17.353 ng/ml
3) t n-Heptane	7.949	150869	3.950 ng/ml
4) t Benzene	8.083	346501	7.718 ng/ml
6) t Toluene	10.829	615464	20.020 ng/ml
7) t Ethylbenzene	13.275	143740	7.044 ng/ml
8) t m-Xylene	13.408	294453	13.981 ng/ml
9) t O-Xylene	14.137	328206	14.675 ng/ml
10) t 1,2,4-Trimethylbenzene	16.416	334732	13.052 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082919\
Data File : FB022250.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2019 13:56
Operator : DD/AJ
Sample : K4439-03MS
Misc : 5.07/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
S-2-(1-3)MS

Integration File: Calibration.e
Quant Time: Aug 30 00:14:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

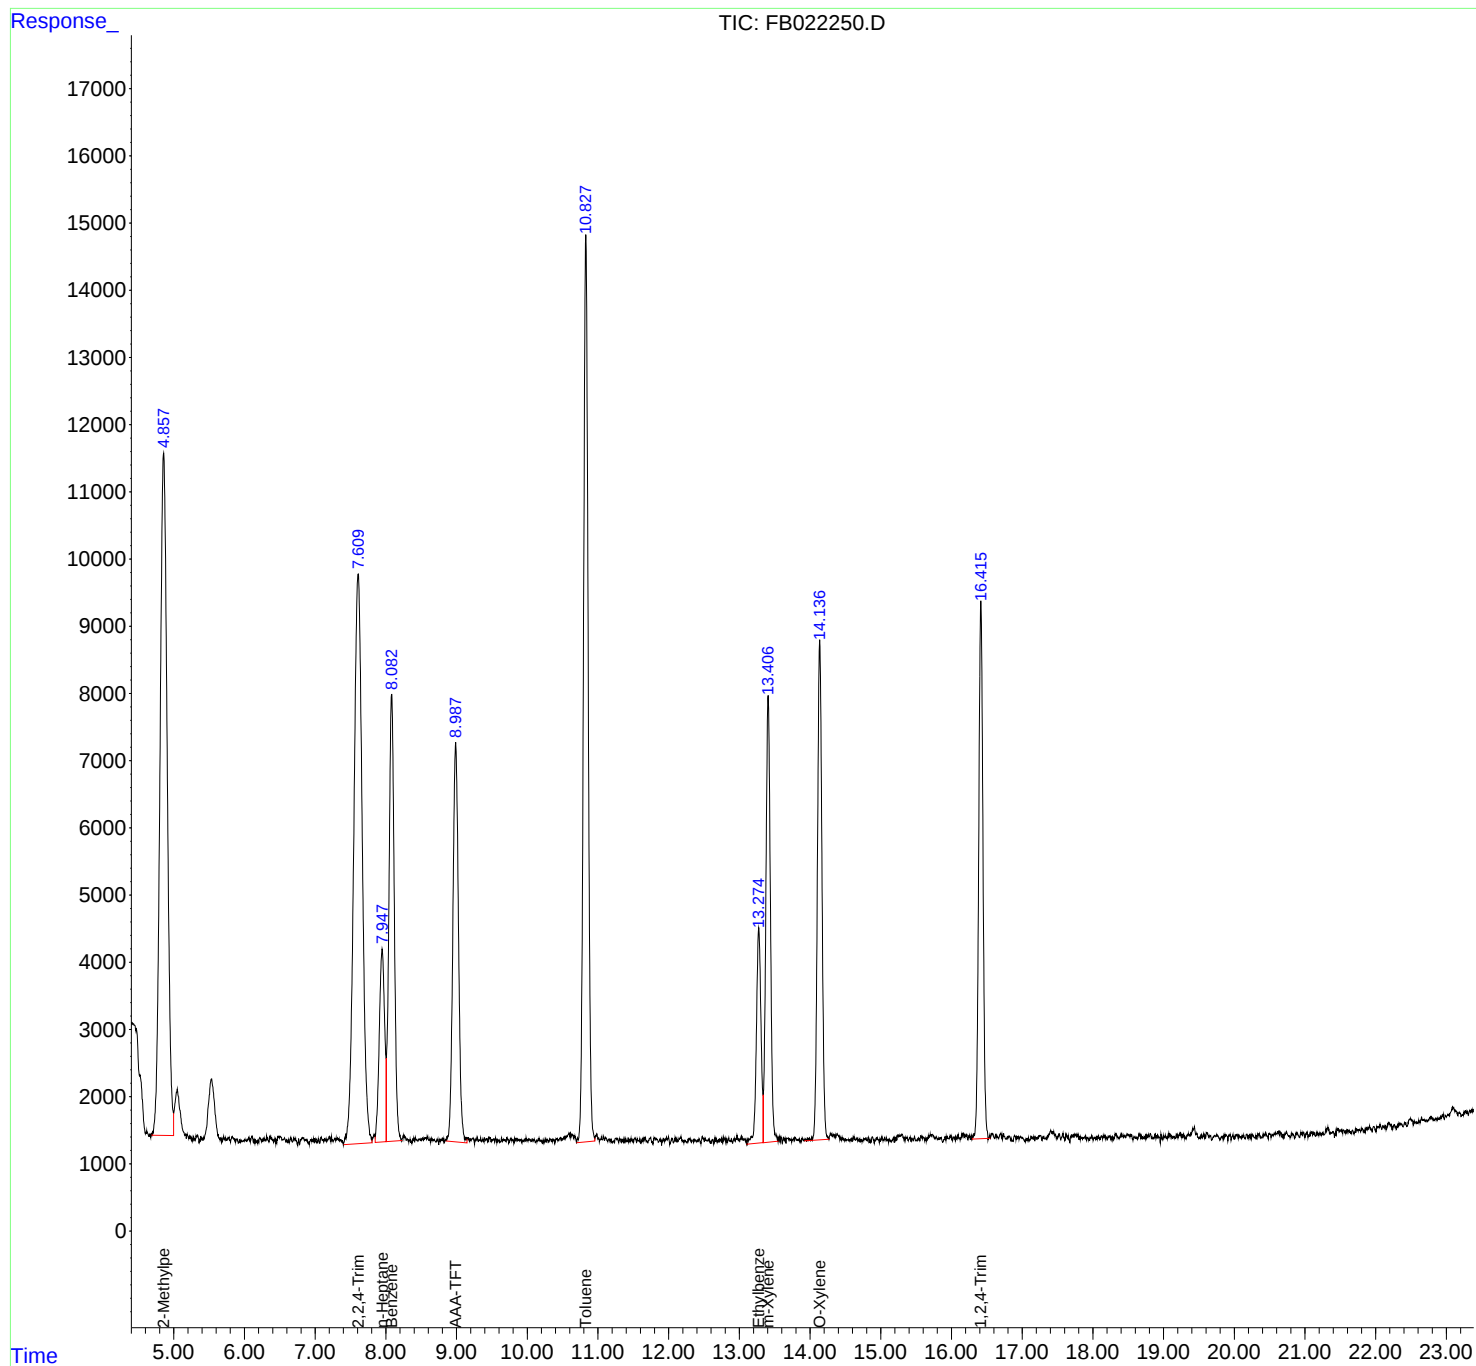


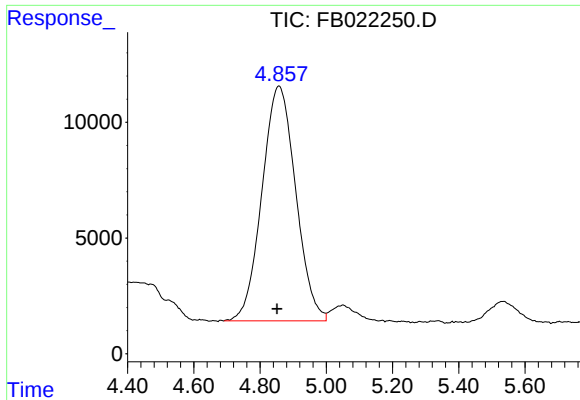

#1 2-Methylpentane


R.T.: 4.858 min
Delta R.T.: 0.006 min
Response: 717989
Conc: 17.94 ng/ml

Instrument :
FID_B
ClientSampleId :
S-2-(1-3)MS

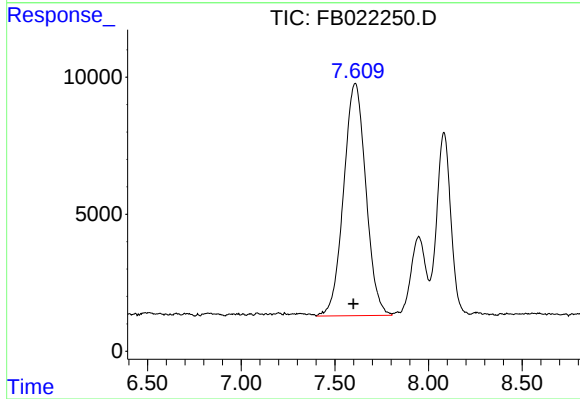


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: 0.010 min
Response: 698945
Conc: 17.35 ng/ml

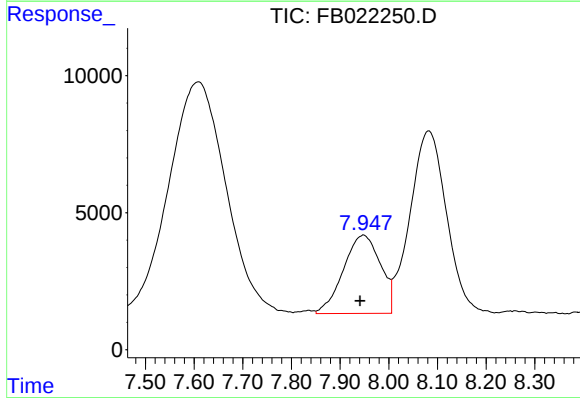


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: 0.008 min
Response: 150869
Conc: 3.95 ng/ml

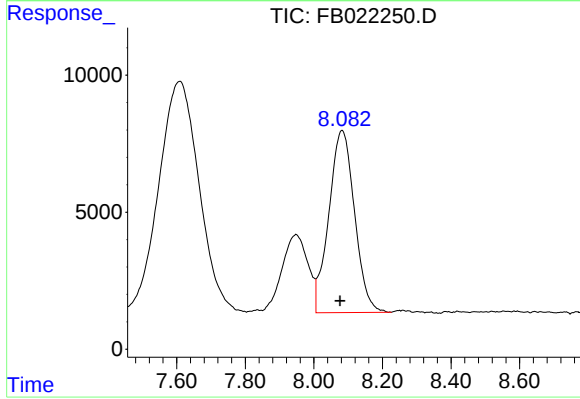

#4 Benzene


R.T.: 8.083 min
Delta R.T.: 0.006 min
Response: 346501
Conc: 7.72 ng/ml

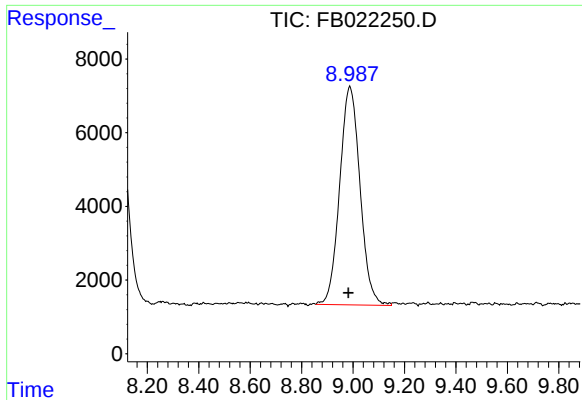

#5 AAA-TFT


R.T.: 8.988 min
Delta R.T.: 0.006 min
Response: 325732
Conc: 15.34 ng/ml

Instrument :
FID_B
ClientSampleId :
S-2-(1-3)MS

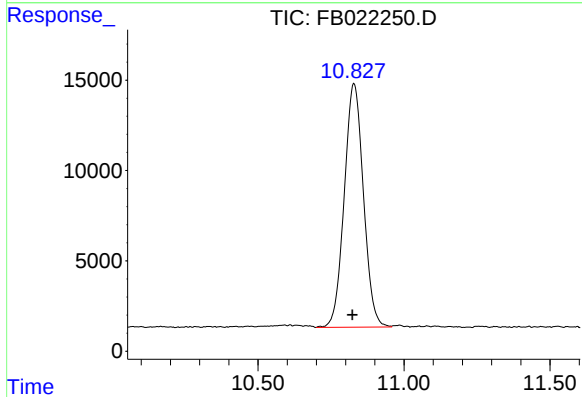


#6 Toluene

R.T.: 10.829 min
Delta R.T.: 0.006 min
Response: 615464
Conc: 20.02 ng/ml

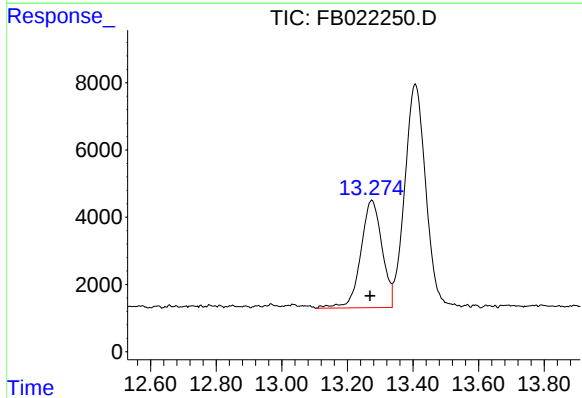


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: 0.005 min
Response: 143740
Conc: 7.04 ng/ml

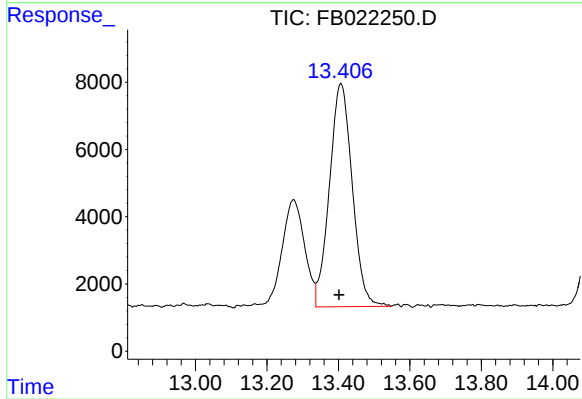

#8 m-Xylene


R.T.: 13.408 min
Delta R.T.: 0.006 min
Response: 294453
Conc: 13.98 ng/ml

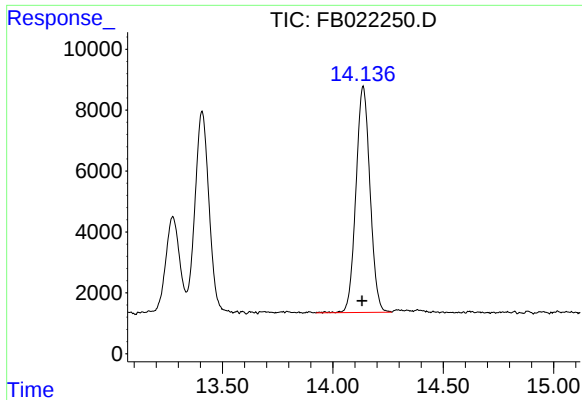

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: 0.005 min
Response: 328206
Conc: 14.67 ng/ml

Instrument :
FID_B
ClientSampleId :
S-2-(1-3)MS

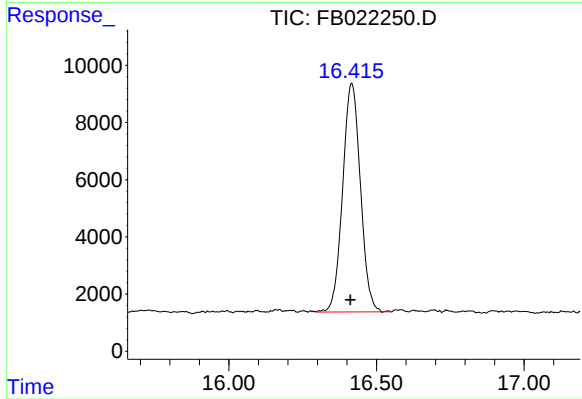

#10 1,2,4-Trimethylbenzene

R.T.: 16.416 min
Delta R.T.: 0.005 min
Response: 334732
Conc: 13.05 ng/ml