

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082919\  
Data File : FB022252.D  
Signal(s) : FID2B.CH  
Acq On : 29 Aug 2019 14:58  
Operator : DD/AJ  
Sample : K4596-01  
Misc : 5.02/5.00ml DI WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
S403-K1-1.0-1.5-082819

Integration File: Calibration.e  
Quant Time: Aug 30 00:15:21 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB082019.M  
Quant Title :  
QLast Update : Wed Aug 21 07:59:08 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 5) s AAA-TFT                | 8.989  | 455030   | 21.423 ng/ml |
|                             |        |          |              |
| Target Compounds            |        |          |              |
| 9) t O-Xylene               | 14.181 | 17523    | 0.783 ng/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082919\  
Data File : FB022252.D  
Signal(s) : FID2B.CH  
Acq On : 29 Aug 2019 14:58  
Operator : DD/AJ  
Sample : K4596-01  
Misc : 5.02/5.00ml DI WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
S403-K1-1.0-1.5-082819

Integration File: Calibration.e  
Quant Time: Aug 30 00:15:21 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB082019.M  
Quant Title :  
QLast Update : Wed Aug 21 07:59:08 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

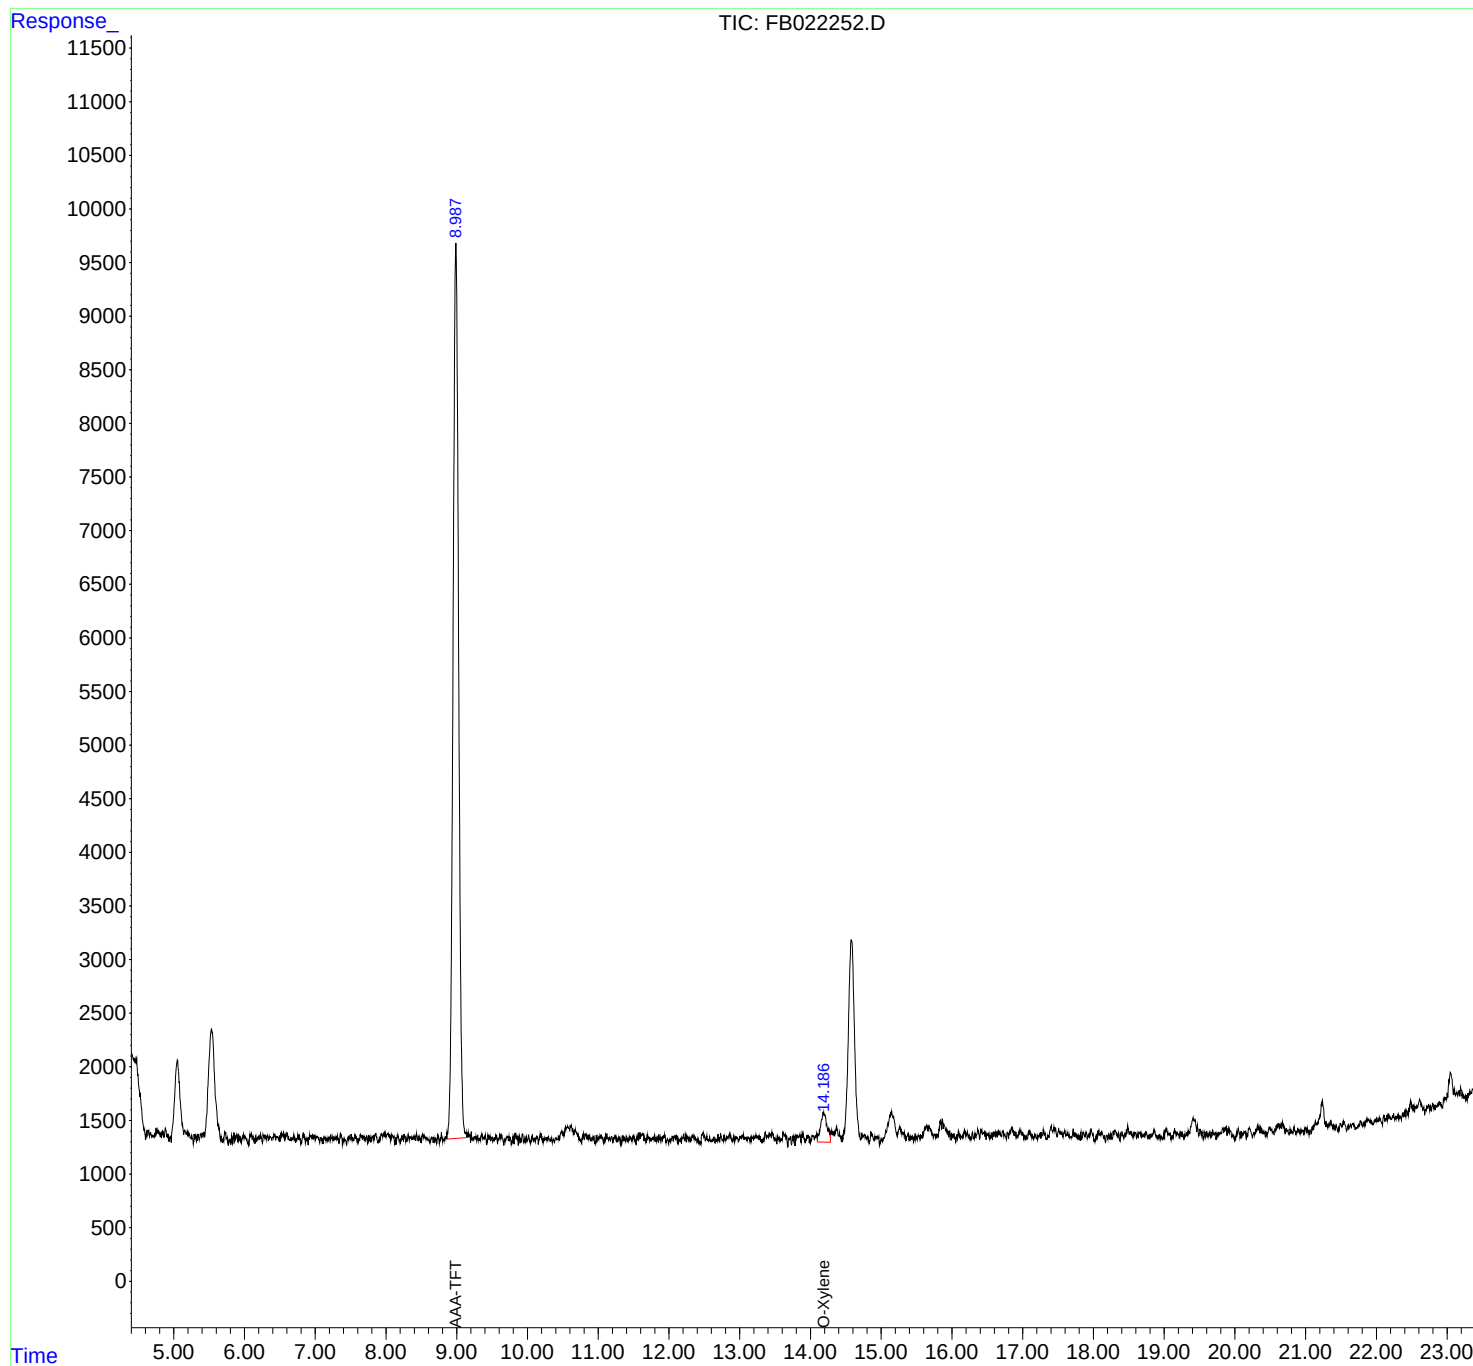


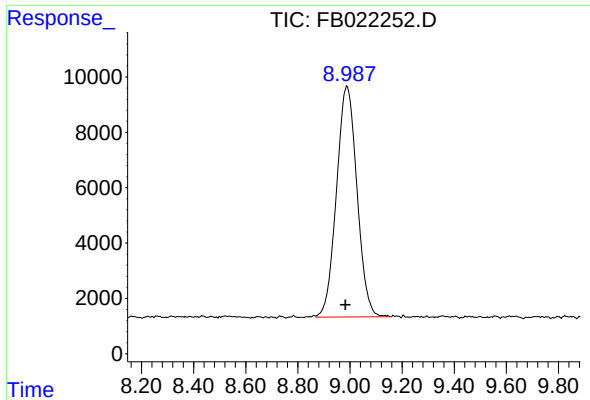

#5 AAA-TFT

R.T.: 8.989 min  
Delta R.T.: 0.007 min  
Response: 455030  
Conc: 21.42 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
S403-K1-1.0-1.5-082819

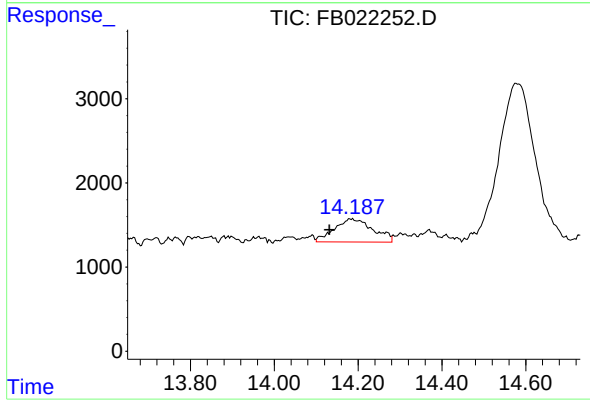

#9 O-Xylene

R.T.: 14.181 min  
Delta R.T.: 0.049 min  
Response: 17523  
Conc: 0.78 ng/ml