

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082919\
Data File : FB022245.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2019 11:23
Operator : DD/AJ
Sample : K4095-14
Misc : 5.04/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SU-01-082819-1

Integration File: Calibration.e
Quant Time: Aug 30 00:14:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.983	442482	20.832 ng/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082919\
Data File : FB022245.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2019 11:23
Operator : DD/AJ
Sample : K4095-14
Misc : 5.04/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SU-01-082819-1

Integration File: Calibration.e
Quant Time: Aug 30 00:14:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

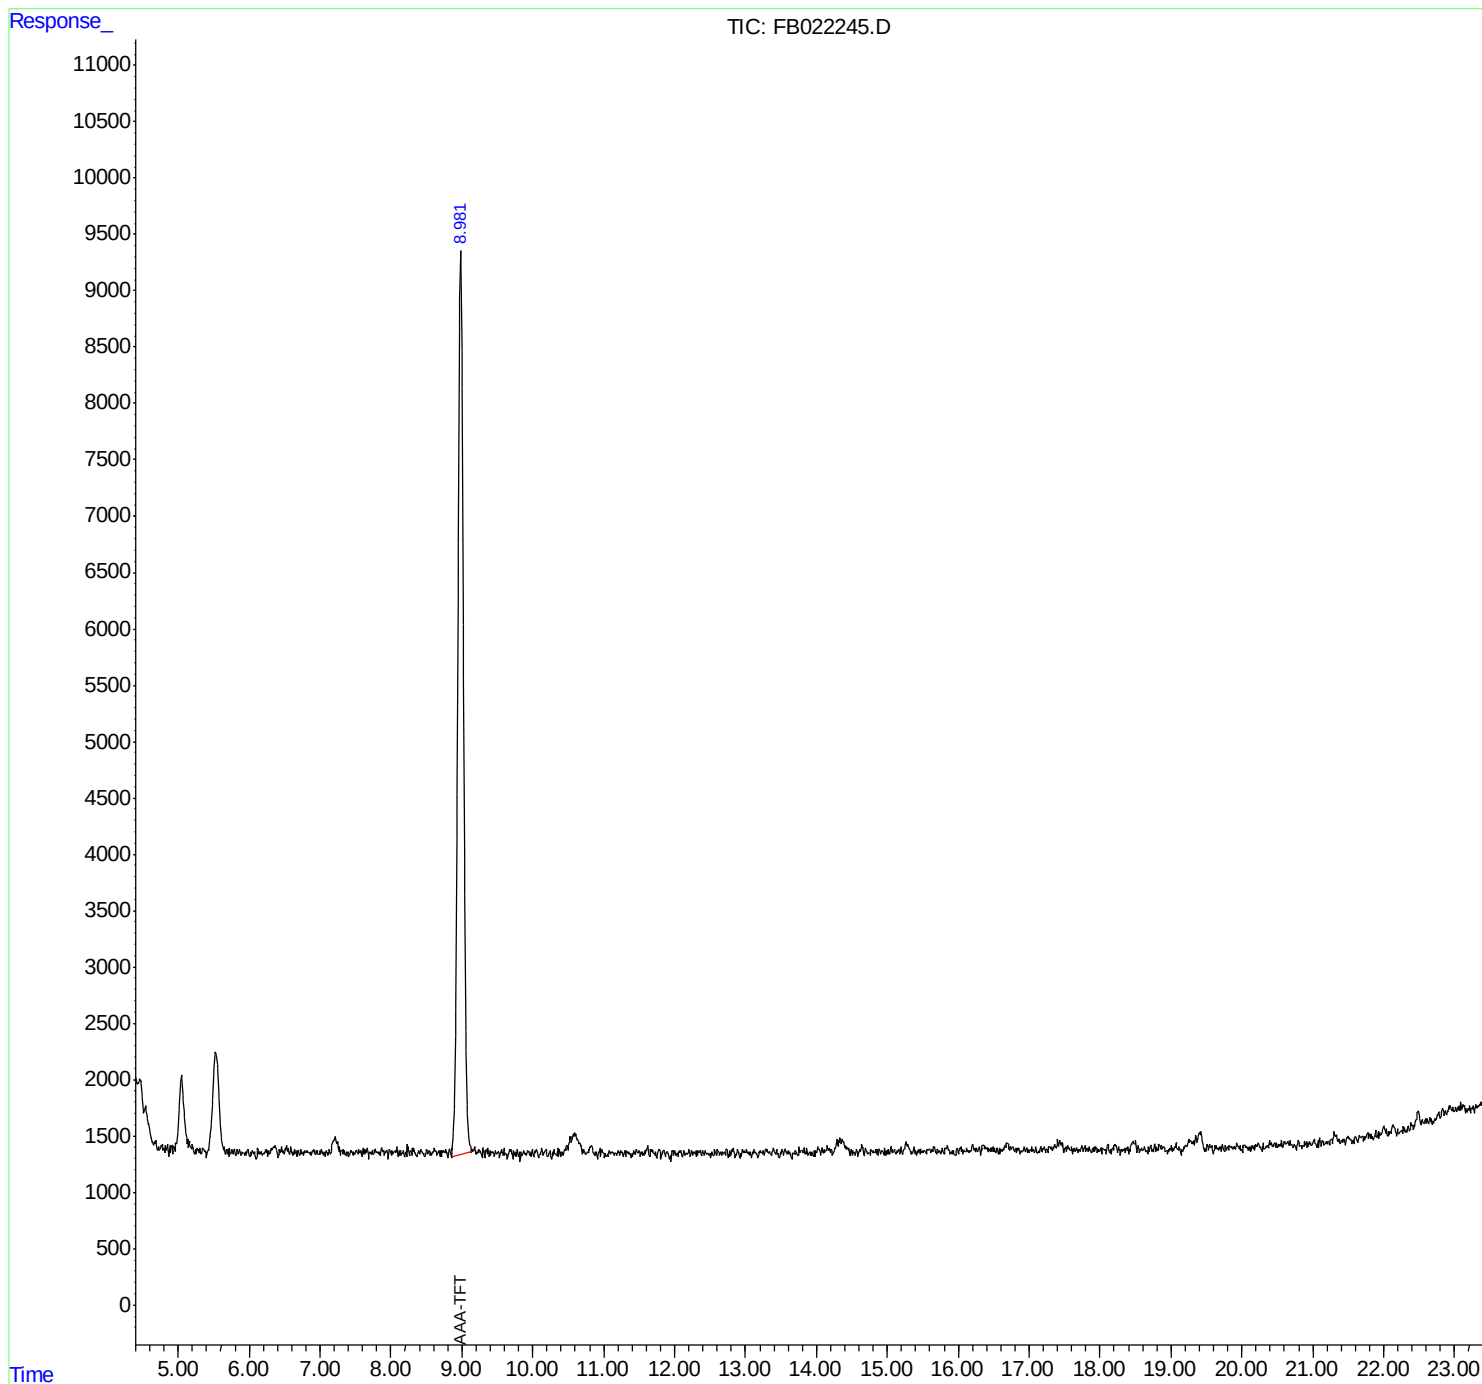

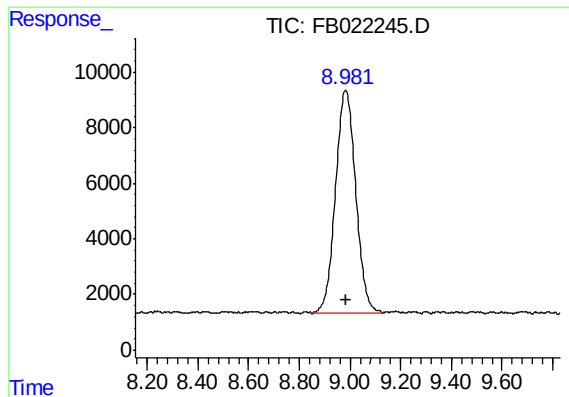

#5 AAA-TFT

R.T.: 8.983 min
Delta R.T.: 0.000 min
Response: 442482
Conc: 20.83 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-01-082819-1