

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091218\
 Data File : FB017689.D
 Signal(s) : FID2B.CH
 Acq On : 12 Sep 2018 10:20
 Operator : MJ/SJ
 Sample : BSF0912S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 13 09:20:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.107	176962	21.464 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.959	290713	20.747 ng/ml
2) t	2,2,4-Trimethylpentane	7.724	354067	25.125 ng/ml
3) t	n-Heptane	8.065	87009	6.313 ng/ml
4) t	Benzene	8.204	156907	8.900 ng/ml
6) t	Toluene	10.958	394484	27.422 ng/ml
7) t	Ethylbenzene	13.406	146396	9.927 ng/ml
8) t	m-Xylene	13.541	309932	19.937 ng/ml
9) t	O-Xylene	14.272	335219	20.421 ng/ml
10) t	1,2,4-Trimethylbenzene	16.554	388133	19.928 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091218\
Data File : FB017689.D
Signal(s) : FID2B.CH
Acq On : 12 Sep 2018 10:20
Operator : MJ/SJ
Sample : BSF0912S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 13 09:20:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

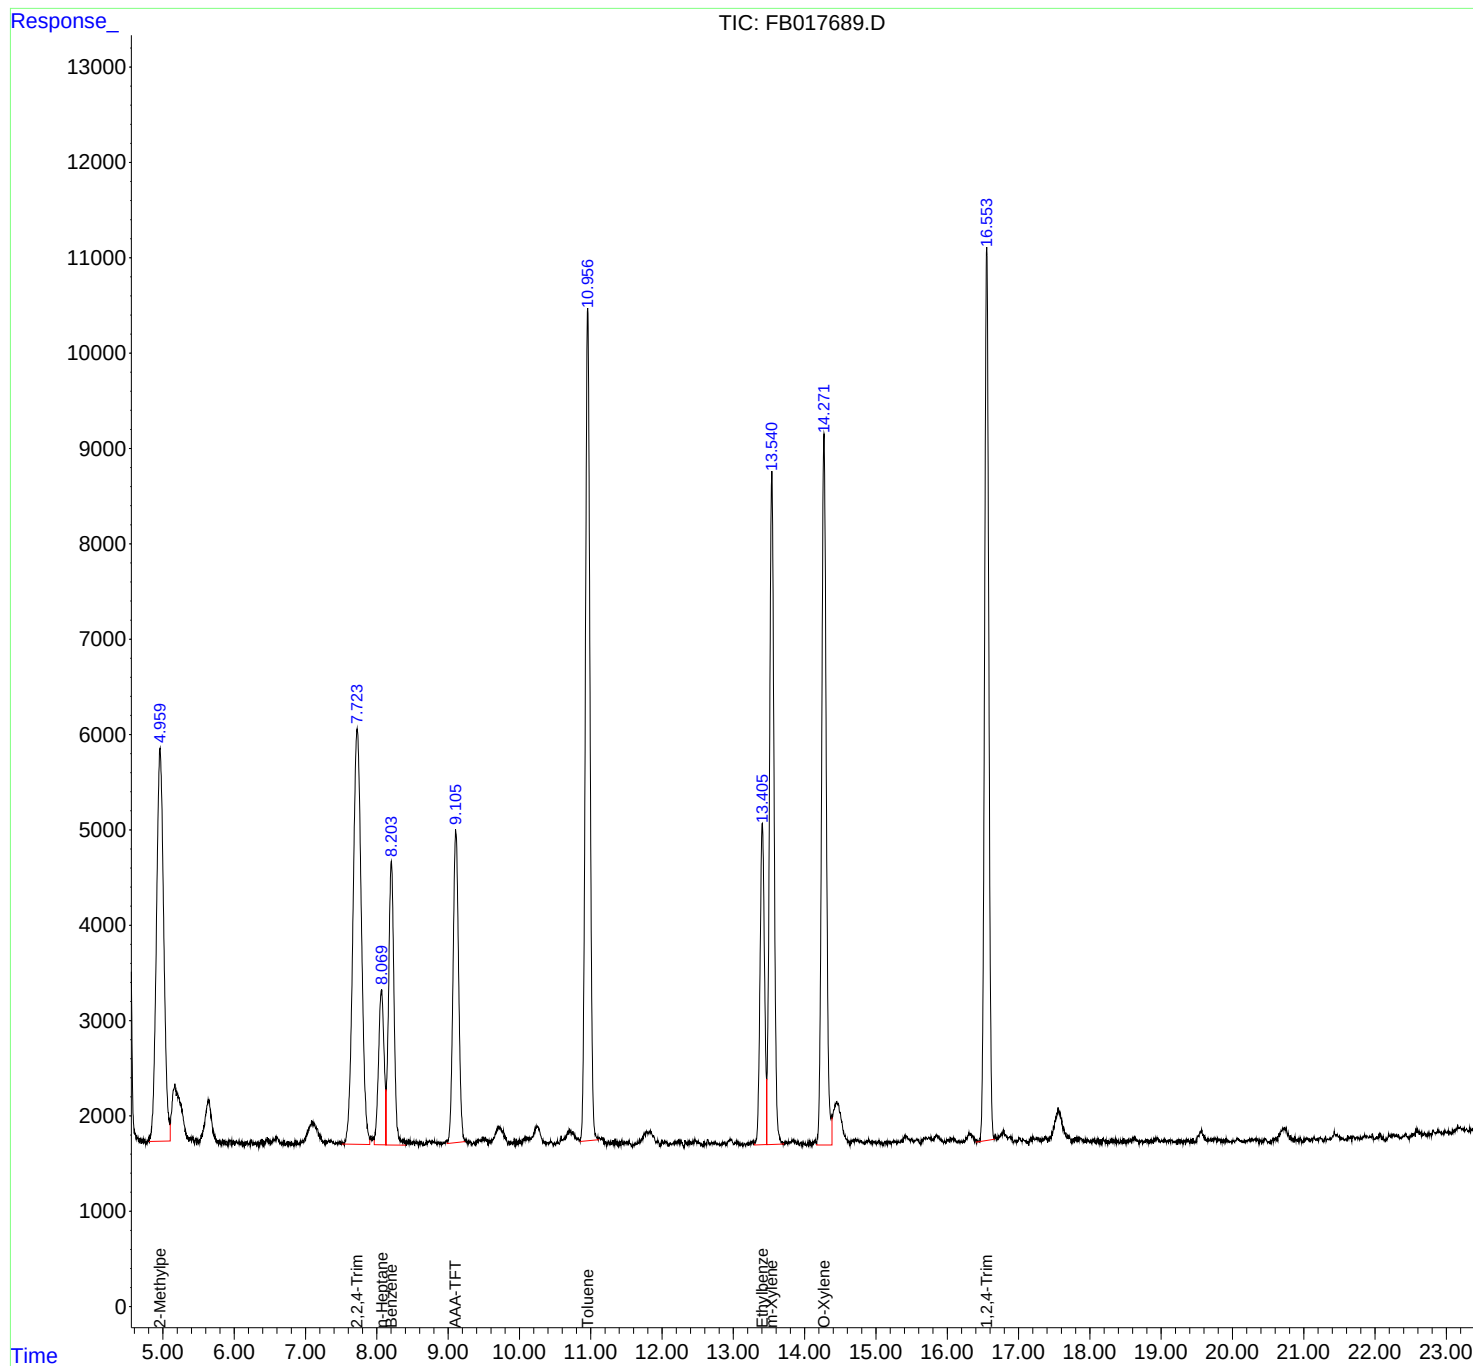

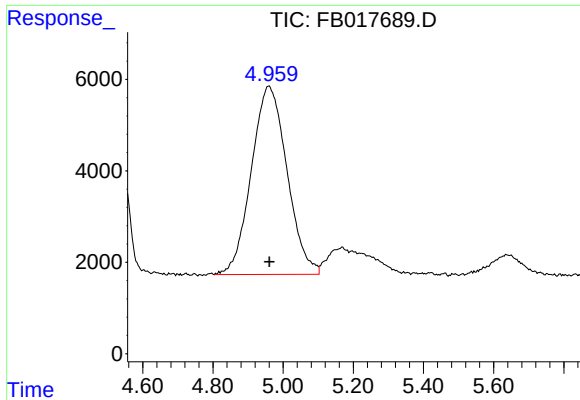


#1 2-Methylpentane

R.T.: 4.959 min
Delta R.T.: -0.002 min
Response: 290713
Conc: 20.75 ng/ml

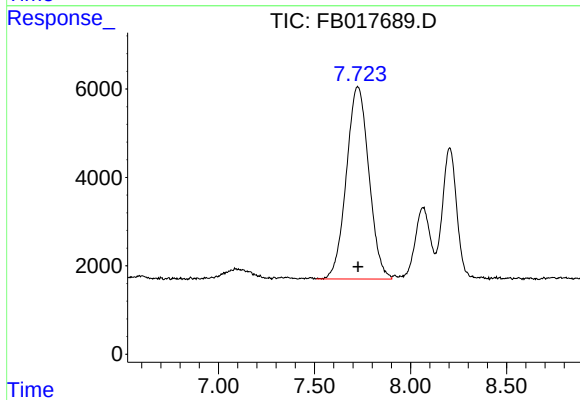


#2 2,2,4-Trimethylpentane

R.T.: 7.724 min
Delta R.T.: -0.003 min
Response: 354067
Conc: 25.13 ng/ml

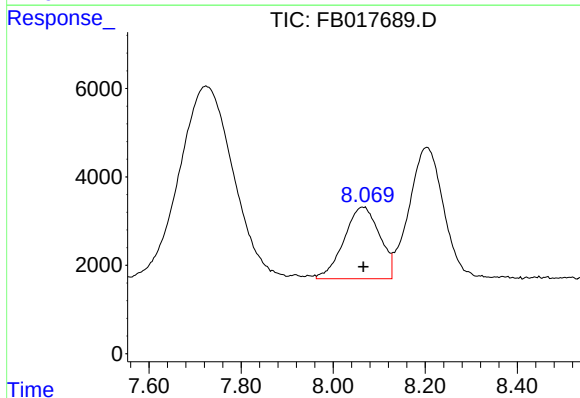


#3 n-Heptane

R.T.: 8.065 min
Delta R.T.: -0.001 min
Response: 87009
Conc: 6.31 ng/ml

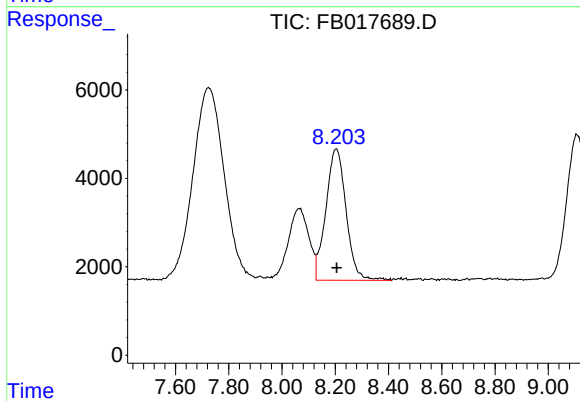


#4 Benzene

R.T.: 8.204 min
Delta R.T.: -0.001 min
Response: 156907
Conc: 8.90 ng/ml

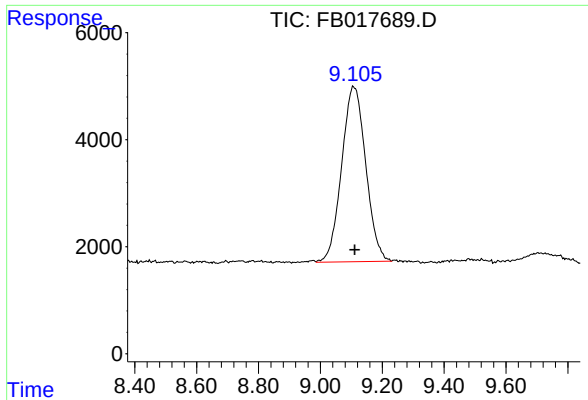


#5 AAA-TFT

R.T.: 9.107 min
Delta R.T.: -0.004 min
Response: 176962
Conc: 21.46 ng/ml

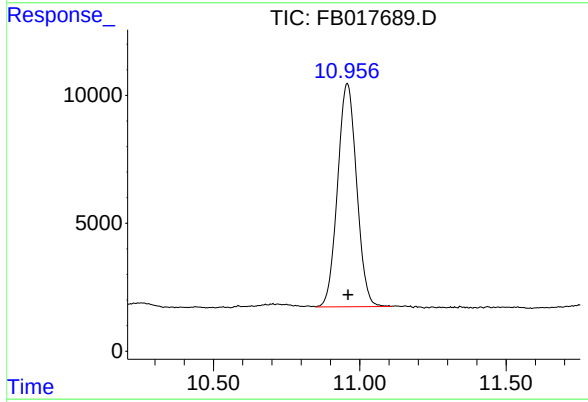


#6 Toluene

R.T.: 10.958 min
Delta R.T.: -0.002 min
Response: 394484
Conc: 27.42 ng/ml

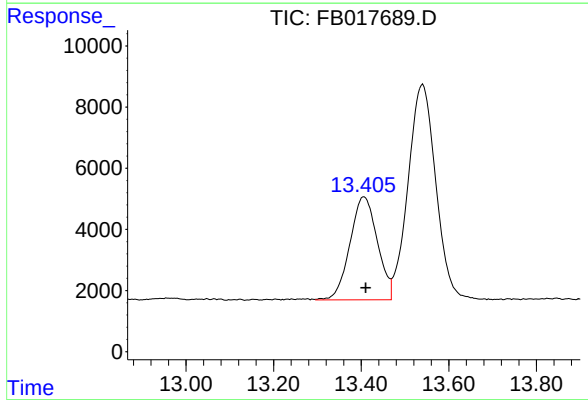


#7 Ethylbenzene

R.T.: 13.406 min
Delta R.T.: -0.004 min
Response: 146396
Conc: 9.93 ng/ml

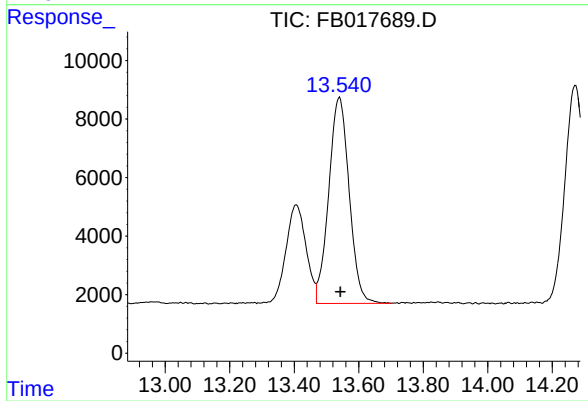


#8 m-Xylene

R.T.: 13.541 min
Delta R.T.: -0.002 min
Response: 309932
Conc: 19.94 ng/ml

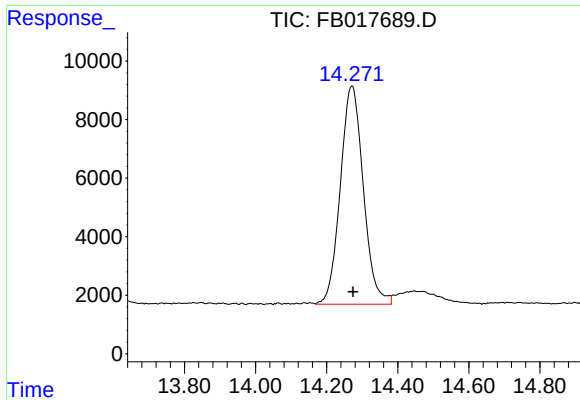

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: -0.002 min
Response: 335219
Conc: 20.42 ng/ml

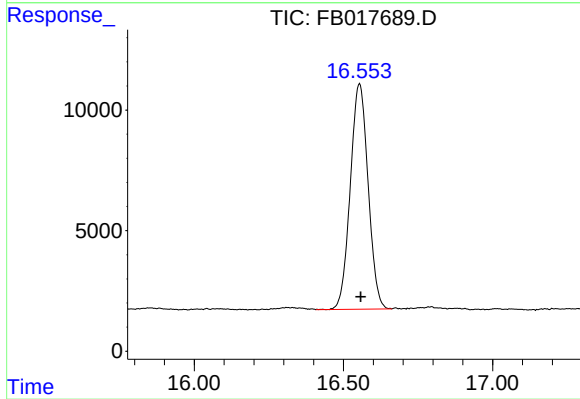

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: -0.003 min
Response: 388133
Conc: 19.93 ng/ml