

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092225\
 Data File : FB032221.D
 Signal(s) : FID2B.CH
 Acq On : 22 Sep 2025 14:08
 Operator : YP/AJ
 Sample : BSF0922S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0922S1

Integration File: autoint1.e
 Quant Time: Sep 23 03:34:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
 Quant Title :
 QLast Update : Mon Sep 22 12:16:10 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	358287	20.017 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	761278	28.189 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	866985	30.691 ng/ml
3) t n-Heptane	7.759	273988	10.028 ng/ml
4) t Benzene	7.897	325871	9.017 ng/ml
6) t Toluene	10.627	988005	26.527 ng/ml
7) t Ethylbenzene	13.063	294071	8.996 ng/ml
8) t m-Xylene	13.197	613401	17.997 ng/ml
9) t O-Xylene	13.924	584850	17.910 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	506239	18.098 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092225\
Data File : FB032221.D
Signal(s) : FID2B.CH
Acq On : 22 Sep 2025 14:08
Operator : YP/AJ
Sample : BSF0922S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0922S1

Integration File: autoint1.e
Quant Time: Sep 23 03:34:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

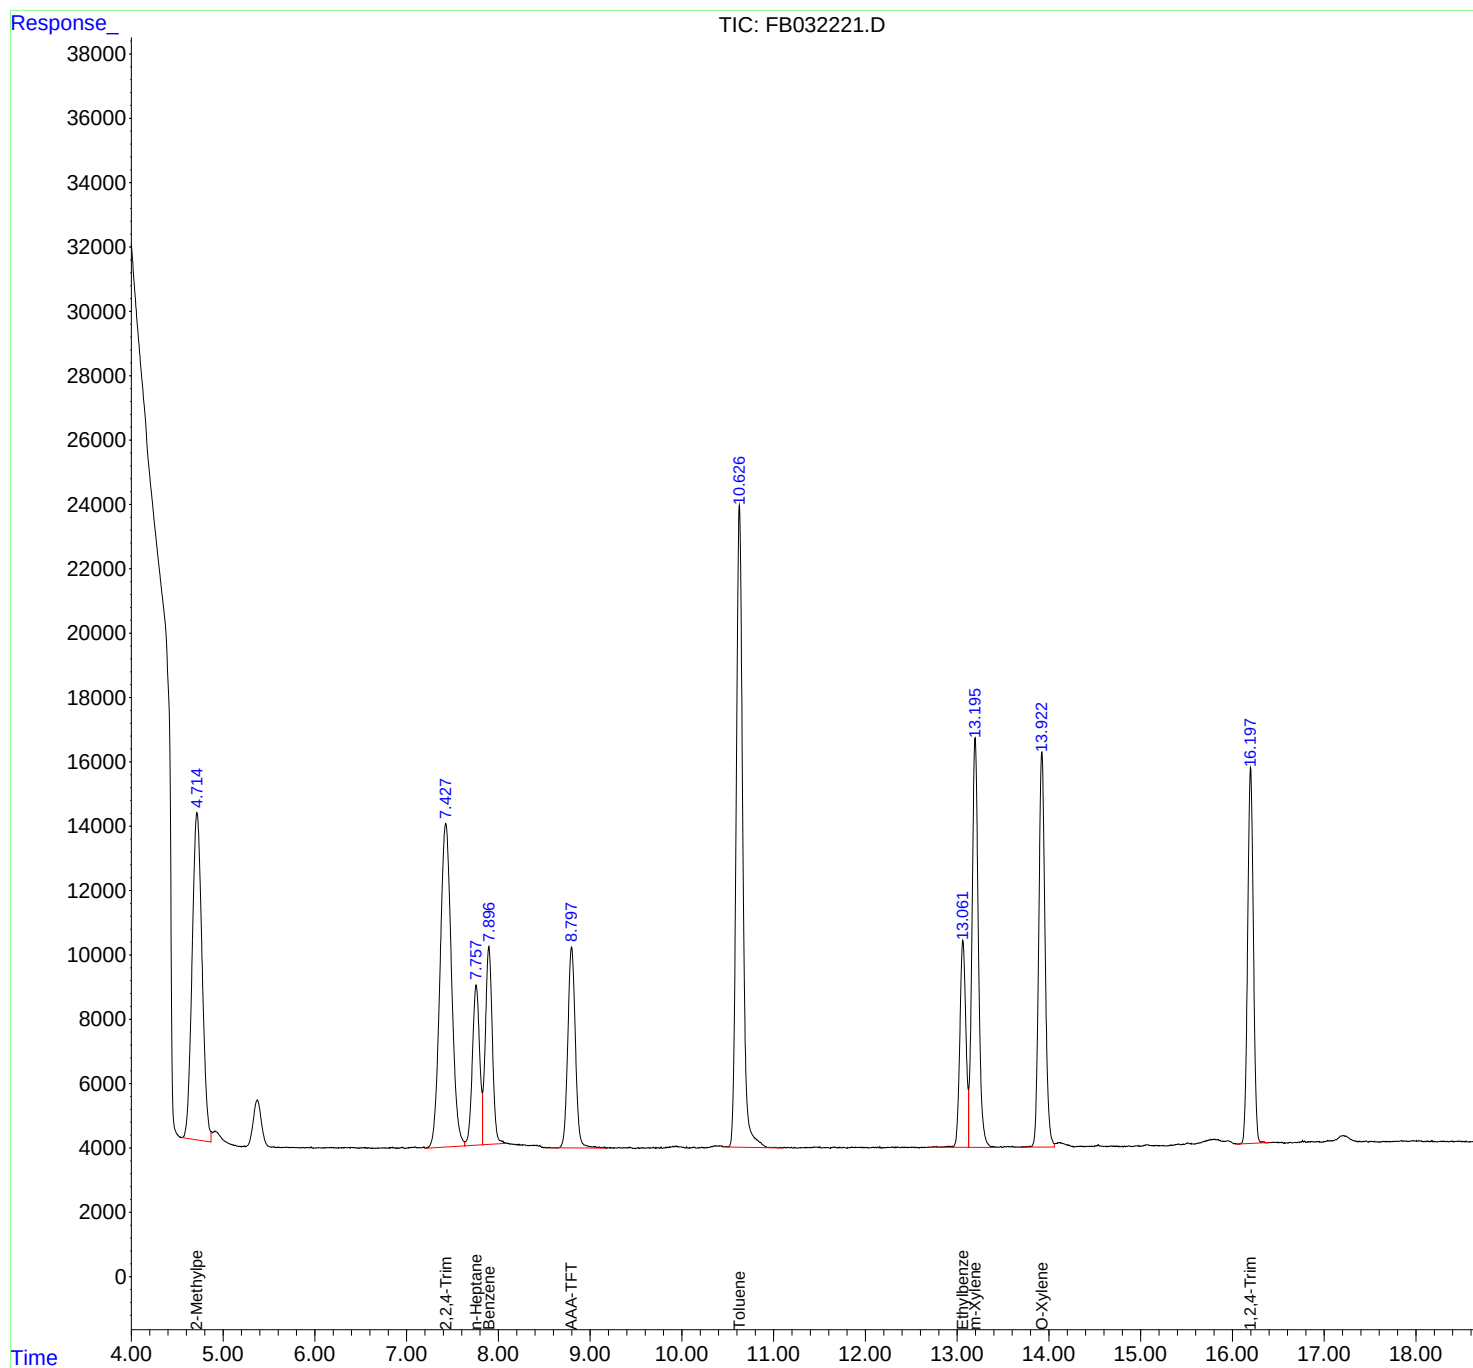


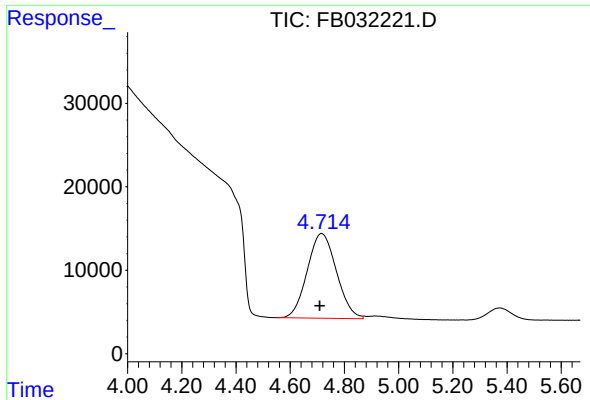

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: 0.007 min
Response: 761278
Conc: 28.19 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0922S1

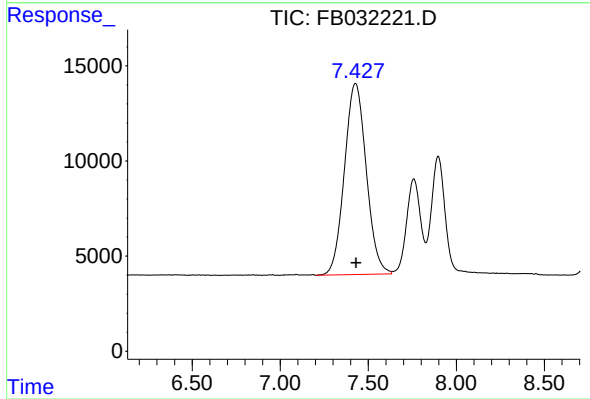


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: -0.002 min
Response: 866985
Conc: 30.69 ng/ml

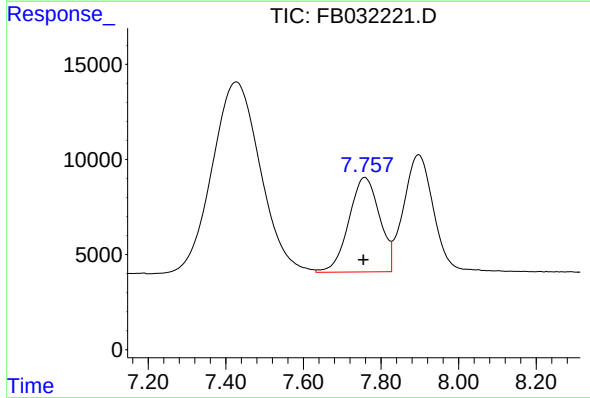


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.004 min
Response: 273988
Conc: 10.03 ng/ml

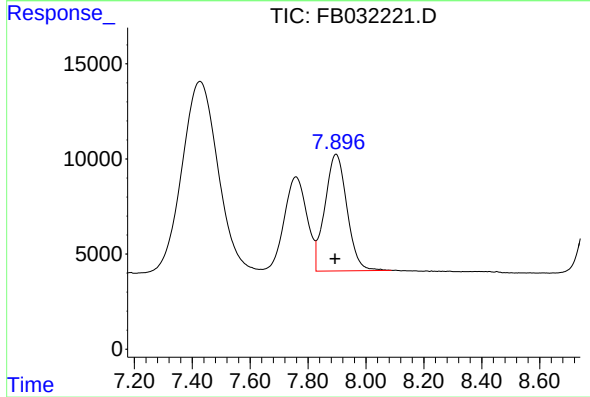

#4 Benzene


R.T.: 7.897 min
Delta R.T.: 0.004 min
Response: 325871
Conc: 9.02 ng/ml

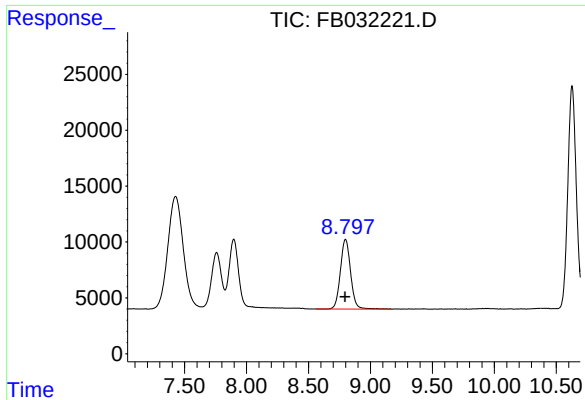

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.003 min
Response: 358287
Conc: 20.02 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0922S1

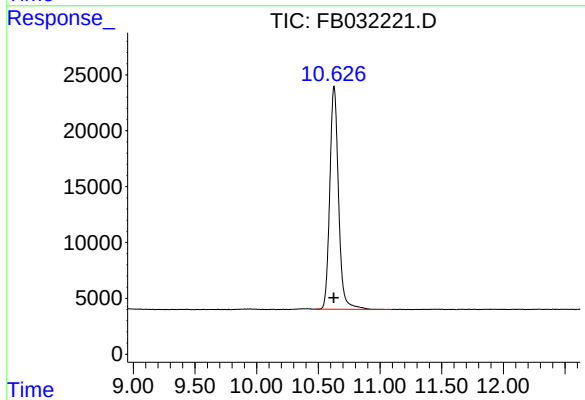


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.002 min
Response: 988005
Conc: 26.53 ng/ml

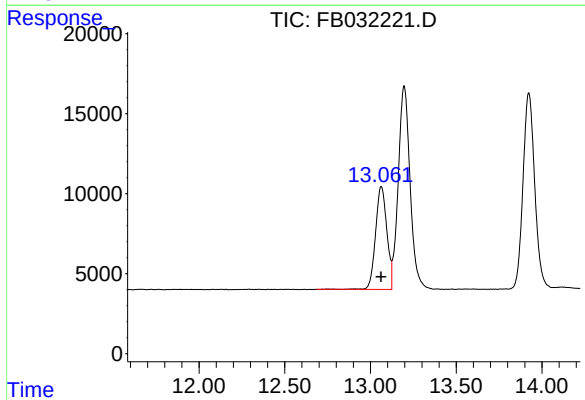


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.001 min
Response: 294071
Conc: 9.00 ng/ml

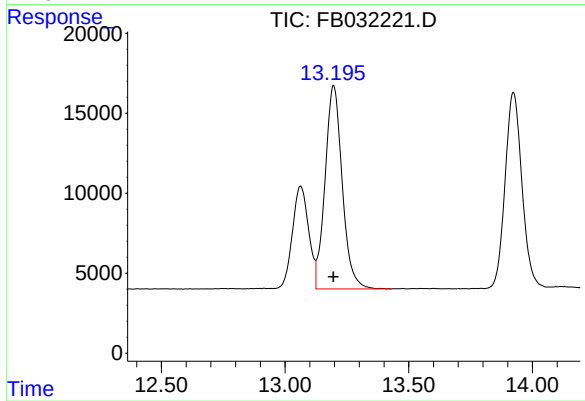

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.001 min
Response: 613401
Conc: 18.00 ng/ml

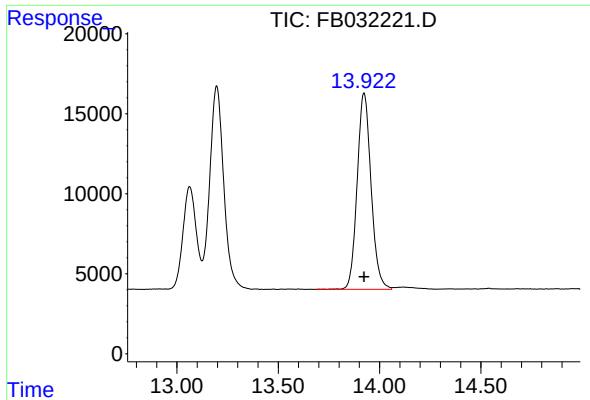

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.000 min
Response: 584850
Conc: 17.91 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0922S1

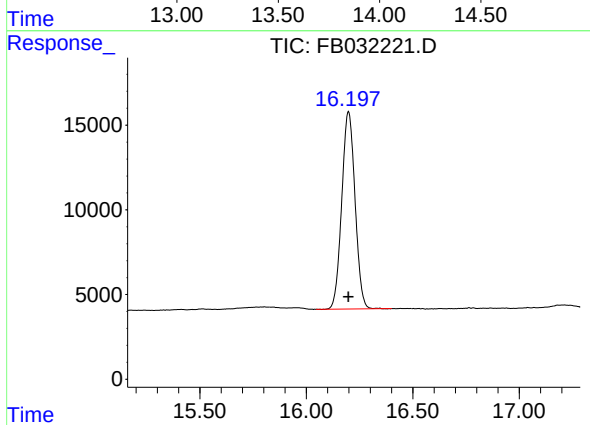

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.000 min
Response: 506239
Conc: 18.10 ng/ml