

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092225\
 Data File : FB032226.D
 Signal(s) : FID2B.CH
 Acq On : 22 Sep 2025 16:35
 Operator : YP/AJ
 Sample : BSF0922S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0922S1

Integration File: autoint1.e
 Quant Time: Sep 23 03:35:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
 Quant Title :
 QLast Update : Mon Sep 22 12:16:10 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	366824	20.493 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	831762	30.799 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	957214	33.885 ng/ml
3) t n-Heptane	7.759	307803	11.265 ng/ml
4) t Benzene	7.897	375572	10.392 ng/ml
6) t Toluene	10.628	1109031	29.777 ng/ml
7) t Ethylbenzene	13.064	324537	9.928 ng/ml
8) t m-Xylene	13.197	673600	19.763 ng/ml
9) t O-Xylene	13.924	646336	19.793 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	547275	19.566 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092225\
Data File : FB032226.D
Signal(s) : FID2B.CH
Acq On : 22 Sep 2025 16:35
Operator : YP/AJ
Sample : BSF0922S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0922S1

Integration File: autoint1.e
Quant Time: Sep 23 03:35:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

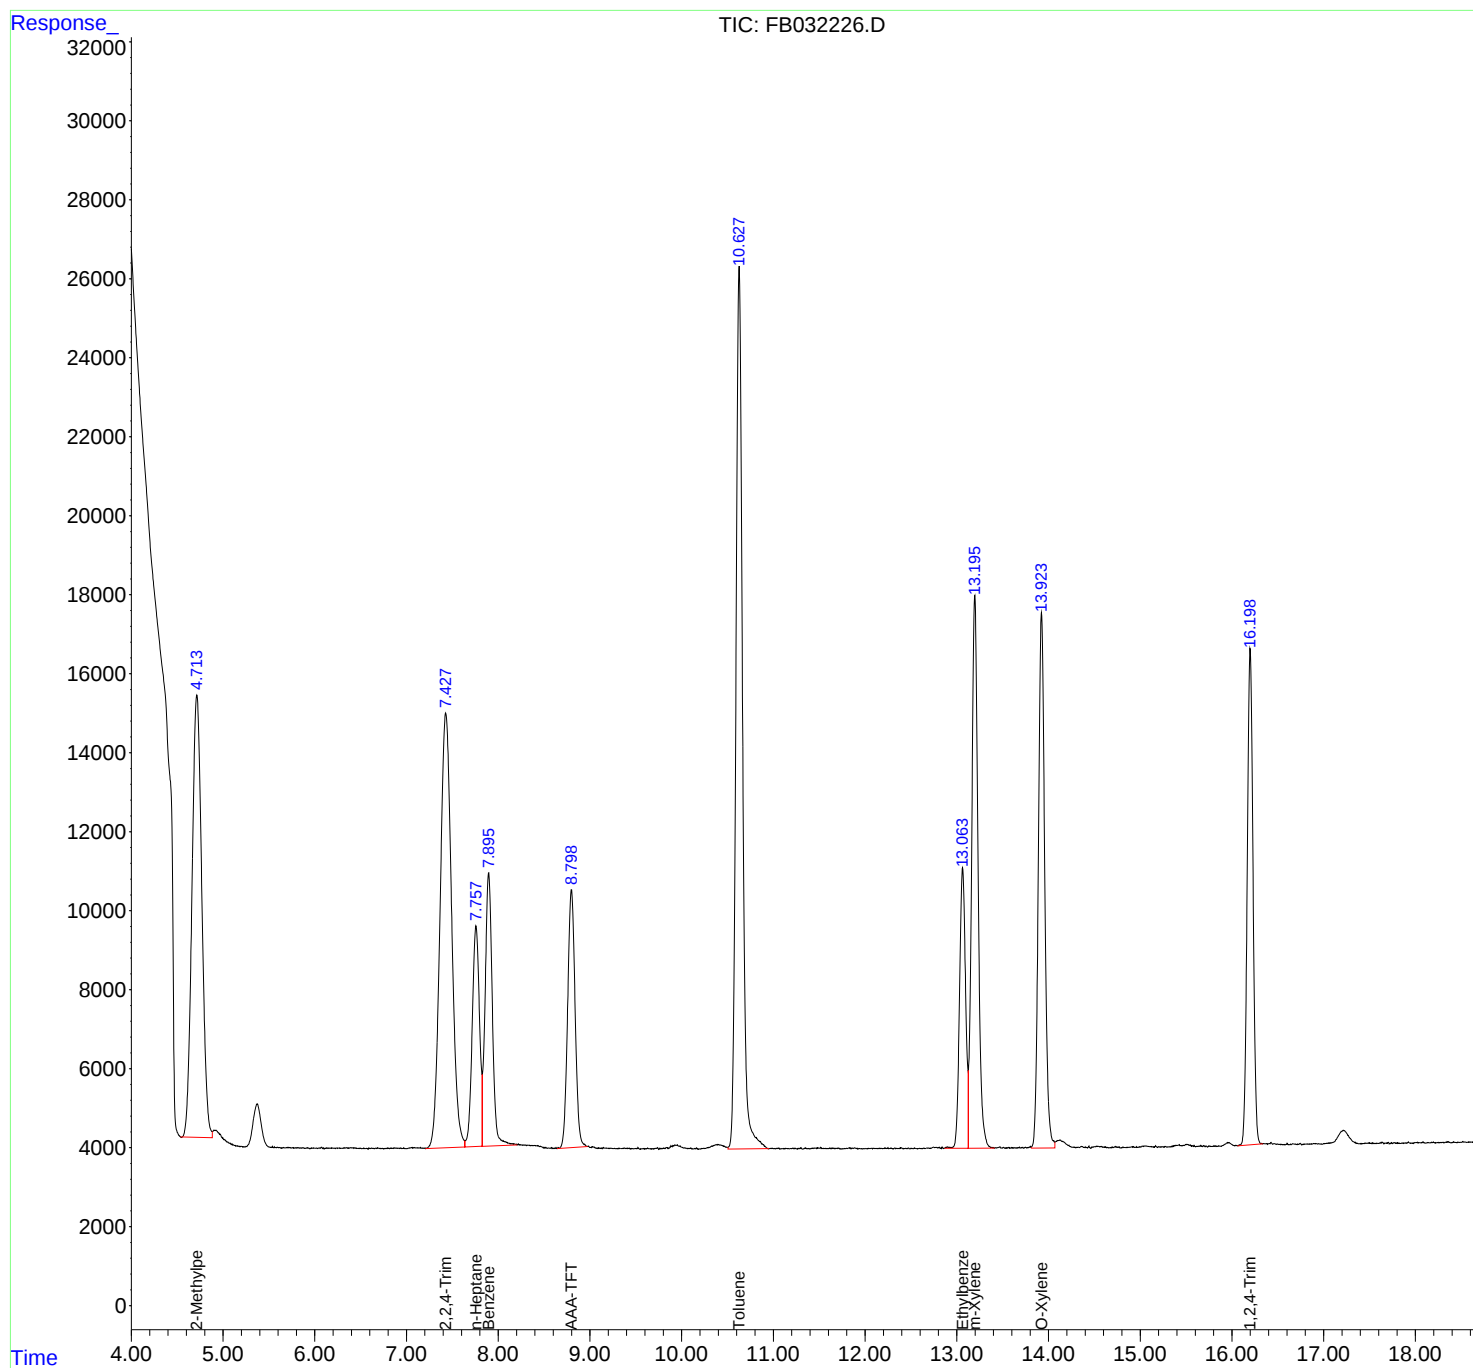


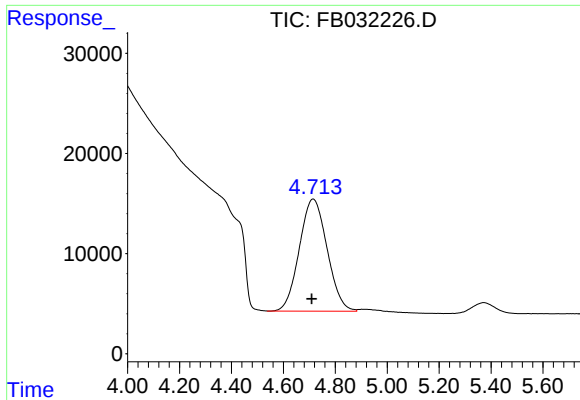

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: 0.006 min
Response: 831762
Conc: 30.80 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0922S1

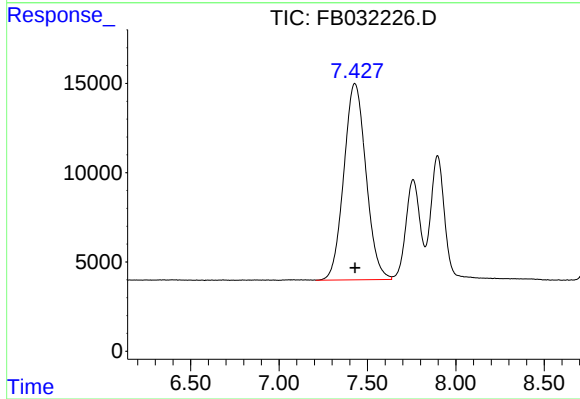


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: -0.002 min
Response: 957214
Conc: 33.89 ng/ml

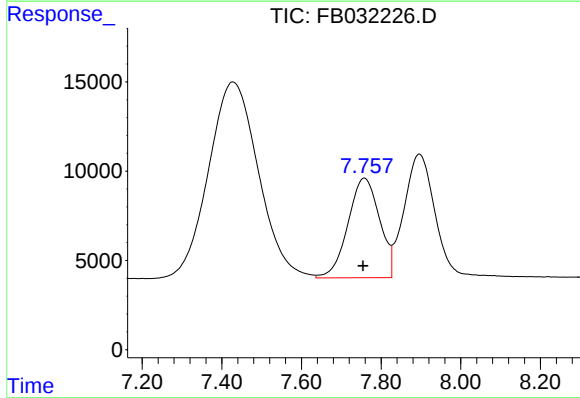


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.004 min
Response: 307803
Conc: 11.27 ng/ml

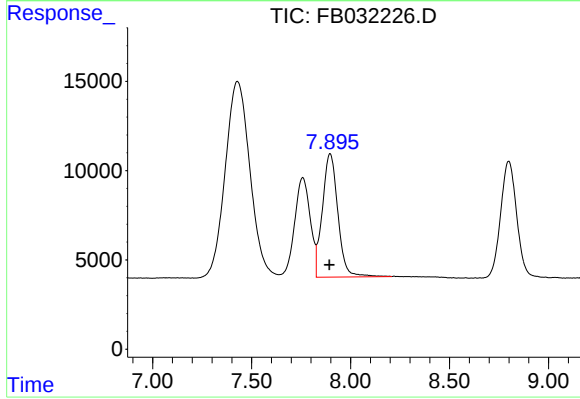

#4 Benzene


R.T.: 7.897 min
Delta R.T.: 0.003 min
Response: 375572
Conc: 10.39 ng/ml

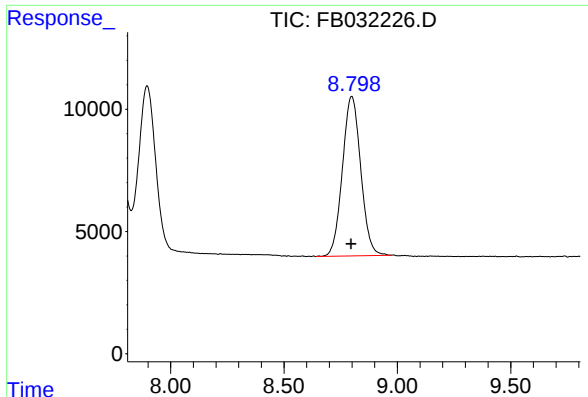

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.003 min
Response: 366824
Conc: 20.49 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0922S1

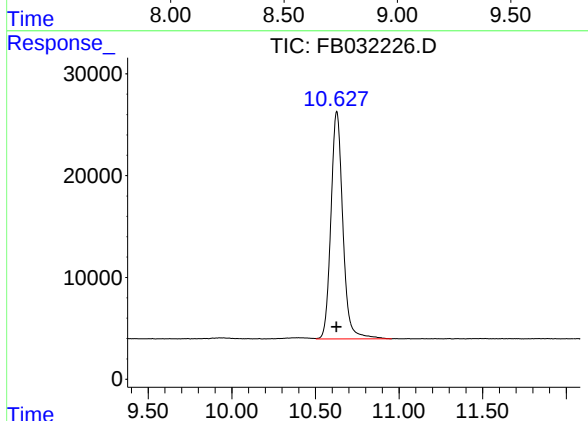


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.002 min
Response: 1109031
Conc: 29.78 ng/ml

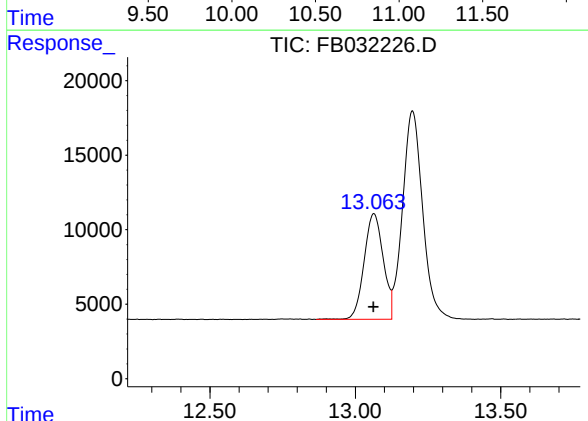


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.002 min
Response: 324537
Conc: 9.93 ng/ml

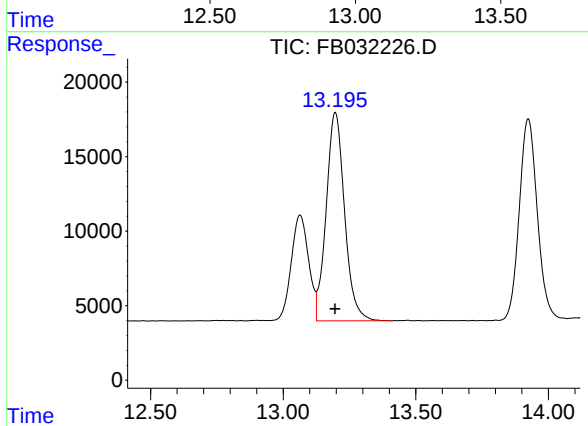

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.002 min
Response: 673600
Conc: 19.76 ng/ml

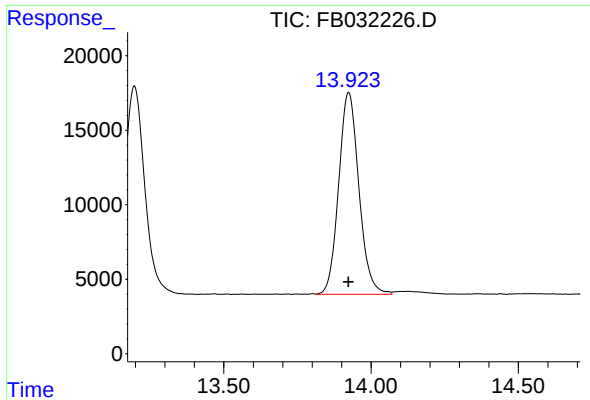

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.001 min
Response: 646336
Conc: 19.79 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0922S1

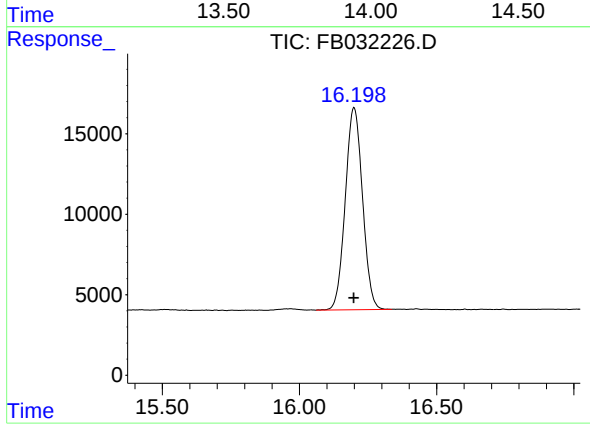

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.002 min
Response: 547275
Conc: 19.57 ng/ml