

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092225\
 Data File : FB032227.D
 Signal(s) : FID2B.CH
 Acq On : 22 Sep 2025 17:02
 Operator : YP/AJ
 Sample : BSF0922S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0922S2

Integration File: autoint1.e
 Quant Time: Sep 23 03:35:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
 Quant Title :
 QLast Update : Mon Sep 22 12:16:10 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	363072	20.284 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	801046	29.661 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	948619	33.581 ng/ml
3) t n-Heptane	7.759	297051	10.872 ng/ml
4) t Benzene	7.898	373962	10.348 ng/ml
6) t Toluene	10.628	1105664	29.686 ng/ml
7) t Ethylbenzene	13.064	323316	9.891 ng/ml
8) t m-Xylene	13.198	674144	19.779 ng/ml
9) t O-Xylene	13.925	649538	19.891 ng/ml
10) t 1,2,4-Trimethylbenzene	16.200	554725	19.832 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092225\
Data File : FB032227.D
Signal(s) : FID2B.CH
Acq On : 22 Sep 2025 17:02
Operator : YP/AJ
Sample : BSF0922S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0922S2

Integration File: autoint1.e
Quant Time: Sep 23 03:35:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

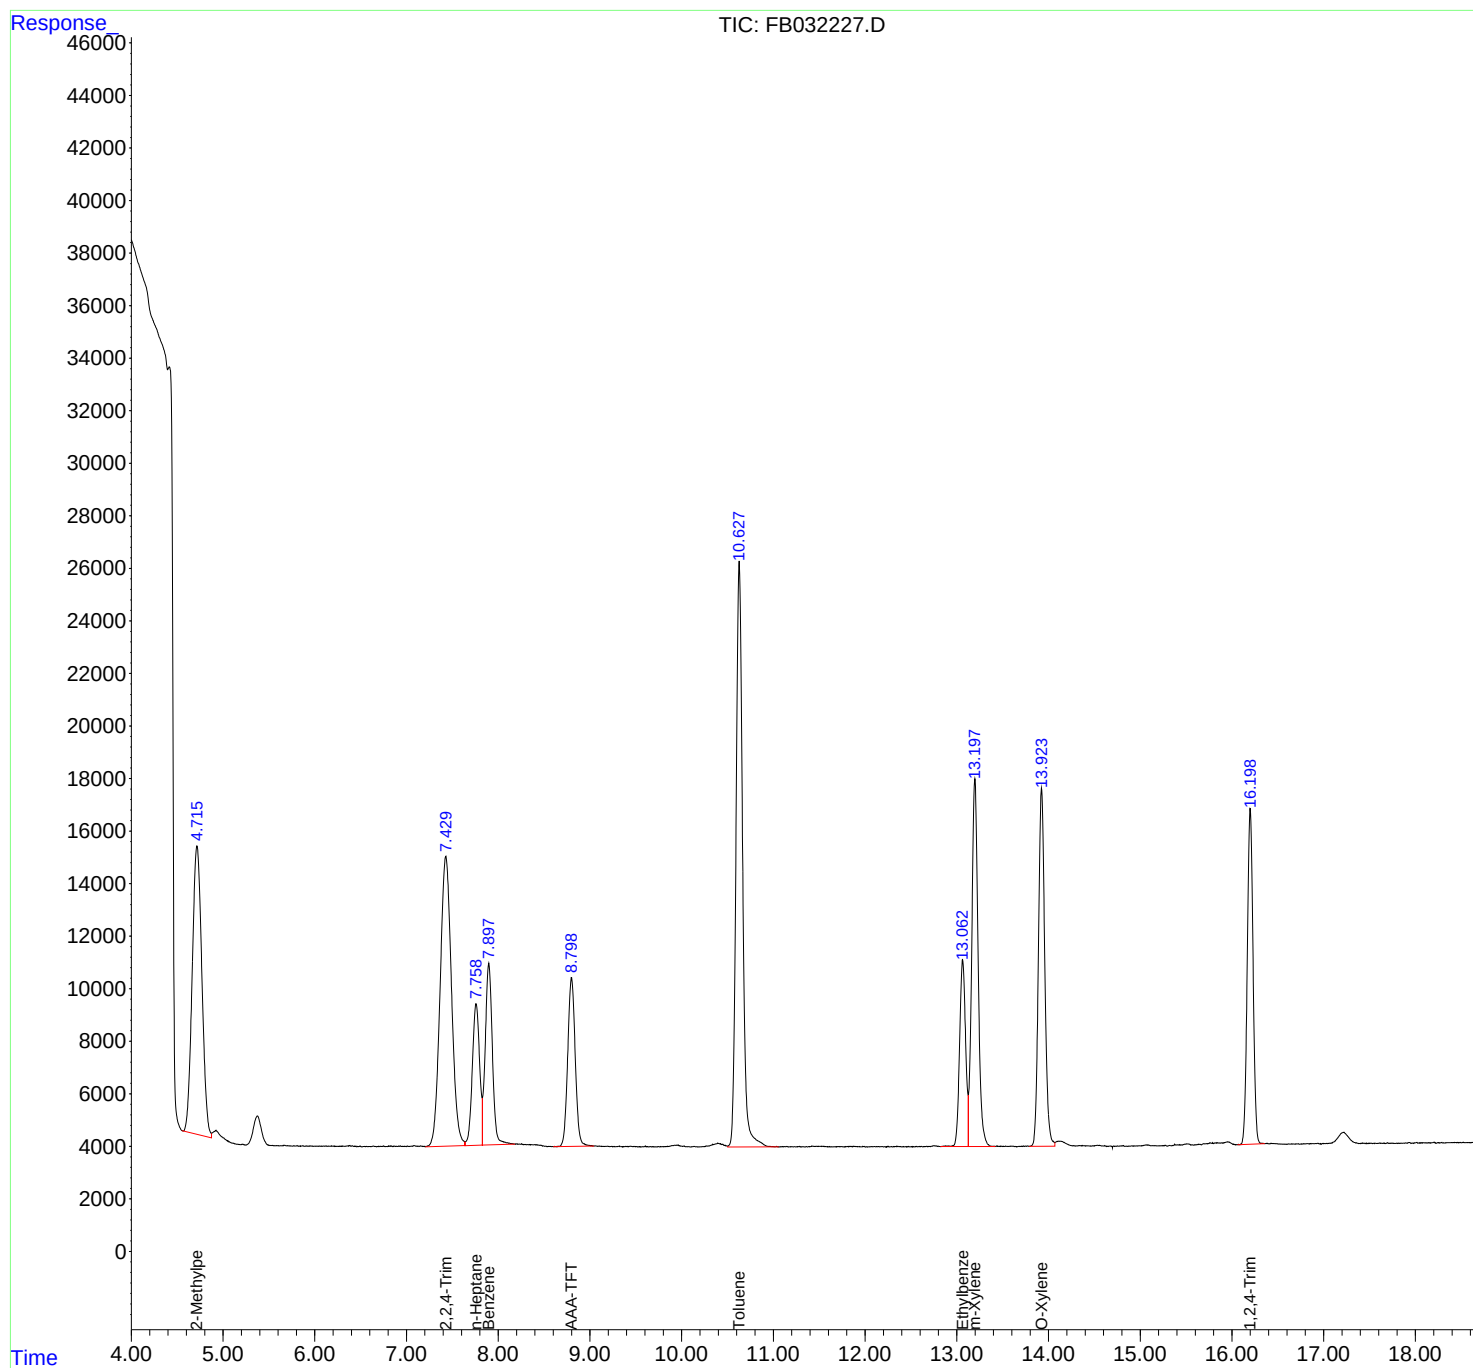


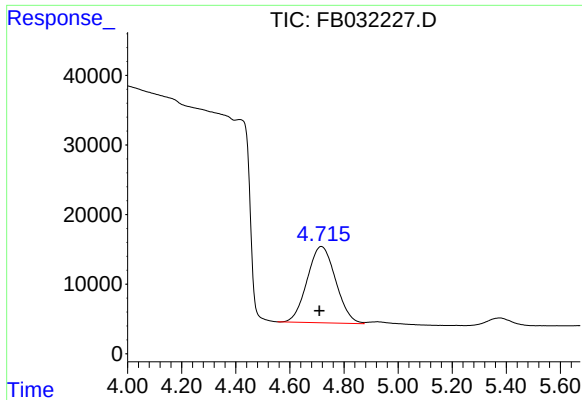

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: 0.007 min
Response: 801046
Conc: 29.66 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0922S2

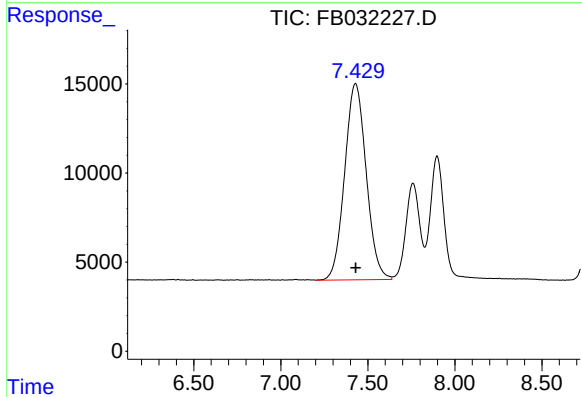


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: 0.000 min
Response: 948619
Conc: 33.58 ng/ml

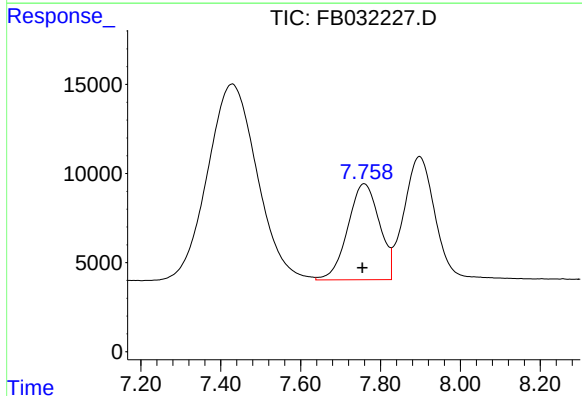


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.004 min
Response: 297051
Conc: 10.87 ng/ml

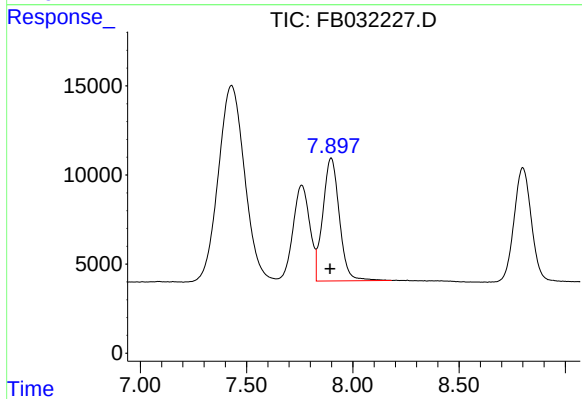

#4 Benzene


R.T.: 7.898 min
Delta R.T.: 0.005 min
Response: 373962
Conc: 10.35 ng/ml

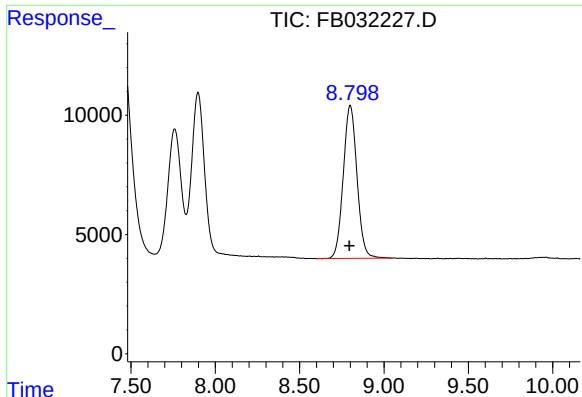

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.004 min
Response: 363072
Conc: 20.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0922S2

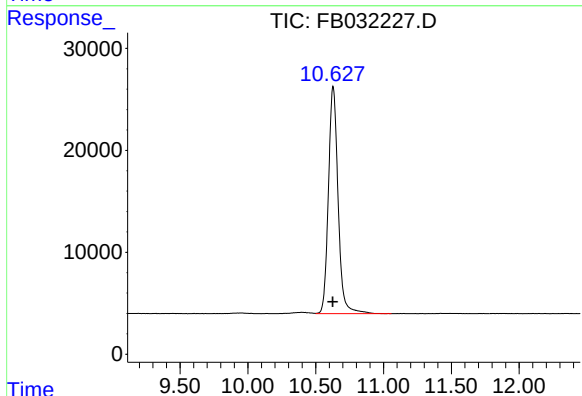


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.003 min
Response: 1105664
Conc: 29.69 ng/ml

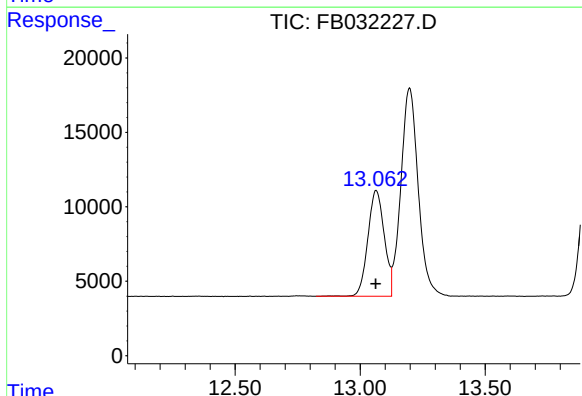


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.002 min
Response: 323316
Conc: 9.89 ng/ml

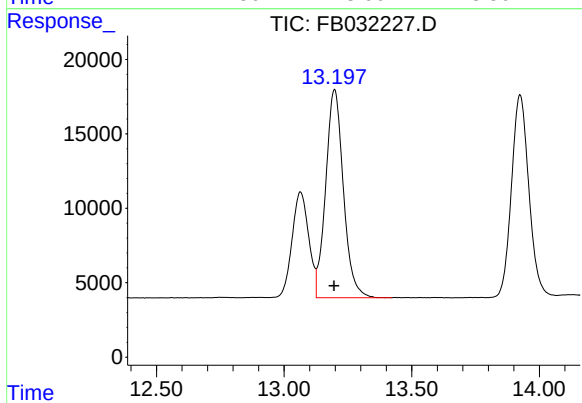

#8 m-Xylene


R.T.: 13.198 min
Delta R.T.: 0.002 min
Response: 674144
Conc: 19.78 ng/ml

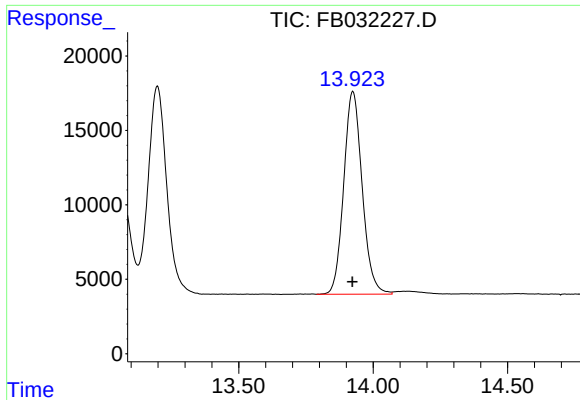

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.002 min
Response: 649538
Conc: 19.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0922S2

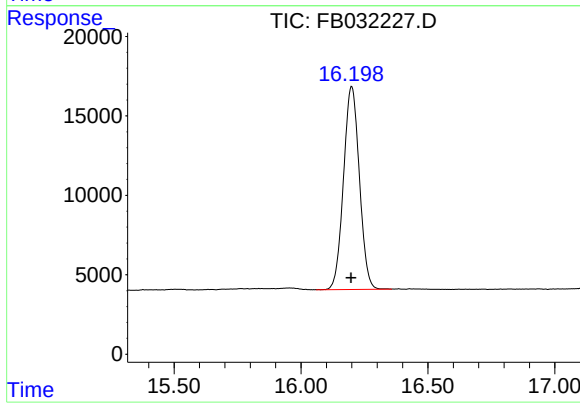

#10 1,2,4-Trimethylbenzene

R.T.: 16.200 min
Delta R.T.: 0.002 min
Response: 554725
Conc: 19.83 ng/ml