

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092325\
Data File : FB032230.D
Signal(s) : FID2B.CH
Acq On : 23 Sep 2025 10:13
Operator : YP/AJ
Sample : VBF0923S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 24 01:33:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	358860	20.049 ng/ml
Target Compounds			
8) t m-Xylene	13.197	4021	0.118 ng/ml
9) t O-Xylene	13.918	5835	0.179 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	11270	0.403 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092325\
Data File : FB032230.D
Signal(s) : FID2B.CH
Acq On : 23 Sep 2025 10:13
Operator : YP/AJ
Sample : VBF0923S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 24 01:33:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

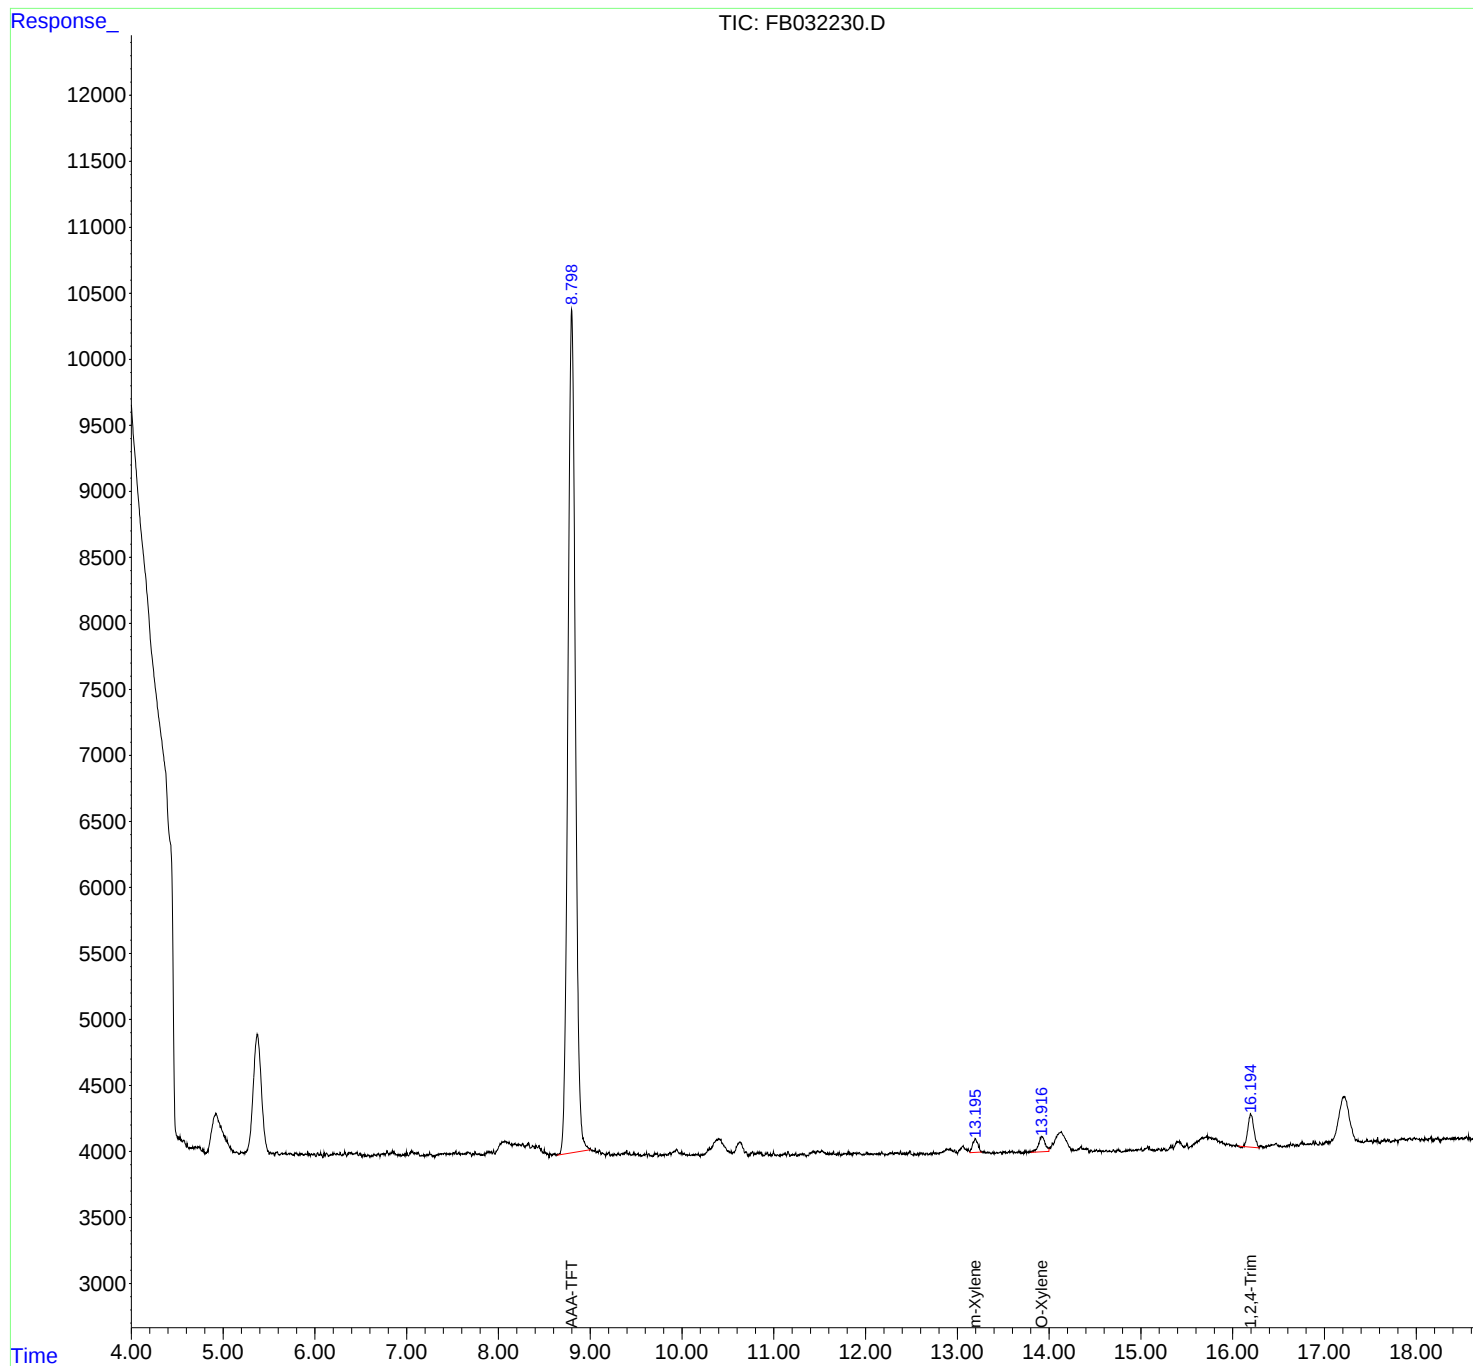


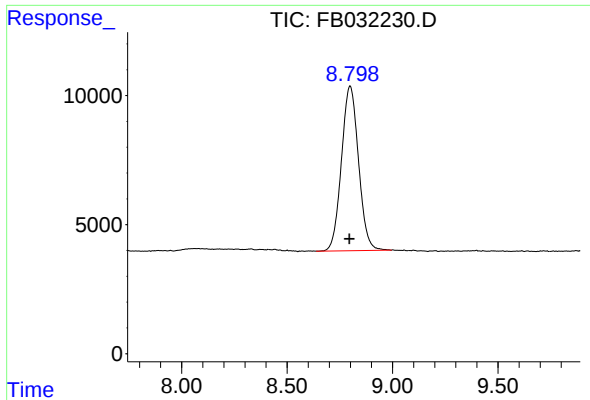

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.003 min
Response: 358860
Conc: 20.05 ng/ml

Instrument :
FID_B
ClientSampleId :

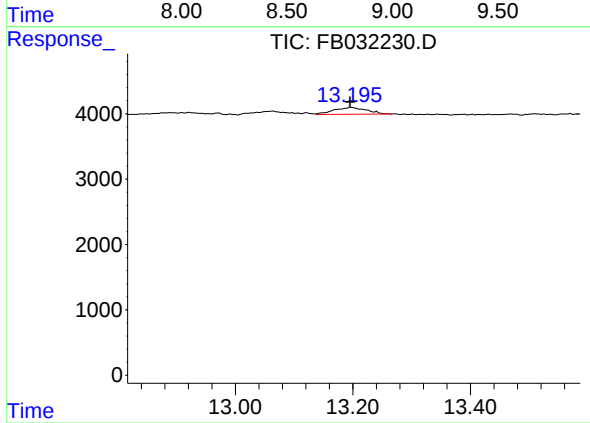


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: 0.002 min
Response: 4021
Conc: 0.12 ng/ml

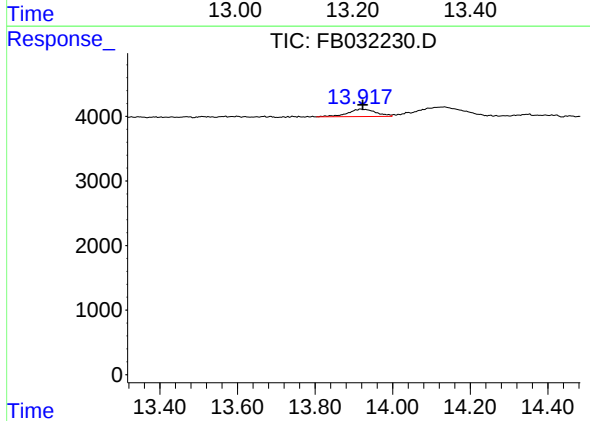

#9 o-Xylene

R.T.: 13.918 min
Delta R.T.: -0.004 min
Response: 5835
Conc: 0.18 ng/ml

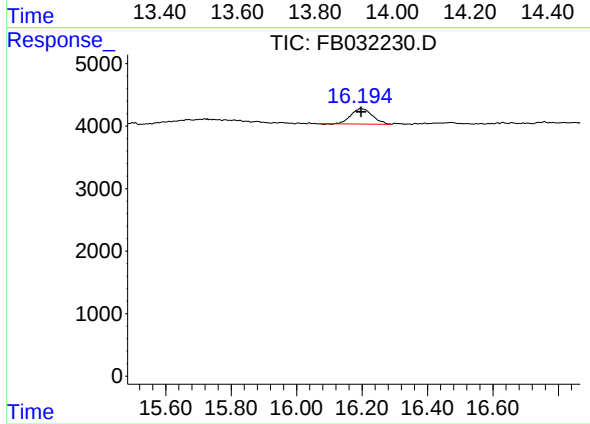

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: -0.001 min
Response: 11270
Conc: 0.40 ng/ml