

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092325\
Data File : FB032234.D
Signal(s) : FID2B.CH
Acq On : 23 Sep 2025 12:20
Operator : YP/AJ
Sample : Q3157-01
Misc : 4.16G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 24 01:34:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	303374	16.949 ng/ml
Target Compounds			
8) t m-Xylene	13.202	4321	0.127 ng/ml
9) t O-Xylene	13.929	4423	0.135 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	10739	0.384 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092325\
Data File : FB032234.D
Signal(s) : FID2B.CH
Acq On : 23 Sep 2025 12:20
Operator : YP/AJ
Sample : Q3157-01
Misc : 4.16G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 24 01:34:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

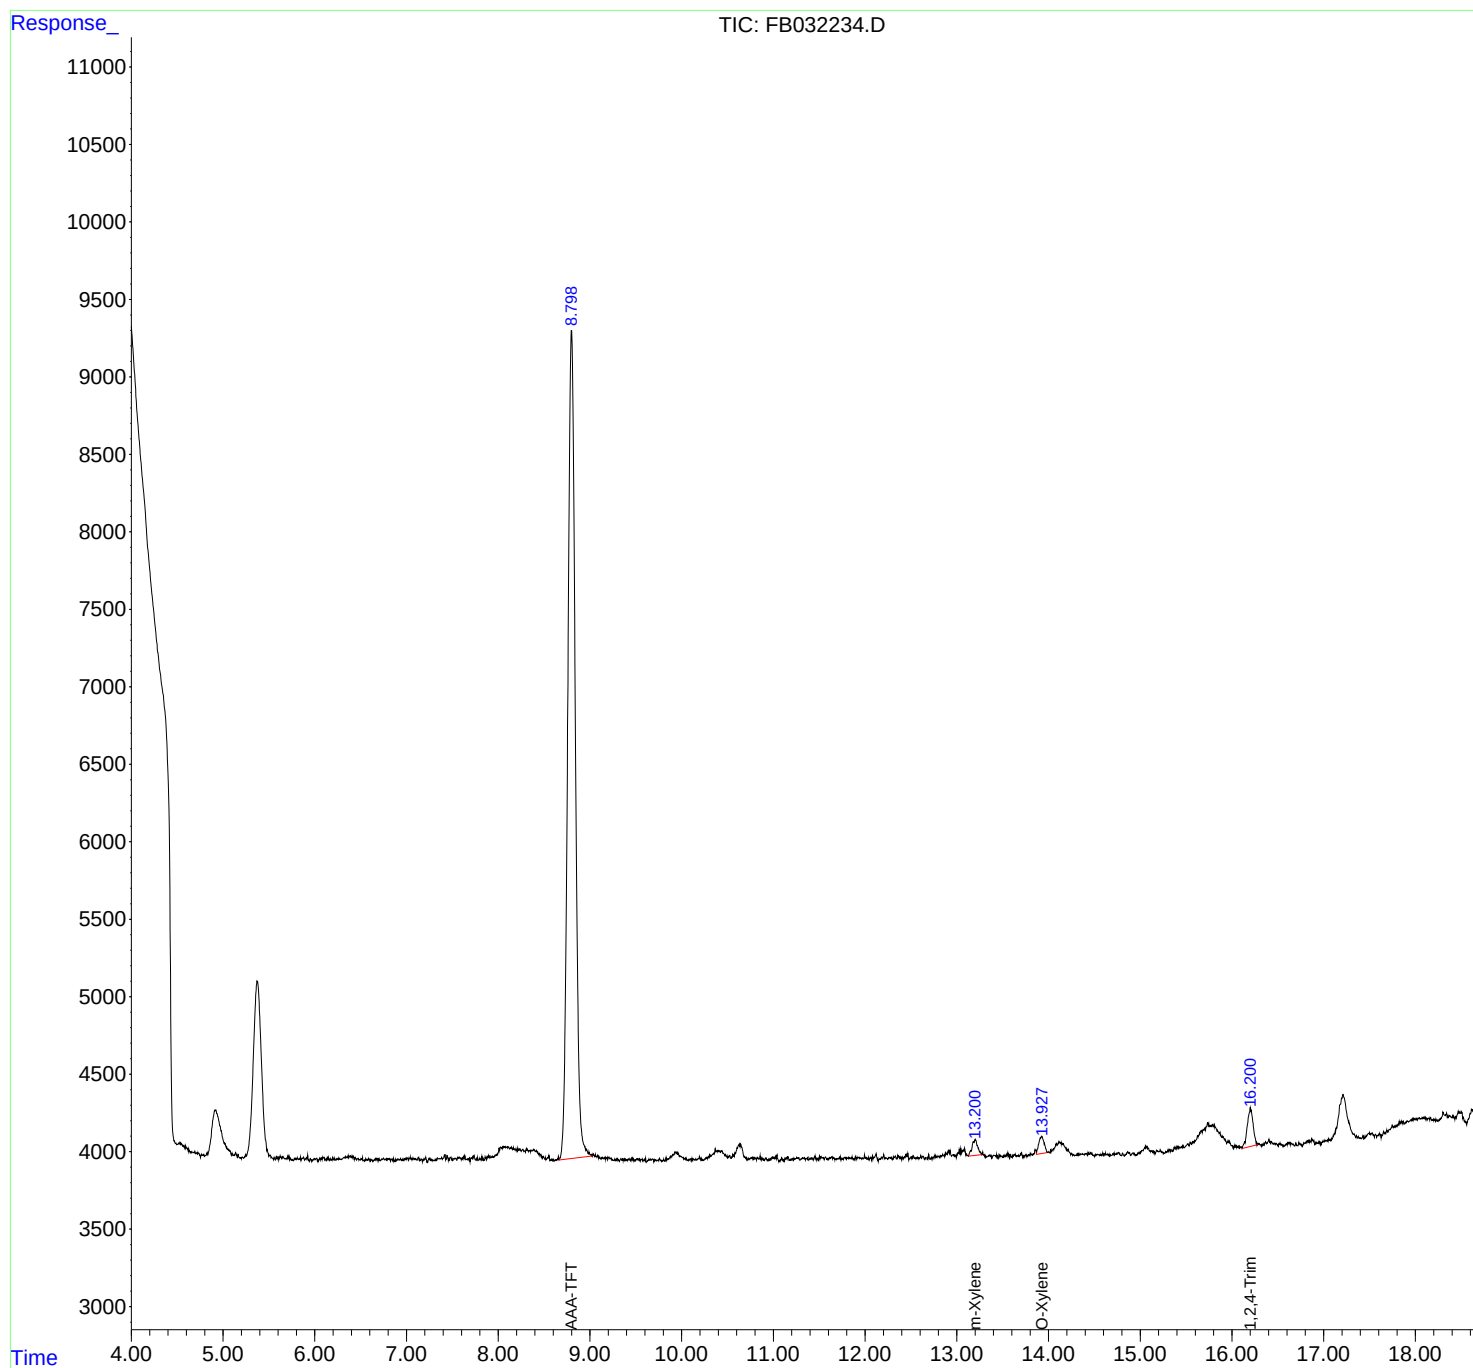


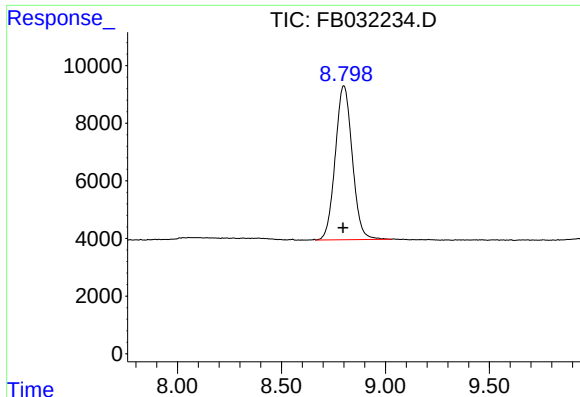

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.004 min
Response: 303374
Conc: 16.95 ng/ml

Instrument :
FID_B
ClientSampleId :

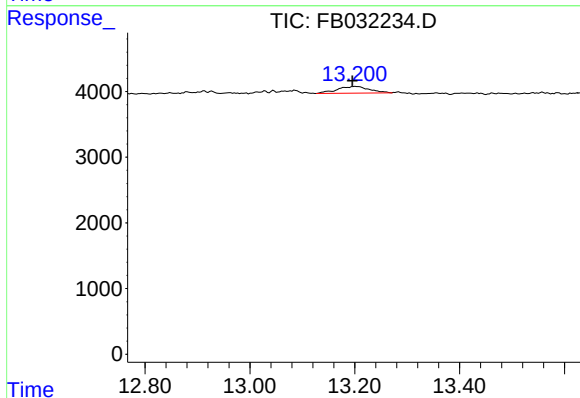


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.006 min
Response: 4321
Conc: 0.13 ng/ml

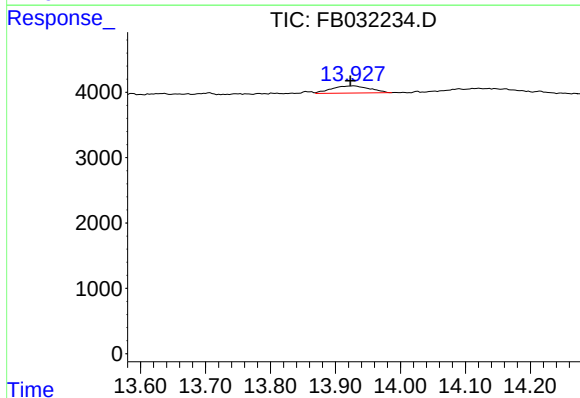

#9 o-Xylene

R.T.: 13.929 min
Delta R.T.: 0.006 min
Response: 4423
Conc: 0.14 ng/ml

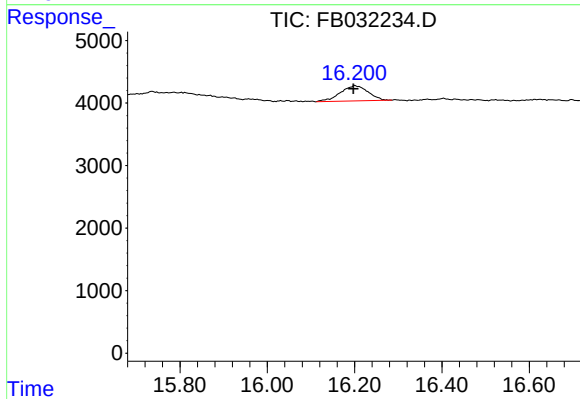

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: 0.004 min
Response: 10739
Conc: 0.38 ng/ml