

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092325\
 Data File : FB032233.D
 Signal(s) : FID2B.CH
 Acq On : 23 Sep 2025 11:36
 Operator : YP/AJ
 Sample : BSF0923S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0923S2

Integration File: autoint1.e
 Quant Time: Sep 24 01:34:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
 Quant Title :
 QLast Update : Mon Sep 22 12:16:10 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	373996	20.894 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	642081	23.775 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	773096	27.368 ng/ml
3) t n-Heptane	7.760	234490	8.582 ng/ml
4) t Benzene	7.898	313104	8.664 ng/ml
6) t Toluene	10.629	917032	24.622 ng/ml
7) t Ethylbenzene	13.065	267806	8.193 ng/ml
8) t m-Xylene	13.197	560582	16.447 ng/ml
9) t O-Xylene	13.925	549054	16.814 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	468859	16.762 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092325\
Data File : FB032233.D
Signal(s) : FID2B.CH
Acq On : 23 Sep 2025 11:36
Operator : YP/AJ
Sample : BSF0923S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0923S2

Integration File: autoint1.e
Quant Time: Sep 24 01:34:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

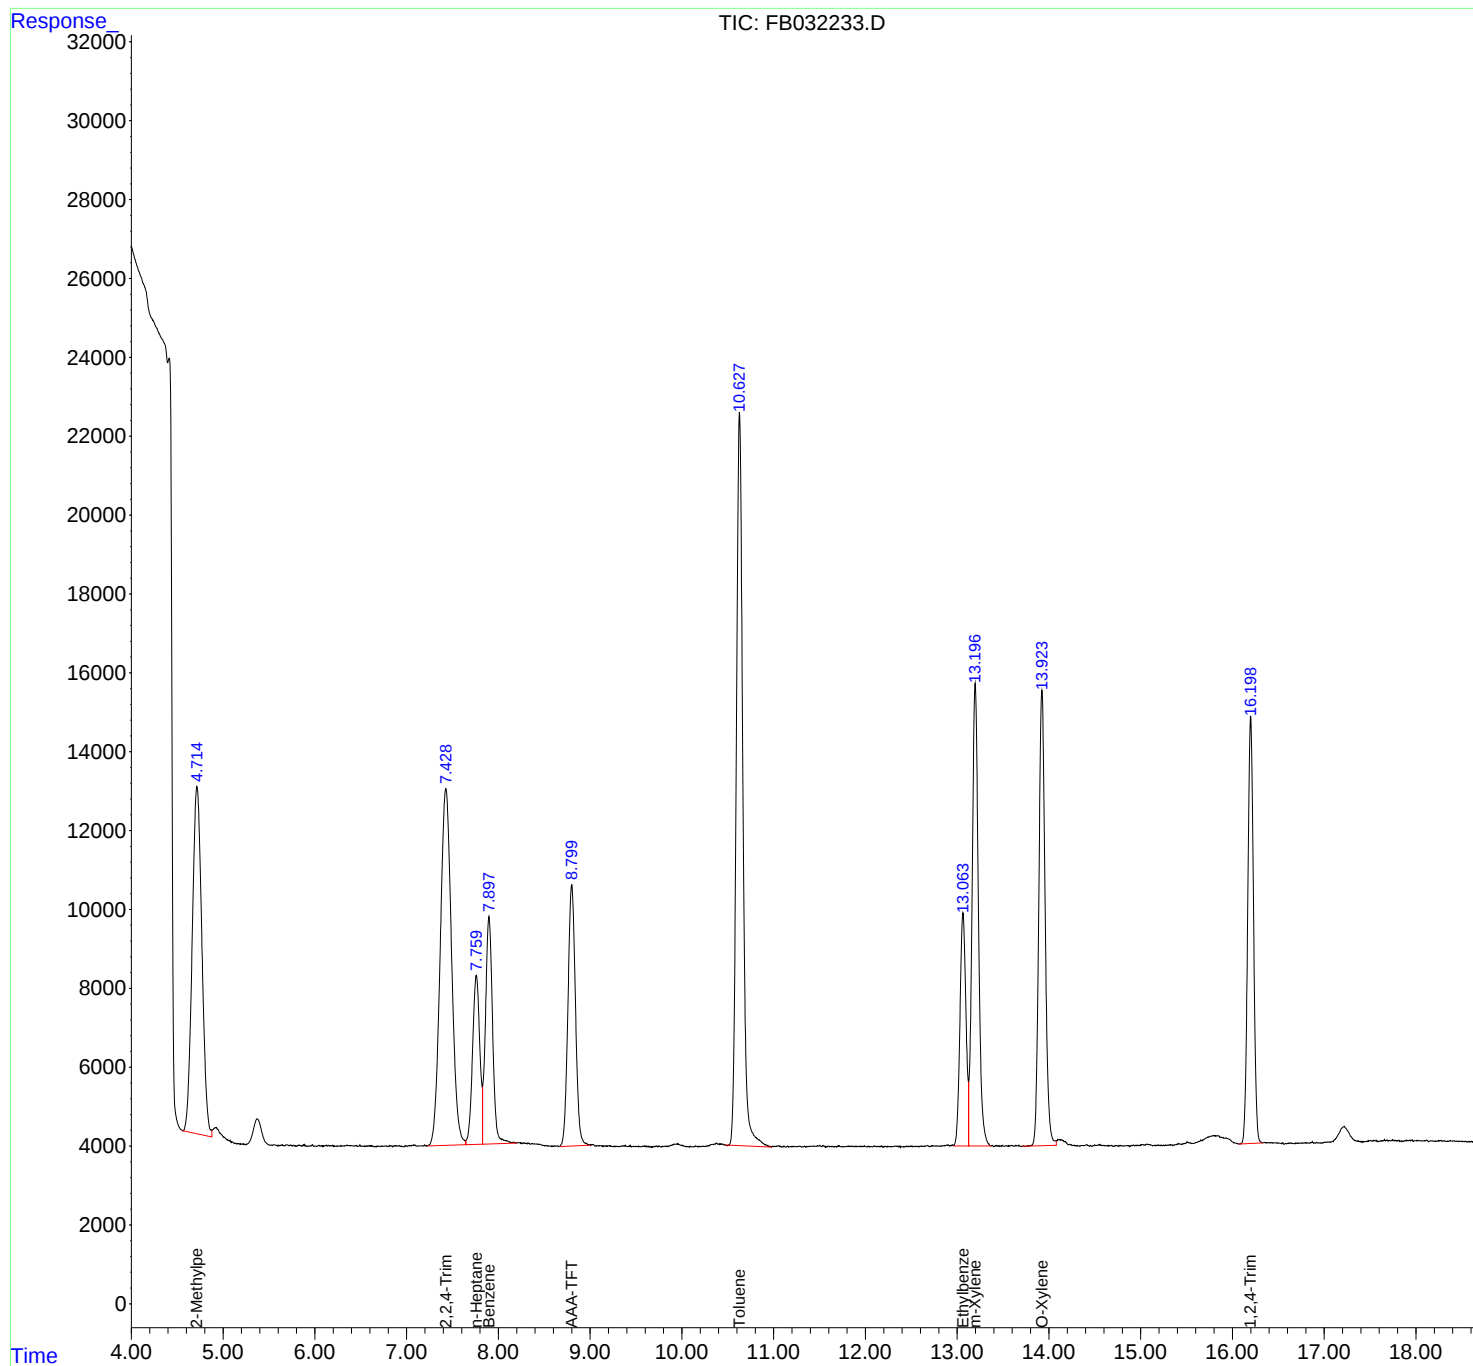


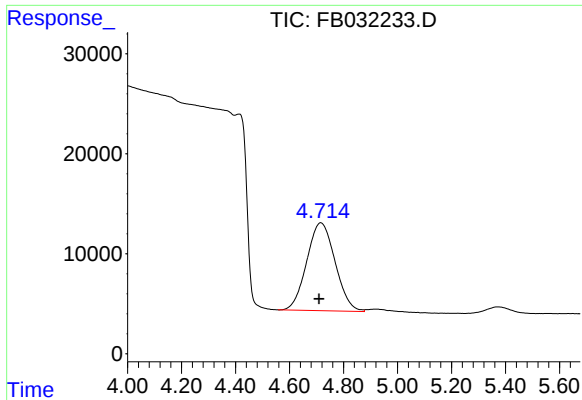

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: 0.007 min
Response: 642081
Conc: 23.78 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0923S2

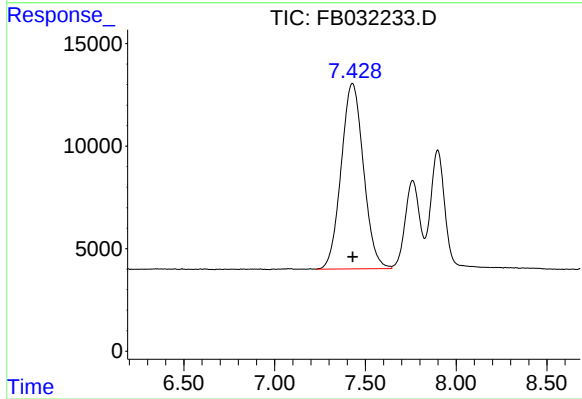


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: -0.001 min
Response: 773096
Conc: 27.37 ng/ml

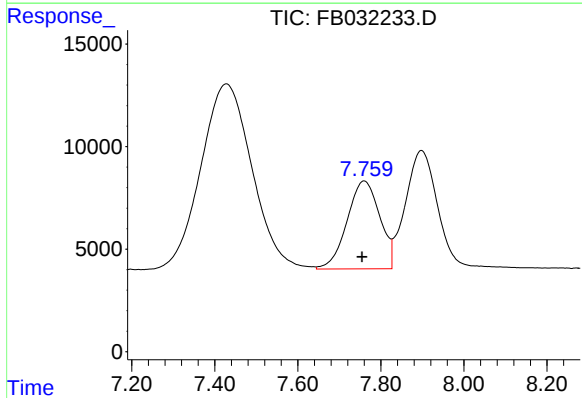


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.006 min
Response: 234490
Conc: 8.58 ng/ml

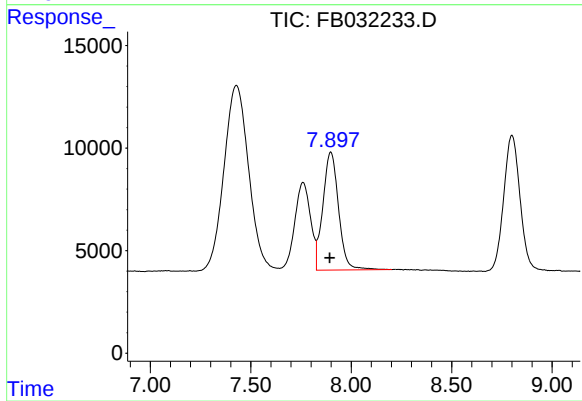

#4 Benzene


R.T.: 7.898 min
Delta R.T.: 0.005 min
Response: 313104
Conc: 8.66 ng/ml

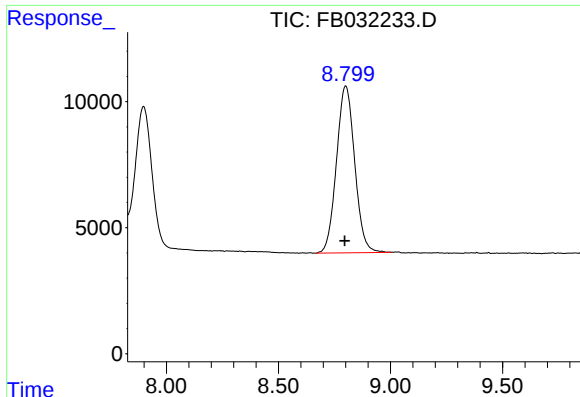

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.004 min
Response: 373996
Conc: 20.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0923S2

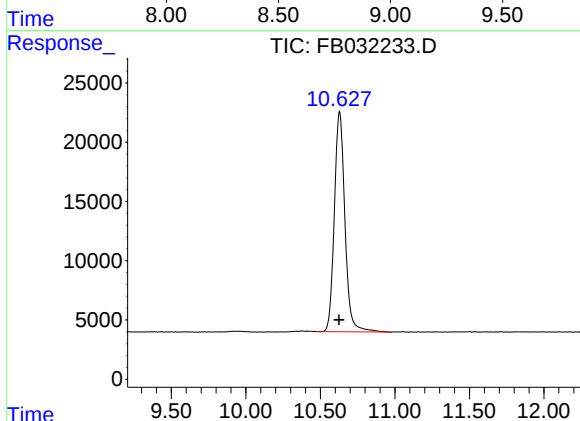


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.003 min
Response: 917032
Conc: 24.62 ng/ml

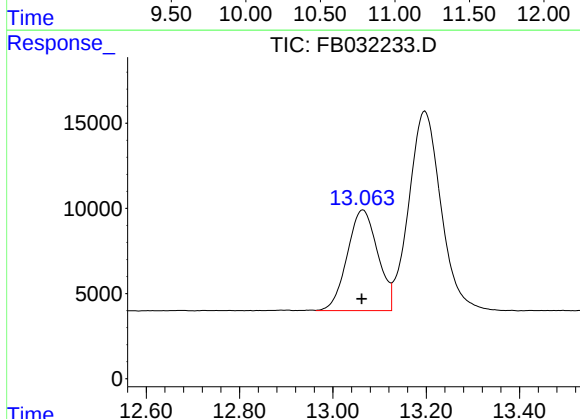


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: 0.003 min
Response: 267806
Conc: 8.19 ng/ml

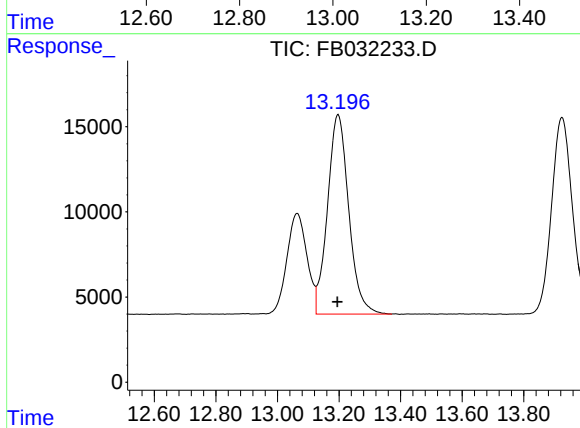

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.002 min
Response: 560582
Conc: 16.45 ng/ml

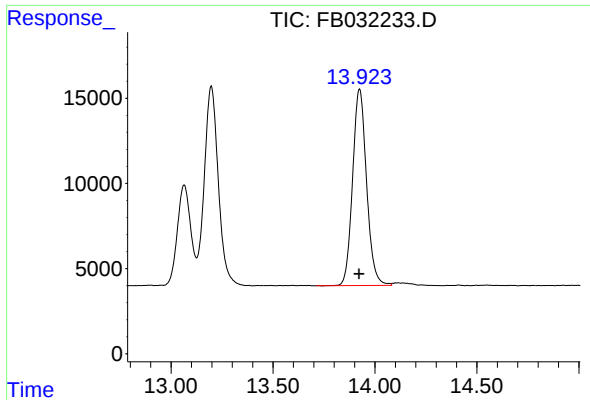

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.002 min
Response: 549054
Conc: 16.81 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0923S2

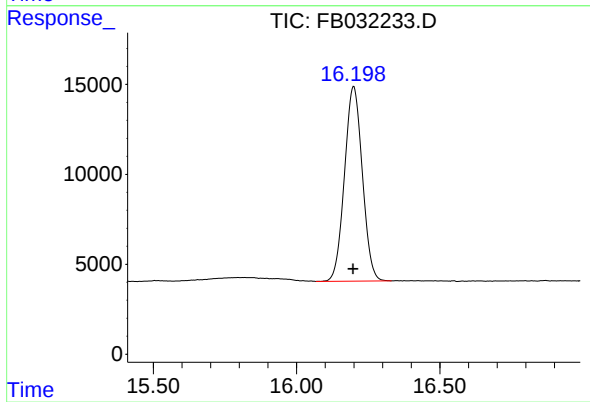

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.002 min
Response: 468859
Conc: 16.76 ng/ml