

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092418\
 Data File : FB017897.D
 Signal(s) : FID2B.CH
 Acq On : 24 Sep 2018 14:48
 Operator : MJ/SJ
 Sample : J5061-03MSD
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 24 15:47:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.104	186189	22.011 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.957	407453	25.585 ng/ml
2) t 2,2,4-Trimethylpentane	7.720	414844	26.068 ng/ml
3) t n-Heptane	8.059	128704	8.352 ng/ml
4) t Benzene	8.198	170446	8.954 ng/ml
6) t Toluene	10.954	434831	27.476 ng/ml
7) t Ethylbenzene	13.404	157488	9.638 ng/ml
8) t m-Xylene	13.536	334070	19.311 ng/ml
9) t O-Xylene	14.268	351609	19.349 ng/ml
10) t 1,2,4-Trimethylbenzene	16.551	392701	18.461 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092418\
Data File : FB017897.D
Signal(s) : FID2B.CH
Acq On : 24 Sep 2018 14:48
Operator : MJ/SJ
Sample : J5061-03MSD
Misc : 5.02g/5.00mL DI Water
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 24 15:47:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

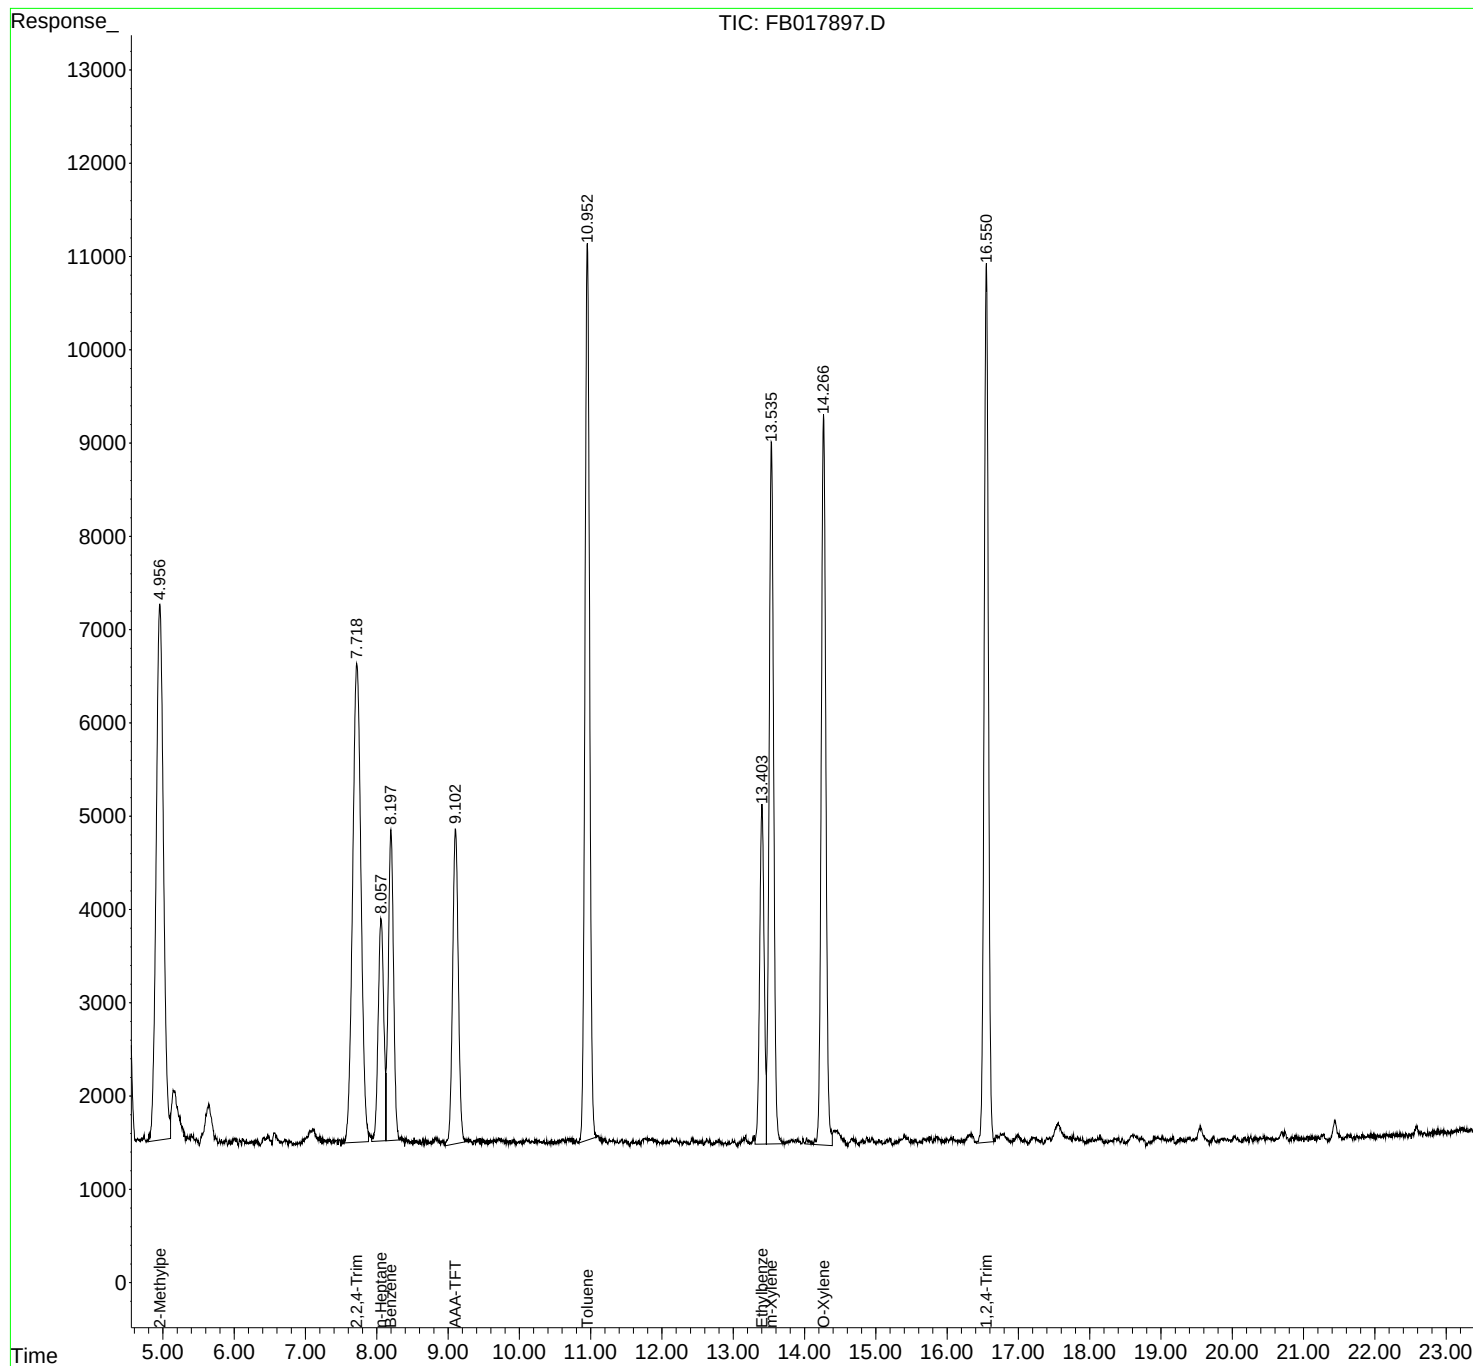

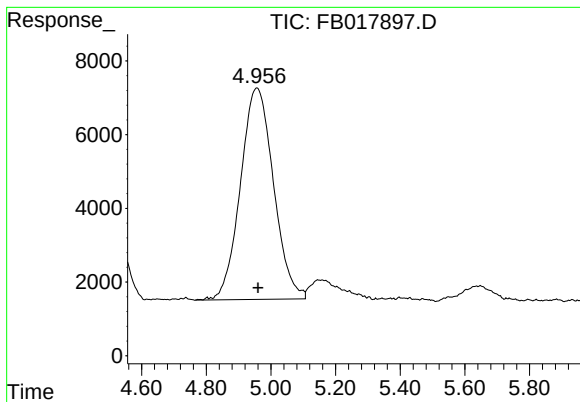


#1 2-Methylpentane

R.T.: 4.957 min
Delta R.T.: -0.003 min
Response: 407453
Conc: 25.59 ng/ml

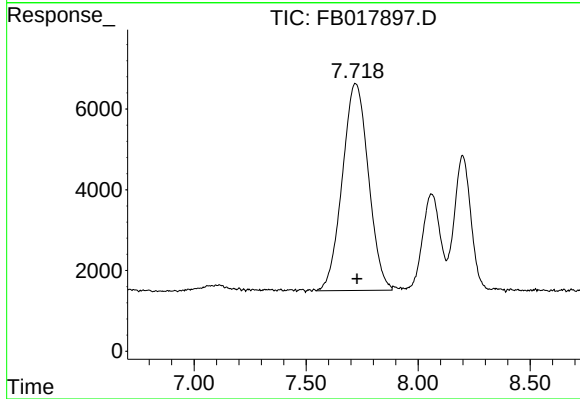


#2 2,2,4-Trimethylpentane

R.T.: 7.720 min
Delta R.T.: -0.007 min
Response: 414844
Conc: 26.07 ng/ml

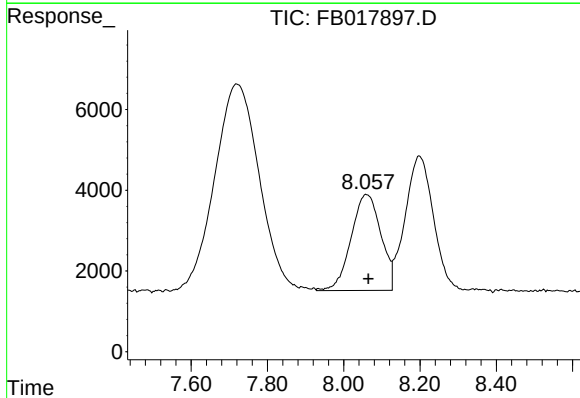


#3 n-Heptane

R.T.: 8.059 min
Delta R.T.: -0.006 min
Response: 128704
Conc: 8.35 ng/ml

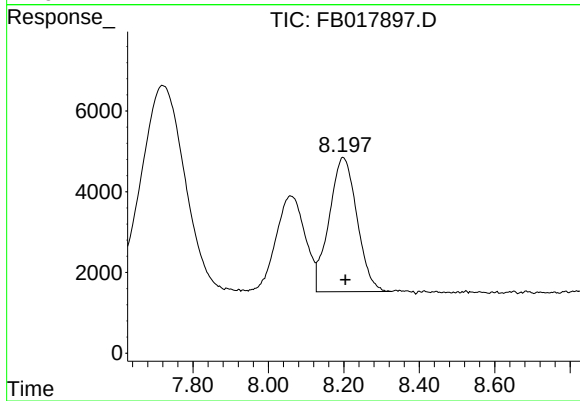


#4 Benzene

R.T.: 8.198 min
Delta R.T.: -0.006 min
Response: 170446
Conc: 8.95 ng/ml

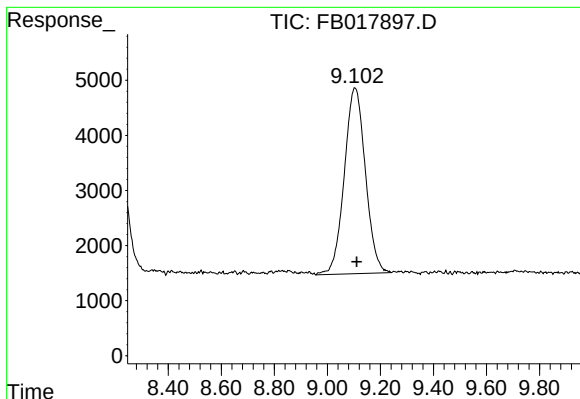


#5 AAA-TFT

R.T.: 9.104 min
Delta R.T.: -0.006 min
Response: 186189
Conc: 22.01 ng/ml

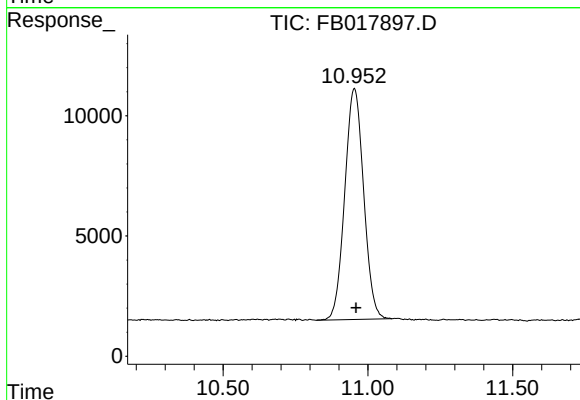


#6 Toluene

R.T.: 10.954 min
Delta R.T.: -0.005 min
Response: 434831
Conc: 27.48 ng/ml

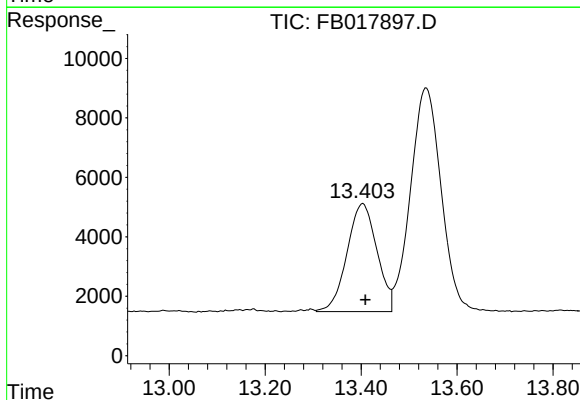


#7 Ethylbenzene

R.T.: 13.404 min
Delta R.T.: -0.005 min
Response: 157488
Conc: 9.64 ng/ml

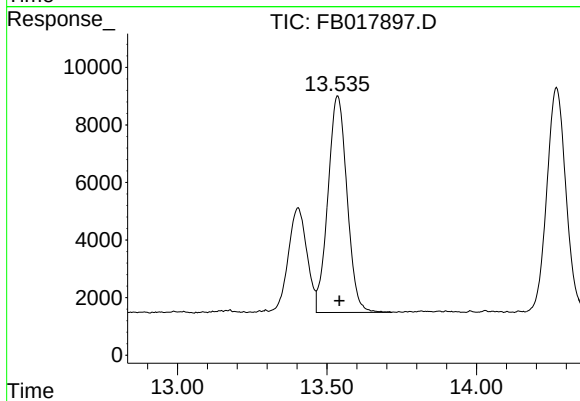


#8 m-Xylene

R.T.: 13.536 min
Delta R.T.: -0.005 min
Response: 334070
Conc: 19.31 ng/ml

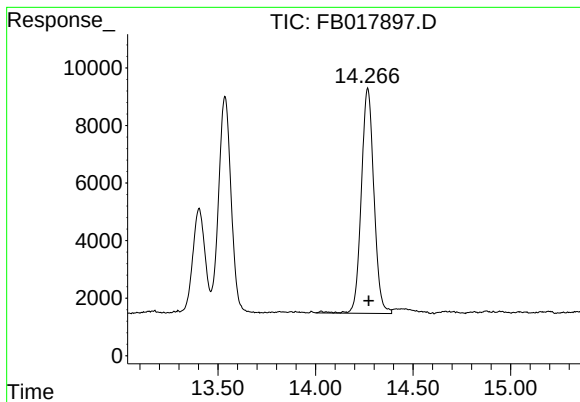

#9 O-Xylene

R.T.: 14.268 min
Delta R.T.: -0.005 min
Response: 351609
Conc: 19.35 ng/ml

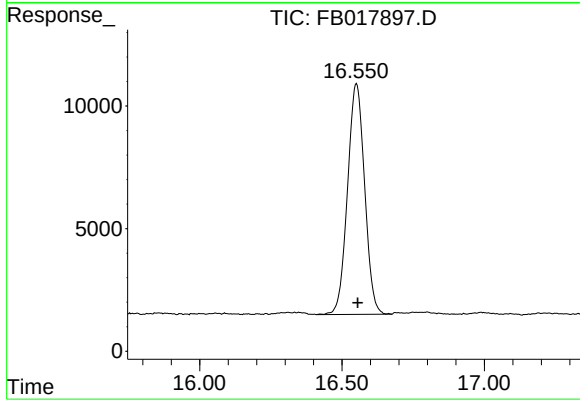

#10 1,2,4-Trimethylbenzene

R.T.: 16.551 min
Delta R.T.: -0.005 min
Response: 392701
Conc: 18.46 ng/ml