

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092418\
 Data File : FB017893.D
 Signal(s) : FID2B.CH
 Acq On : 24 Sep 2018 12:06
 Operator : MJ/SJ
 Sample : BSF0924S1
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 24 13:13:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.104	168789	19.954 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.958	433948	27.249 ng/ml
2) t 2,2,4-Trimethylpentane	7.721	451993	28.403 ng/ml
3) t n-Heptane	8.059	140475	9.116 ng/ml
4) t Benzene	8.199	183002	9.613 ng/ml
6) t Toluene	10.953	446124	28.189 ng/ml
7) t Ethylbenzene	13.403	158959	9.728 ng/ml
8) t m-Xylene	13.536	340102	19.659 ng/ml
9) t O-Xylene	14.267	358009	19.701 ng/ml
10) t 1,2,4-Trimethylbenzene	16.550	405654	19.070 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092418\
Data File : FB017893.D
Signal(s) : FID2B.CH
Acq On : 24 Sep 2018 12:06
Operator : MJ/SJ
Sample : BSF0924S1
Misc : 5.01g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 24 13:13:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

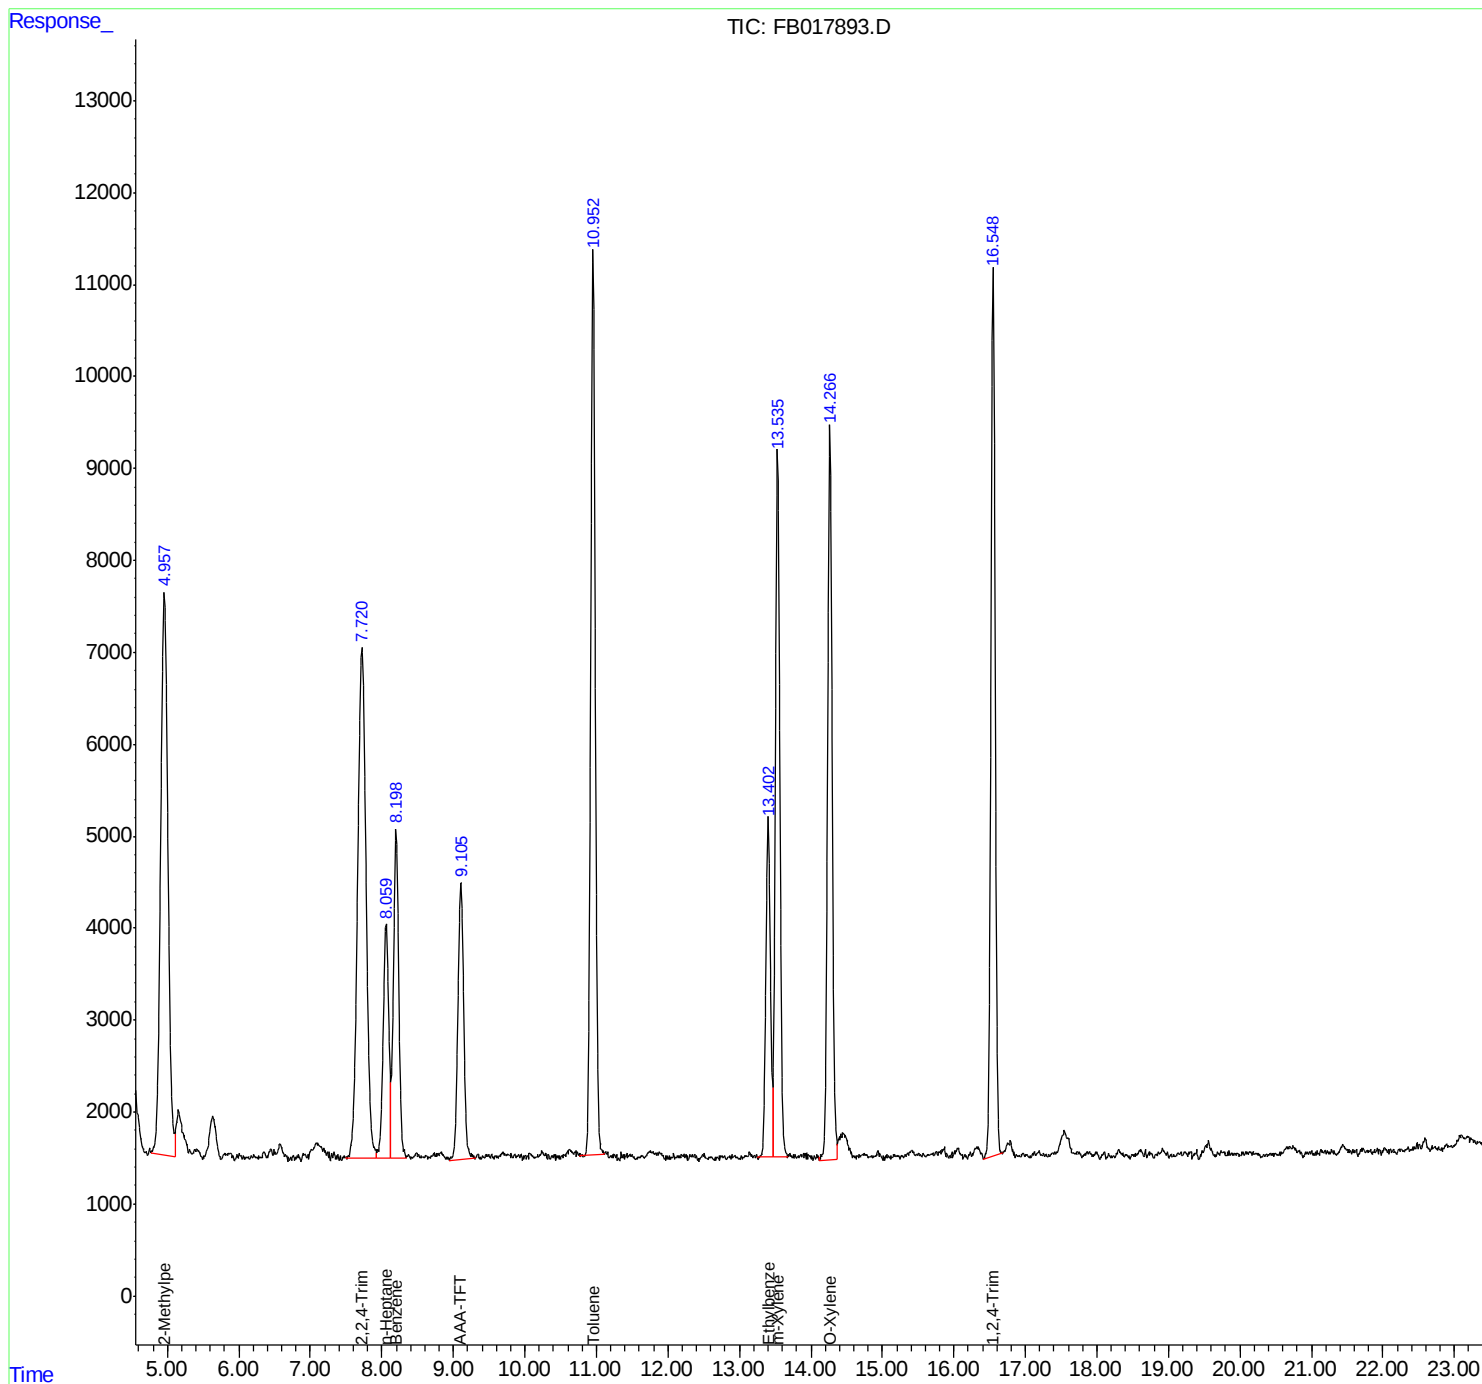

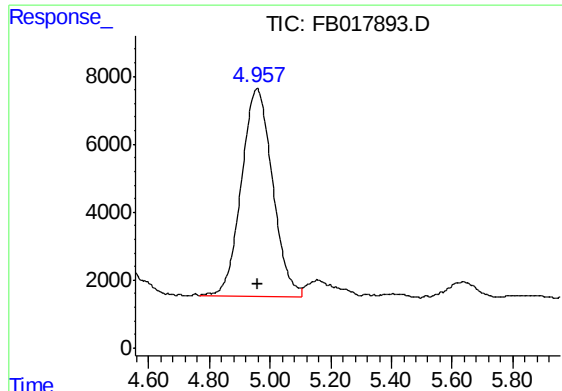


#1 2-Methylpentane

R.T.: 4.958 min
Delta R.T.: -0.002 min
Response: 433948
Conc: 27.25 ng/ml

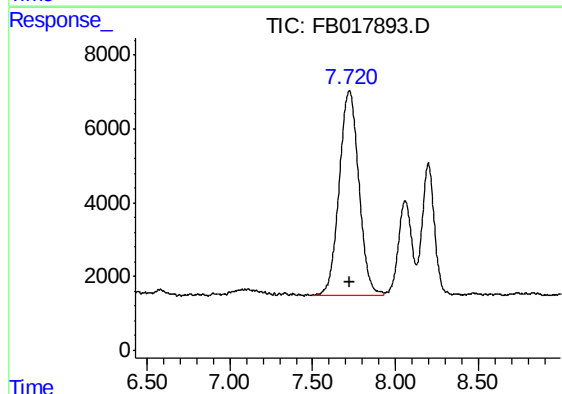


#2 2,2,4-Trimethylpentane

R.T.: 7.721 min
Delta R.T.: -0.006 min
Response: 451993
Conc: 28.40 ng/ml

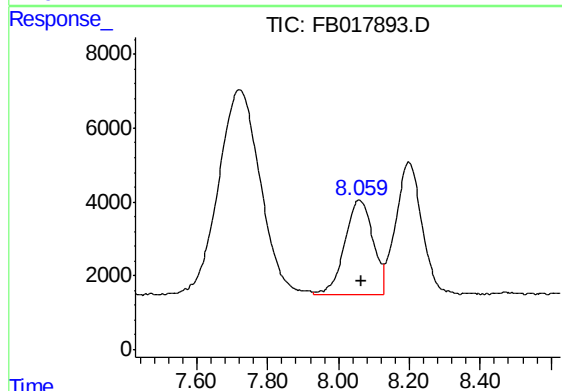


#3 n-Heptane

R.T.: 8.059 min
Delta R.T.: -0.006 min
Response: 140475
Conc: 9.12 ng/ml

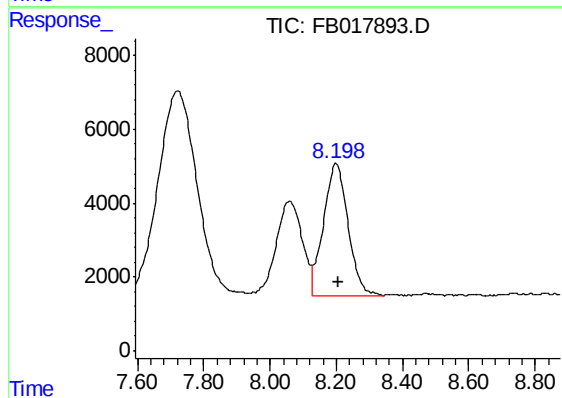


#4 Benzene

R.T.: 8.199 min
Delta R.T.: -0.005 min
Response: 183002
Conc: 9.61 ng/ml

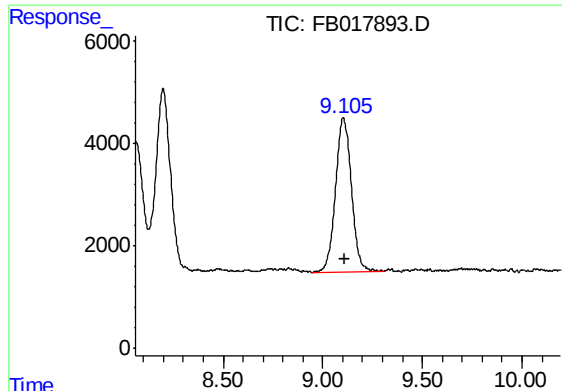


#5 AAA-TFT

R.T.: 9.104 min
Delta R.T.: -0.006 min
Response: 168789
Conc: 19.95 ng/ml

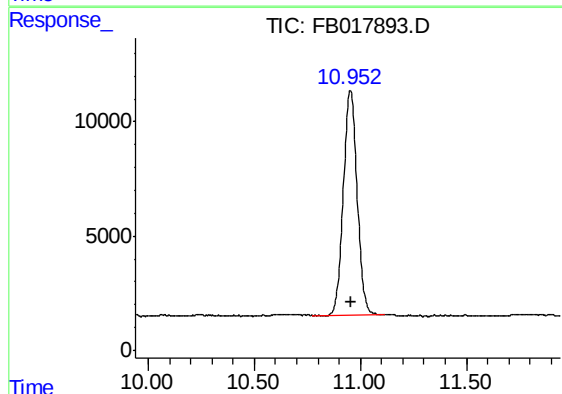


#6 Toluene

R.T.: 10.953 min
Delta R.T.: -0.006 min
Response: 446124
Conc: 28.19 ng/ml

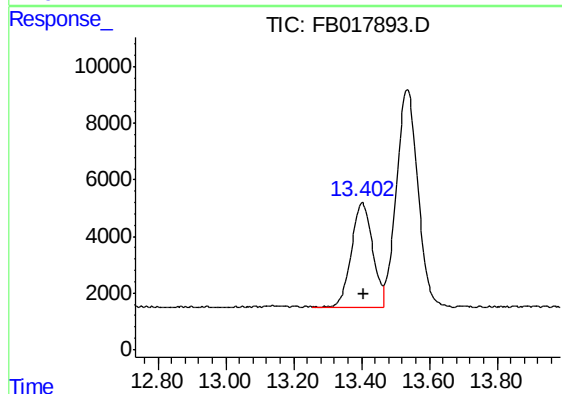


#7 Ethylbenzene

R.T.: 13.403 min
Delta R.T.: -0.006 min
Response: 158959
Conc: 9.73 ng/ml

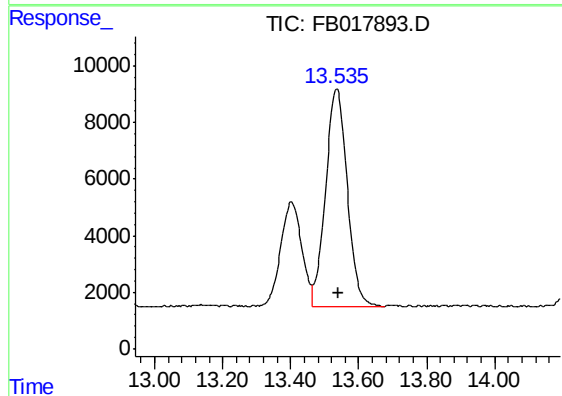


#8 m-Xylene

R.T.: 13.536 min
Delta R.T.: -0.006 min
Response: 340102
Conc: 19.66 ng/ml

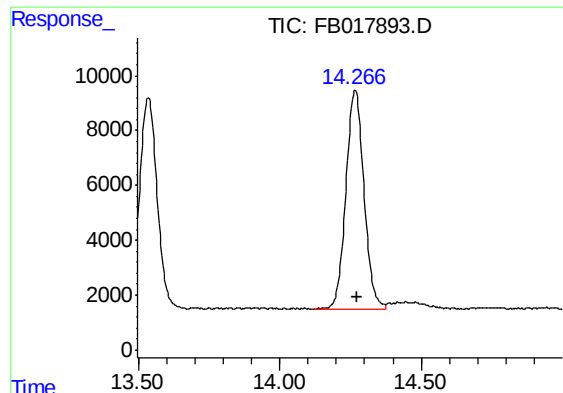

#9 O-Xylene

R.T.: 14.267 min
Delta R.T.: -0.006 min
Response: 358009
Conc: 19.70 ng/ml

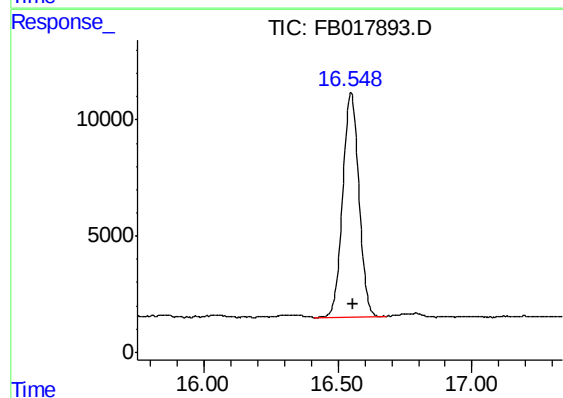

#10 1,2,4-Trimethylbenzene

R.T.: 16.550 min
Delta R.T.: -0.006 min
Response: 405654
Conc: 19.07 ng/ml