

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092418\
 Data File : FB017896.D
 Signal(s) : FID2B.CH
 Acq On : 24 Sep 2018 14:19
 Operator : MJ/SJ
 Sample : J5061-03MS
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 24 15:47:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.105	177679	21.005 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.958	414785	26.046 ng/ml
2) t 2,2,4-Trimethylpentane	7.721	425920	26.764 ng/ml
3) t n-Heptane	8.060	134725	8.742 ng/ml
4) t Benzene	8.200	175053	9.196 ng/ml
6) t Toluene	10.954	443506	28.024 ng/ml
7) t Ethylbenzene	13.403	159428	9.757 ng/ml
8) t m-Xylene	13.536	340526	19.684 ng/ml
9) t O-Xylene	14.267	351250	19.329 ng/ml
10) t 1,2,4-Trimethylbenzene	16.550	397826	18.702 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092418\
Data File : FB017896.D
Signal(s) : FID2B.CH
Acq On : 24 Sep 2018 14:19
Operator : MJ/SJ
Sample : J5061-03MS
Misc : 5.01g/5.00mL DI Water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 24 15:47:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

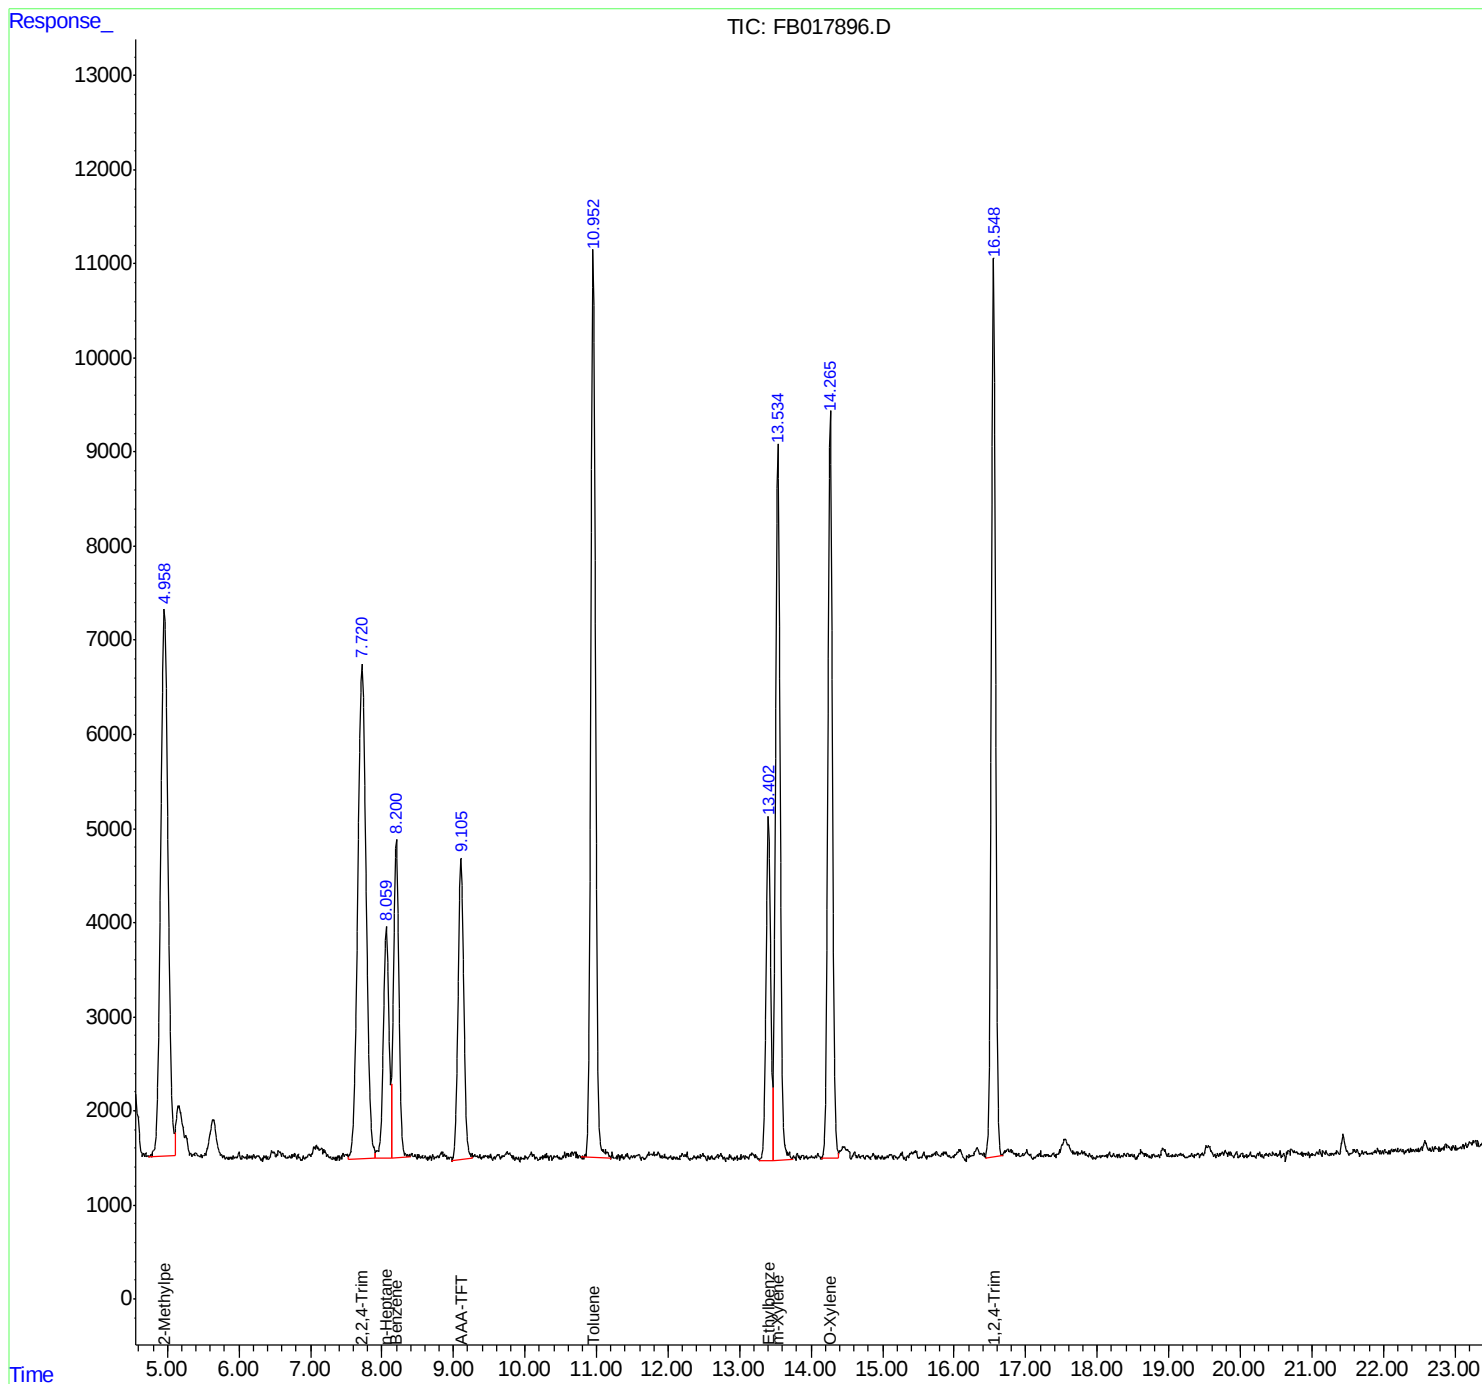

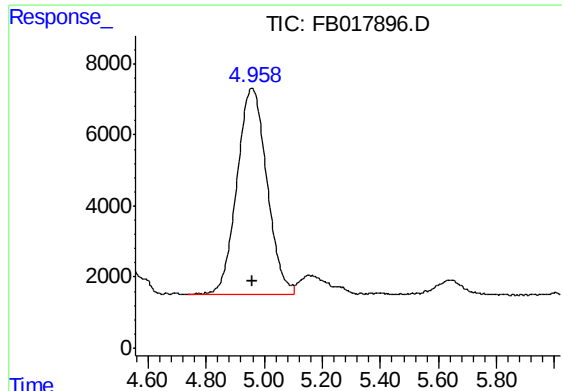


#1 2-Methylpentane

R.T.: 4.958 min
Delta R.T.: -0.002 min
Response: 414785
Conc: 26.05 ng/ml

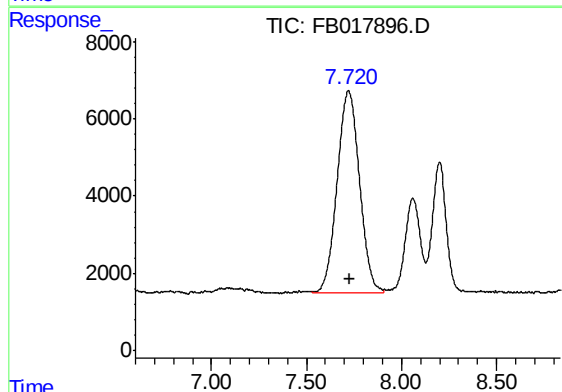


#2 2,2,4-Trimethylpentane

R.T.: 7.721 min
Delta R.T.: -0.006 min
Response: 425920
Conc: 26.76 ng/ml

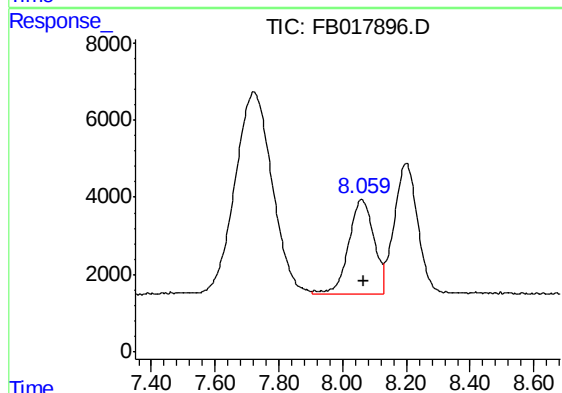


#3 n-Heptane

R.T.: 8.060 min
Delta R.T.: -0.005 min
Response: 134725
Conc: 8.74 ng/ml

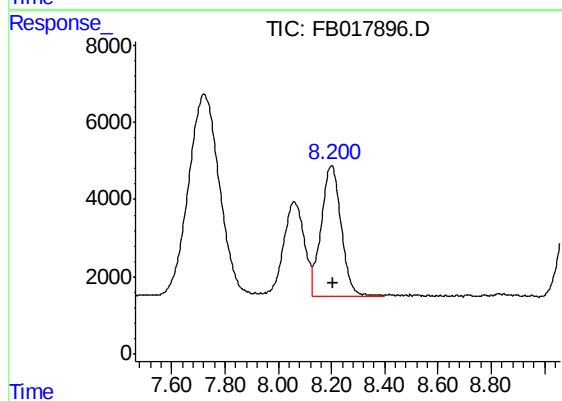


#4 Benzene

R.T.: 8.200 min
Delta R.T.: -0.004 min
Response: 175053
Conc: 9.20 ng/ml

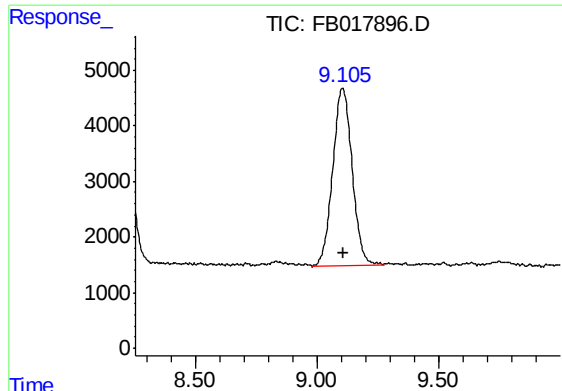


#5 AAA-TFT

R.T.: 9.105 min
Delta R.T.: -0.005 min
Response: 177679
Conc: 21.01 ng/ml

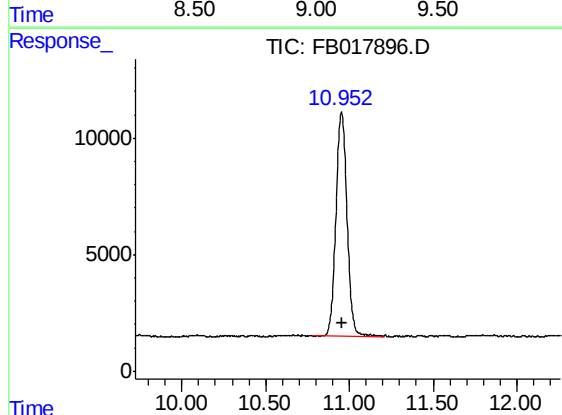


#6 Toluene

R.T.: 10.954 min
Delta R.T.: -0.006 min
Response: 443506
Conc: 28.02 ng/ml

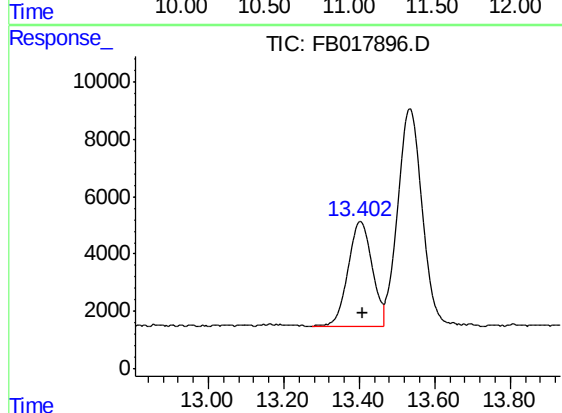


#7 Ethylbenzene

R.T.: 13.403 min
Delta R.T.: -0.006 min
Response: 159428
Conc: 9.76 ng/ml

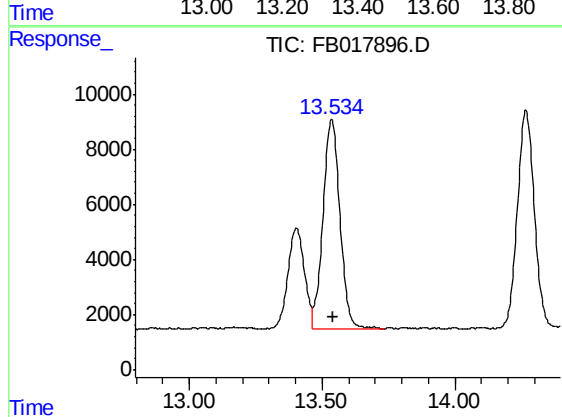


#8 m-Xylene

R.T.: 13.536 min
Delta R.T.: -0.006 min
Response: 340526
Conc: 19.68 ng/ml

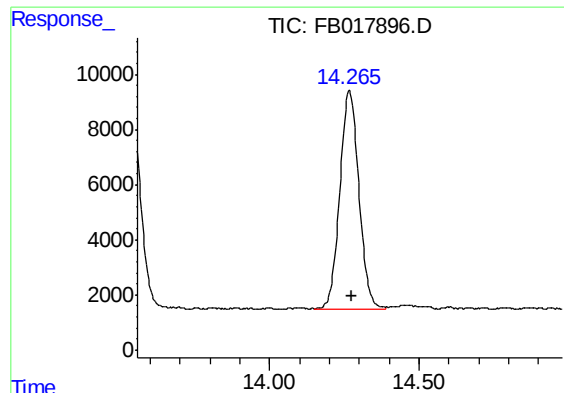

#9 O-Xylene

R.T.: 14.267 min
Delta R.T.: -0.006 min
Response: 351250
Conc: 19.33 ng/ml

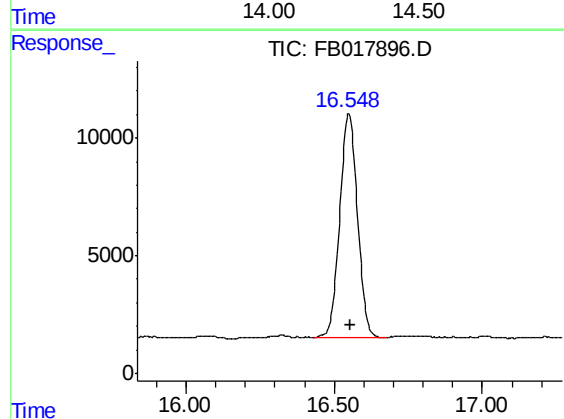

#10 1,2,4-Trimethylbenzene

R.T.: 16.550 min
Delta R.T.: -0.006 min
Response: 397826
Conc: 18.70 ng/ml