

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092618\
 Data File : FB017982.D
 Signal(s) : FID2B.CH
 Acq On : 26 Sep 2018 22:26
 Operator : MJ/SJ
 Sample : J5097-06MSD
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 27 08:14:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.109	182222	21.542 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.960	375625	23.587 ng/ml
2) t 2,2,4-Trimethylpentane	7.725	384188	24.142 ng/ml
3) t n-Heptane	8.063	123018	7.983 ng/ml
4) t Benzene	8.204	153038	8.039 ng/ml
6) t Toluene	10.958	408131	25.788 ng/ml
7) t Ethylbenzene	13.408	146864	8.988 ng/ml
8) t m-Xylene	13.541	307156	17.755 ng/ml
9) t O-Xylene	14.272	325009	17.885 ng/ml
10) t 1,2,4-Trimethylbenzene	16.555	365374	17.177 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092618\
Data File : FB017982.D
Signal(s) : FID2B.CH
Acq On : 26 Sep 2018 22:26
Operator : MJ/SJ
Sample : J5097-06MSD
Misc : 5.00g/5.00mL DI Water
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 27 08:14:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

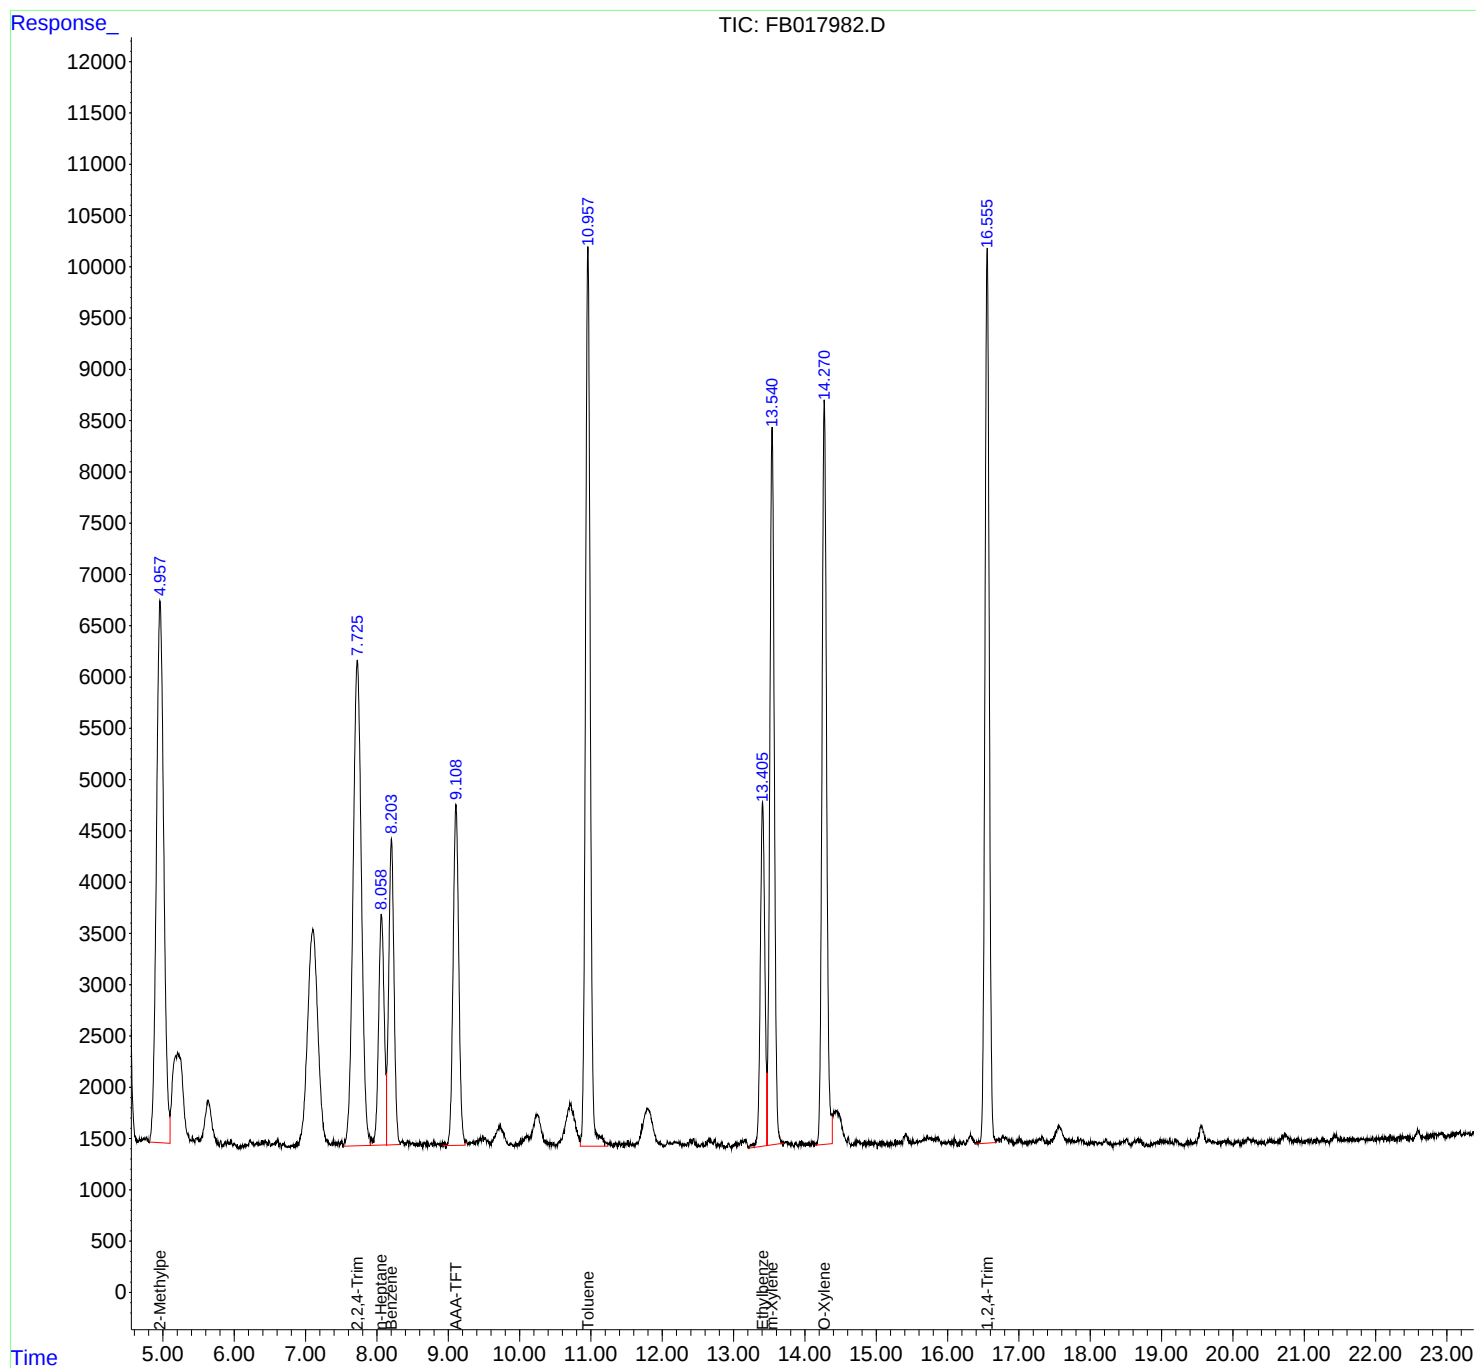

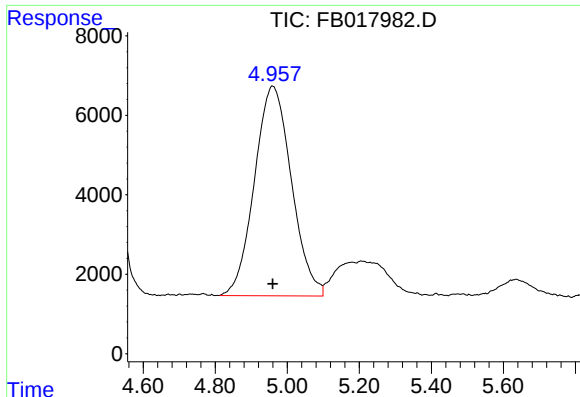


#1 2-Methylpentane

R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 375625
Conc: 23.59 ng/ml

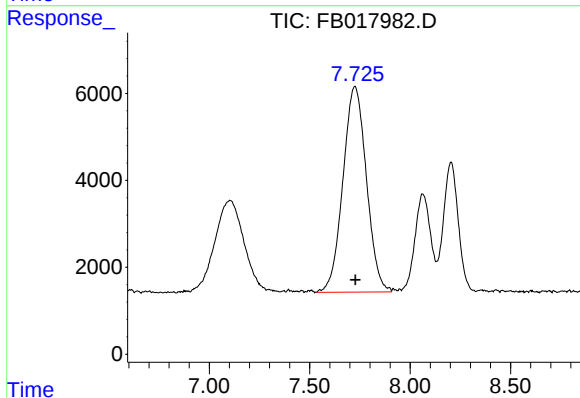


#2 2,2,4-Trimethylpentane

R.T.: 7.725 min
Delta R.T.: -0.002 min
Response: 384188
Conc: 24.14 ng/ml

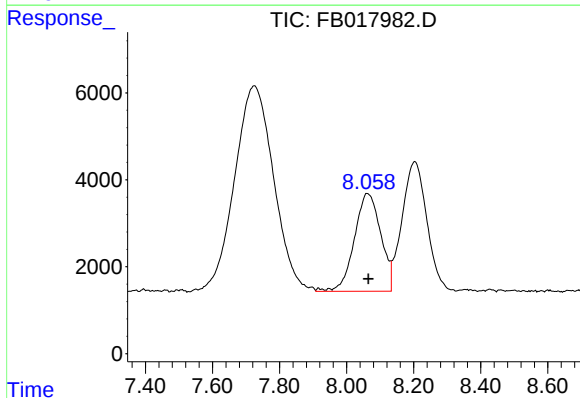


#3 n-Heptane

R.T.: 8.063 min
Delta R.T.: -0.002 min
Response: 123018
Conc: 7.98 ng/ml

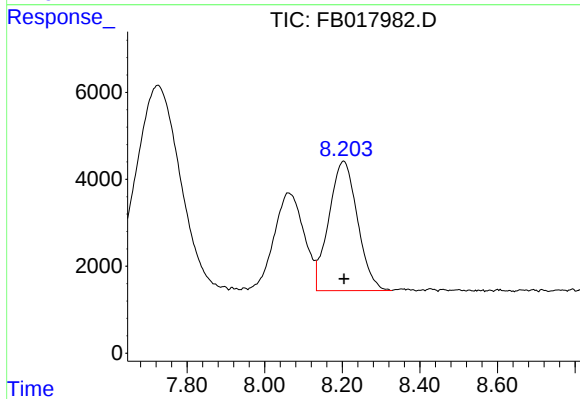


#4 Benzene

R.T.: 8.204 min
Delta R.T.: 0.000 min
Response: 153038
Conc: 8.04 ng/ml

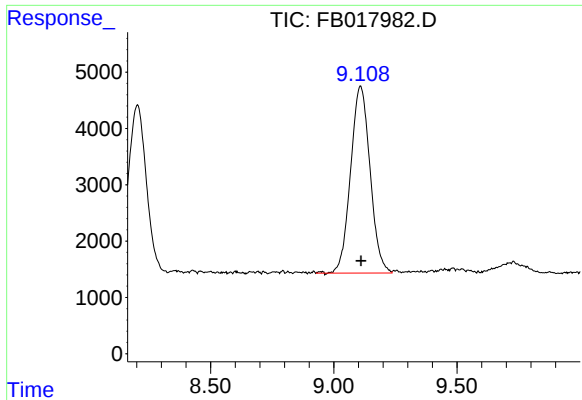


#5 AAA-TFT

R.T.: 9.109 min
Delta R.T.: -0.001 min
Response: 182222
Conc: 21.54 ng/ml

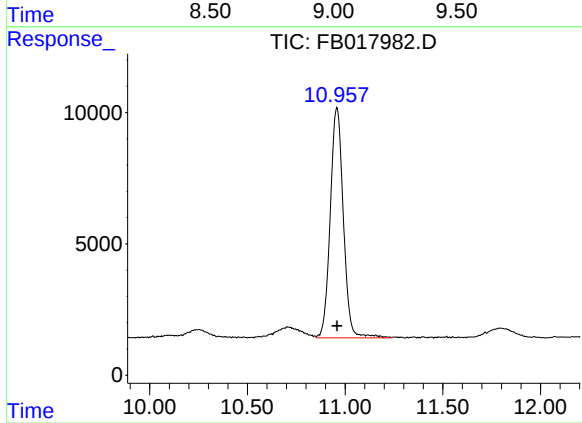


#6 Toluene

R.T.: 10.958 min
Delta R.T.: -0.001 min
Response: 408131
Conc: 25.79 ng/ml

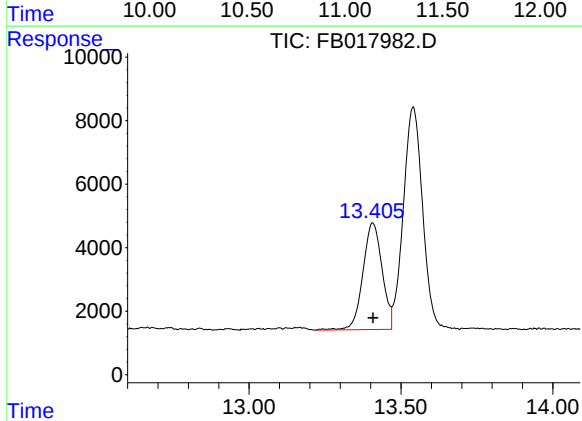


#7 Ethylbenzene

R.T.: 13.408 min
Delta R.T.: -0.001 min
Response: 146864
Conc: 8.99 ng/ml

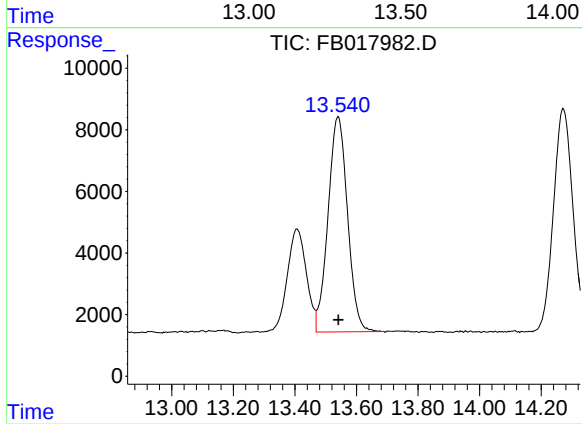


#8 m-Xylene

R.T.: 13.541 min
Delta R.T.: 0.000 min
Response: 307156
Conc: 17.75 ng/ml

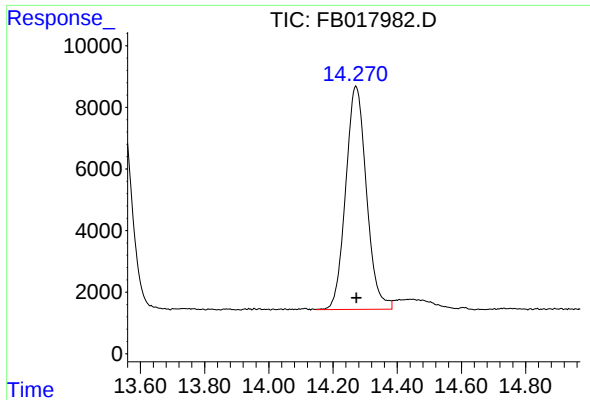

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: 0.000 min
Response: 325009
Conc: 17.88 ng/ml

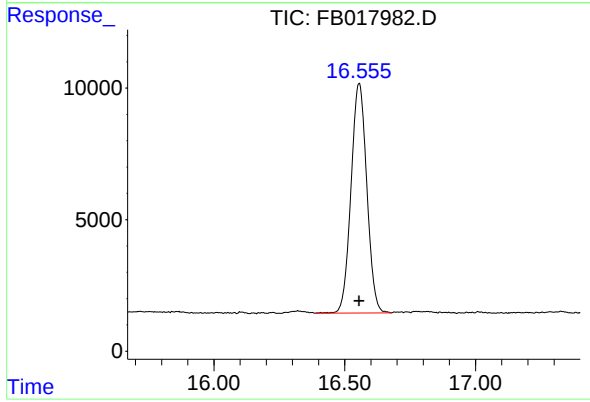

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: 0.000 min
Response: 365374
Conc: 17.18 ng/ml