

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100825\
 Data File : FB032251.D
 Signal(s) : FID2B.CH
 Acq On : 8 Oct 2025 17:29
 Operator : YP/AJ
 Sample : BSF1008S3
 Misc : 4.38G/5.00 ML MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1008S3

Integration File: Calibrat.e
 Quant Time: Oct 09 04:15:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
 Quant Title :
 QLast Update : Mon Sep 22 12:16:10 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	374873	20.943 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	838986	31.066 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	962222	34.063 ng/ml
3) t n-Heptane	7.759	298883	10.939 ng/ml
4) t Benzene	7.897	373216	10.327 ng/ml
6) t Toluene	10.628	1117873	30.014 ng/ml
7) t Ethylbenzene	13.064	322762	9.874 ng/ml
8) t m-Xylene	13.197	674186	19.780 ng/ml
9) t O-Xylene	13.924	651850	19.962 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	549892	19.659 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100825\
Data File : FB032251.D
Signal(s) : FID2B.CH
Acq On : 8 Oct 2025 17:29
Operator : YP/AJ
Sample : BSF1008S3
Misc : 4.38G/5.00 ML MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1008S3

Integration File: Calibrat.e
Quant Time: Oct 09 04:15:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

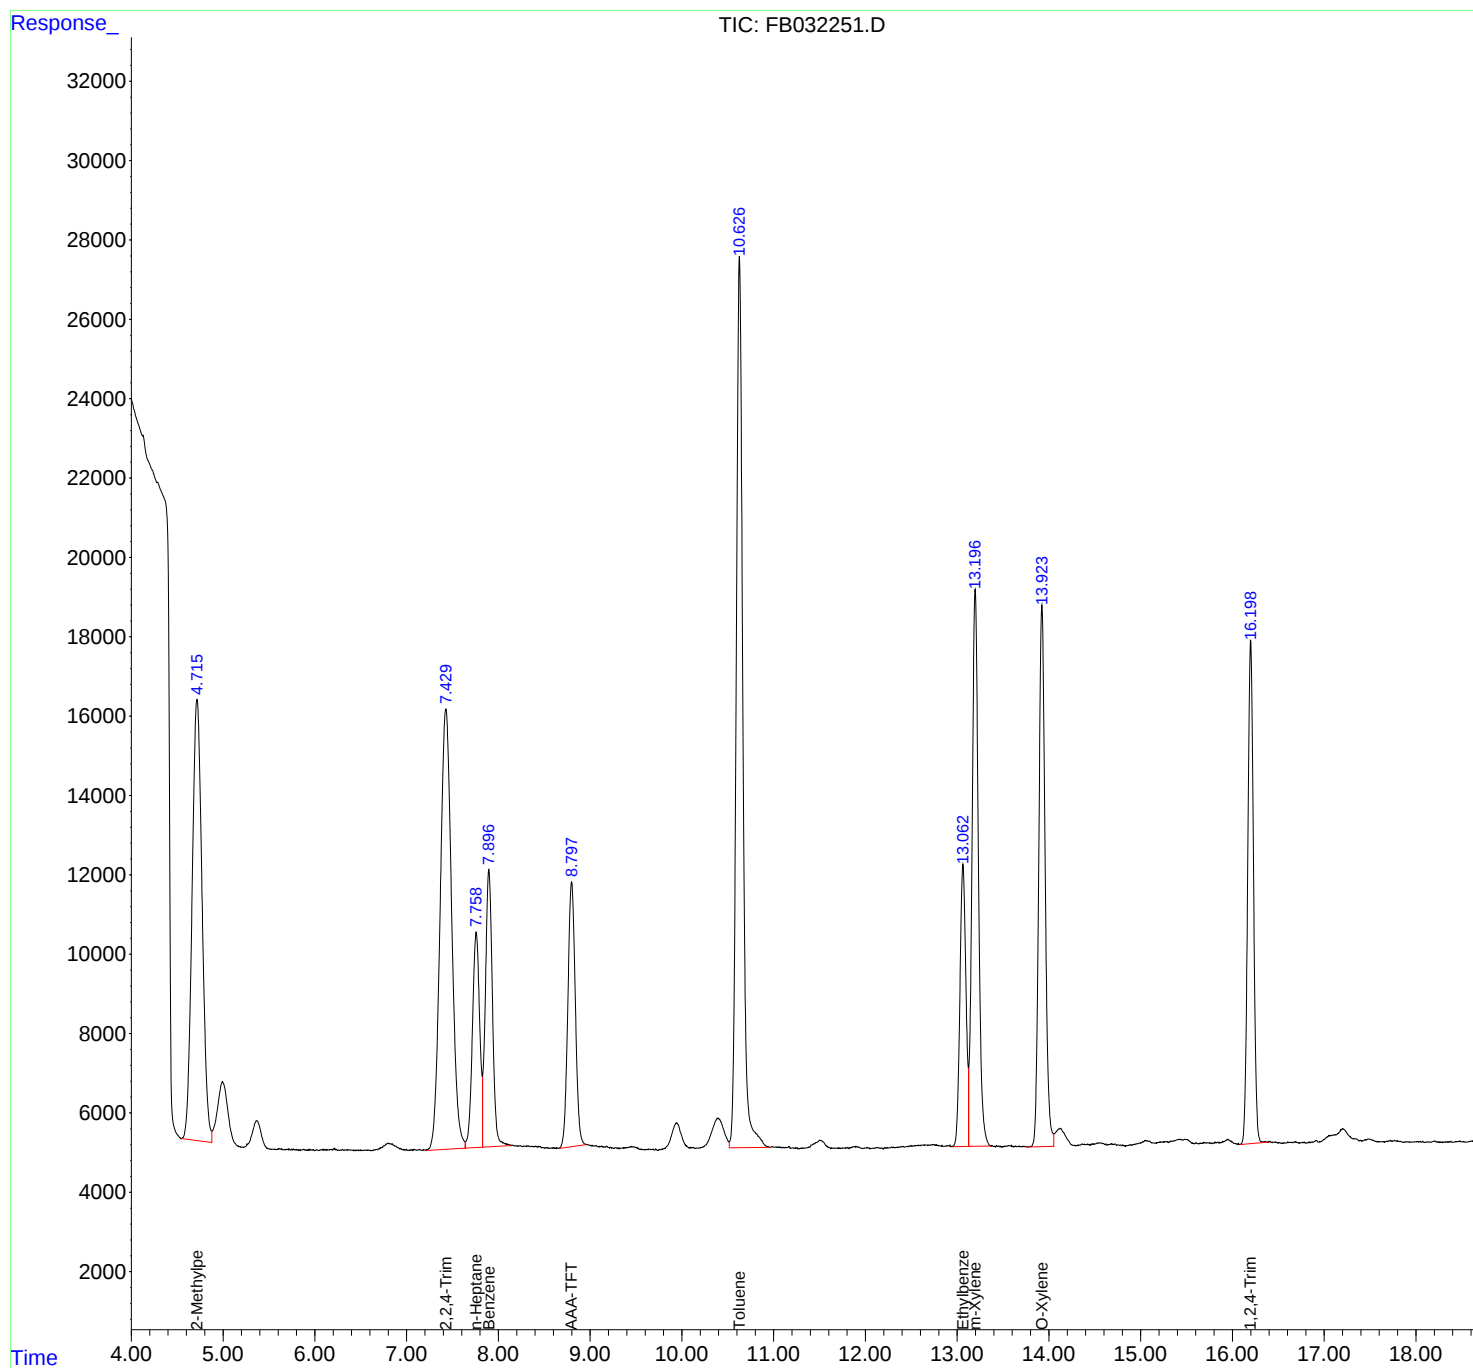


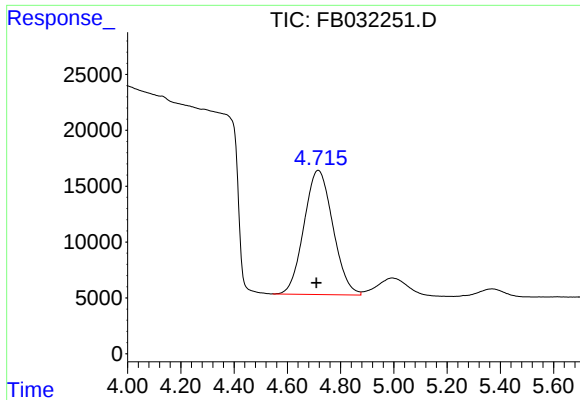

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: 0.008 min
Response: 838986
Conc: 31.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1008S3

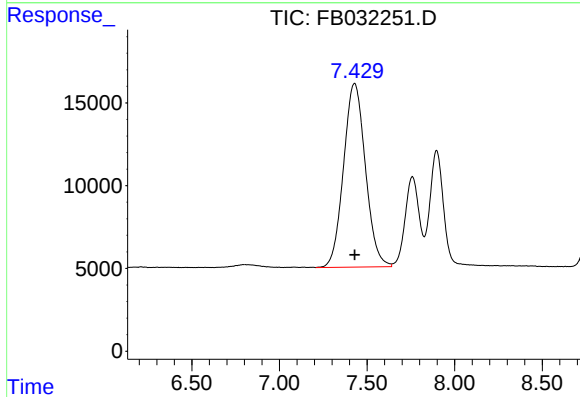


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: 0.000 min
Response: 962222
Conc: 34.06 ng/ml

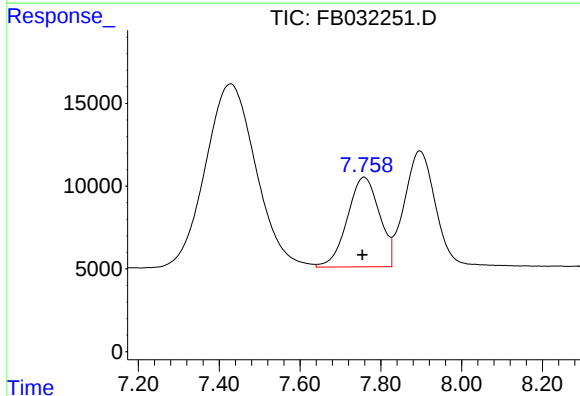


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.004 min
Response: 298883
Conc: 10.94 ng/ml

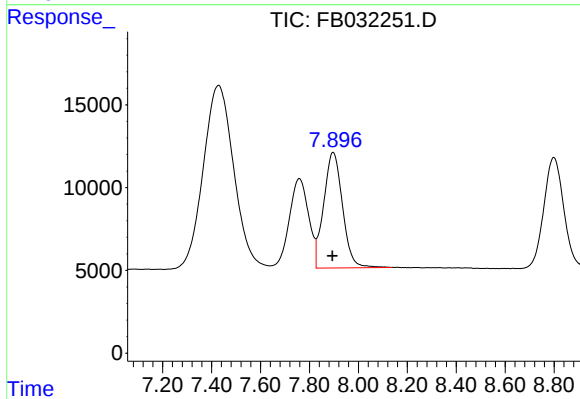

#4 Benzene


R.T.: 7.897 min
Delta R.T.: 0.004 min
Response: 373216
Conc: 10.33 ng/ml

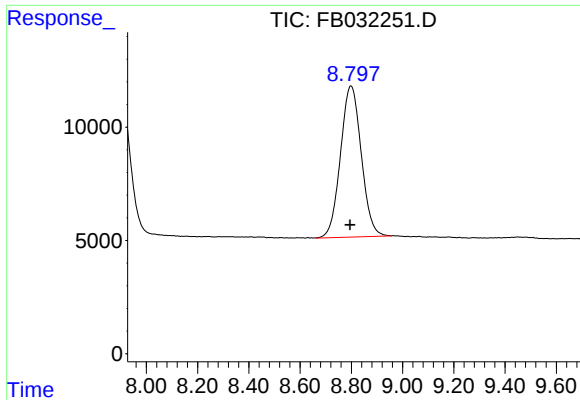

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.003 min
Response: 374873
Conc: 20.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1008S3

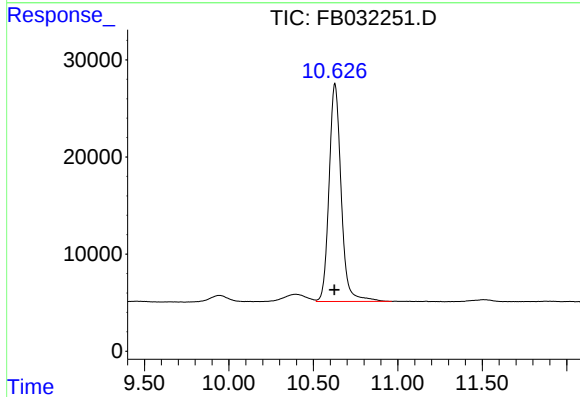


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.002 min
Response: 1117873
Conc: 30.01 ng/ml

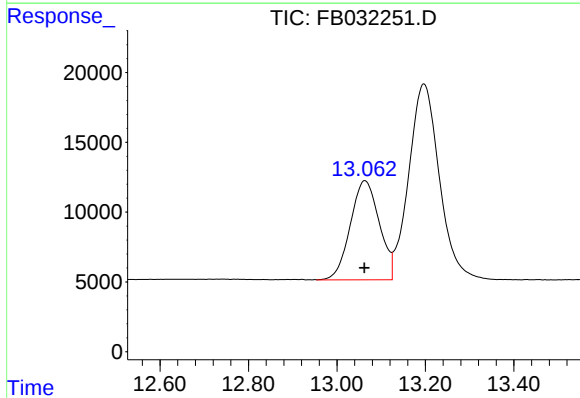


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.002 min
Response: 322762
Conc: 9.87 ng/ml

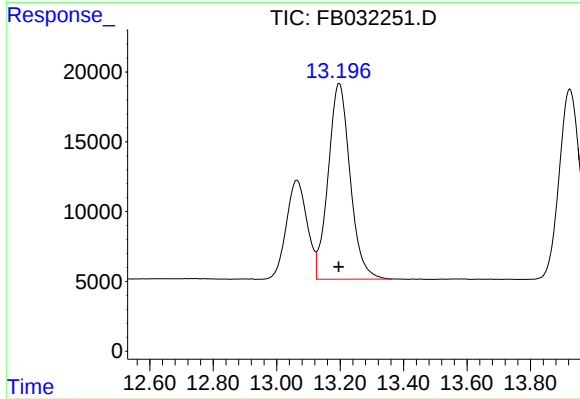

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.002 min
Response: 674186
Conc: 19.78 ng/ml

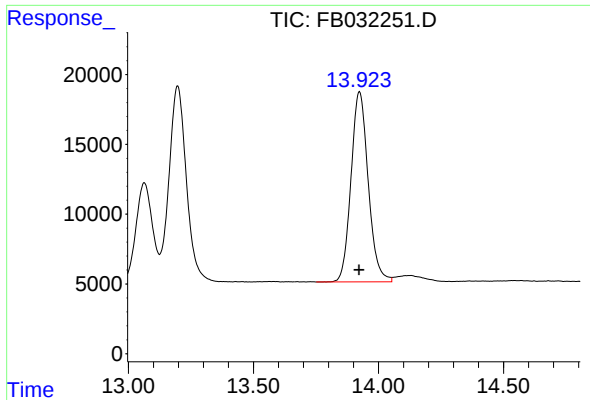

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.001 min
Response: 651850
Conc: 19.96 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1008S3

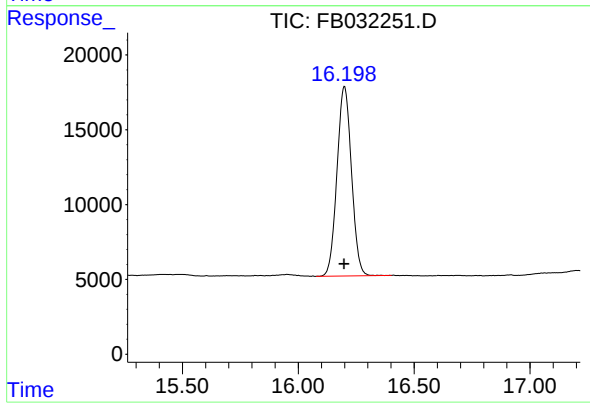

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.002 min
Response: 549892
Conc: 19.66 ng/ml