

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101725\
 Data File : FB032258.D
 Signal(s) : FID2B.CH
 Acq On : 17 Oct 2025 12:12
 Operator : YP/AJ
 Sample : Q3367-01
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibrat.e
 Quant Time: Oct 17 23:04:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
 Quant Title :
 QLast Update : Mon Sep 22 12:16:10 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	328416	18.348 ng/ml
Target Compounds			
8) t m-Xylene	13.193	6519	0.191 ng/ml
9) t O-Xylene	13.917	5617	0.172 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	43015	1.538 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101725\
Data File : FB032258.D
Signal(s) : FID2B.CH
Acq On : 17 Oct 2025 12:12
Operator : YP/AJ
Sample : Q3367-01
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibrat.e
Quant Time: Oct 17 23:04:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

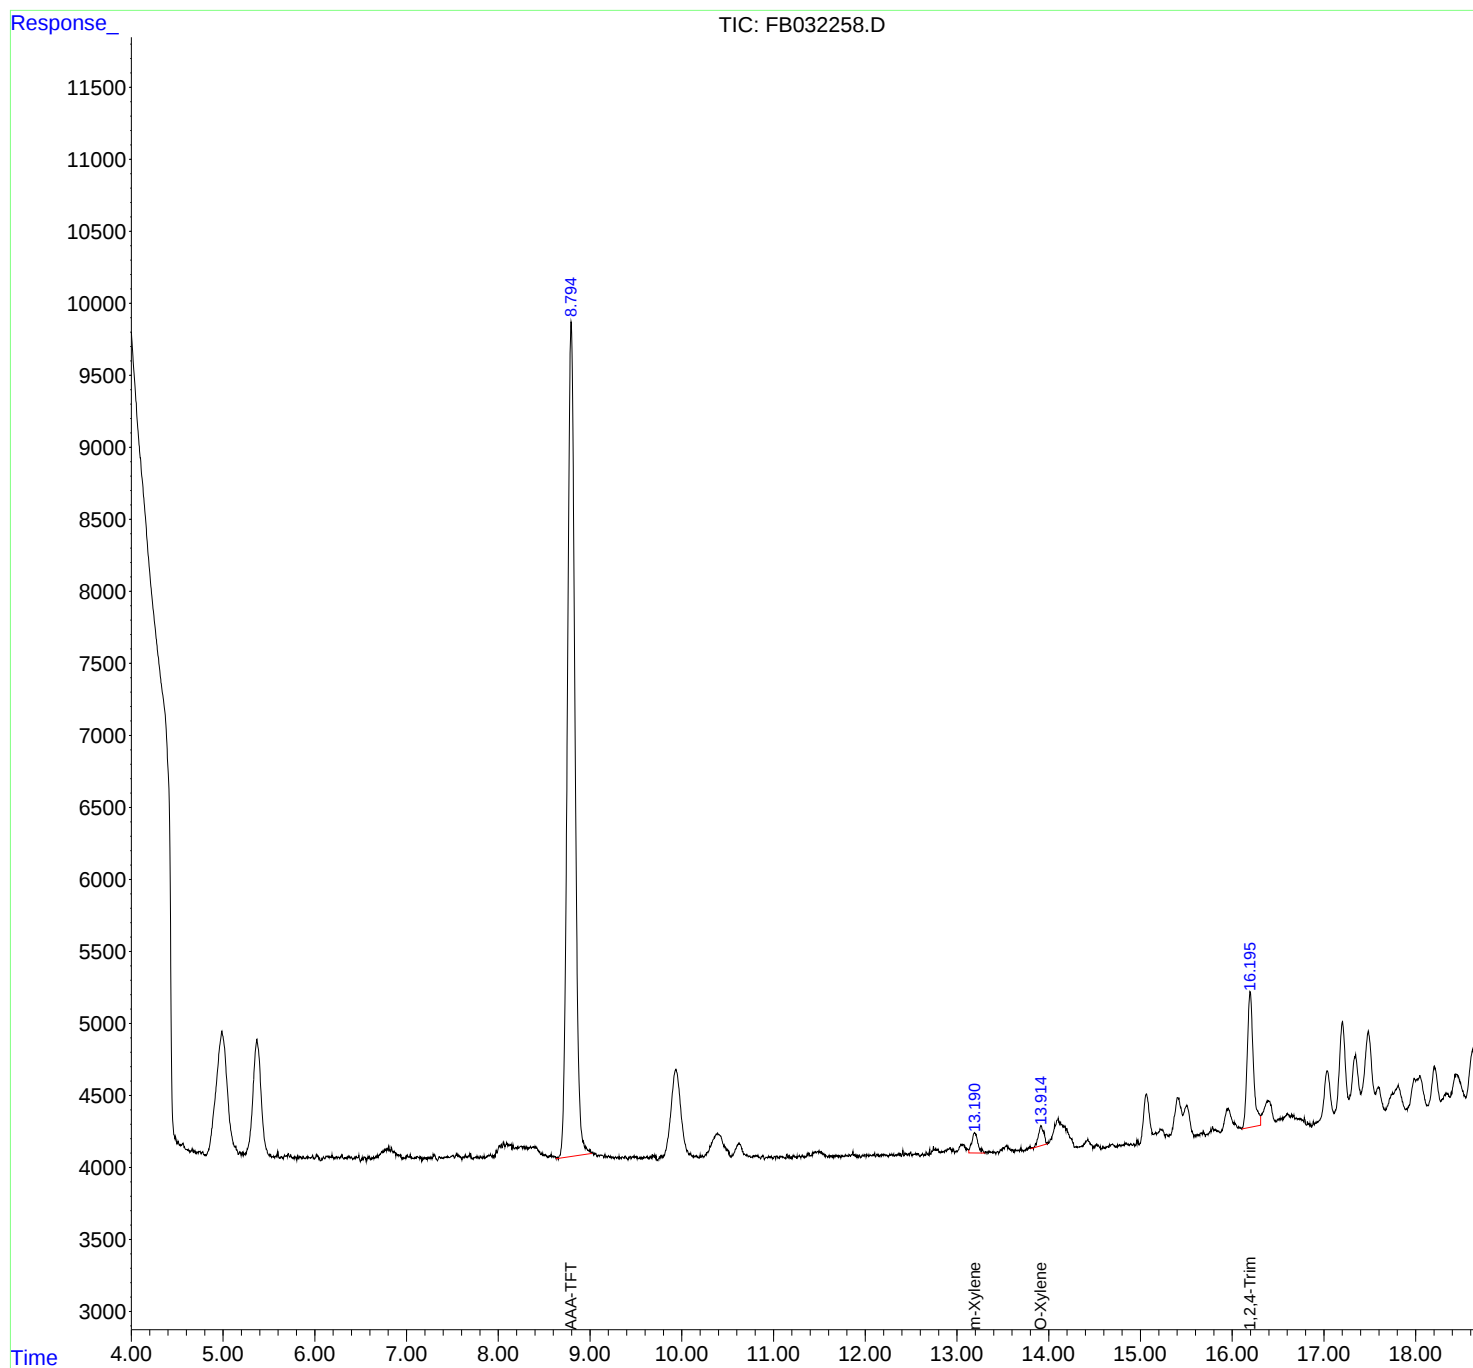


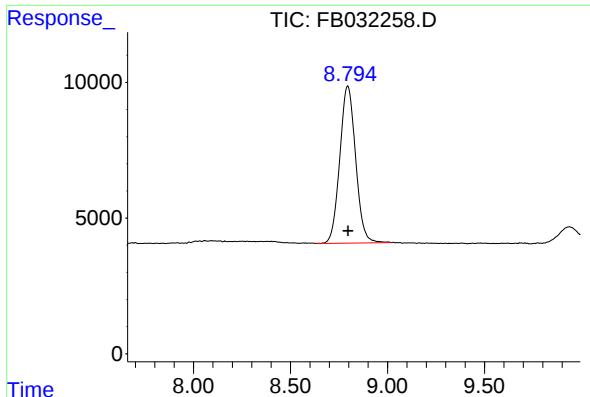

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 328416
Conc: 18.35 ng/ml

Instrument :
FID_B
ClientSampleId :

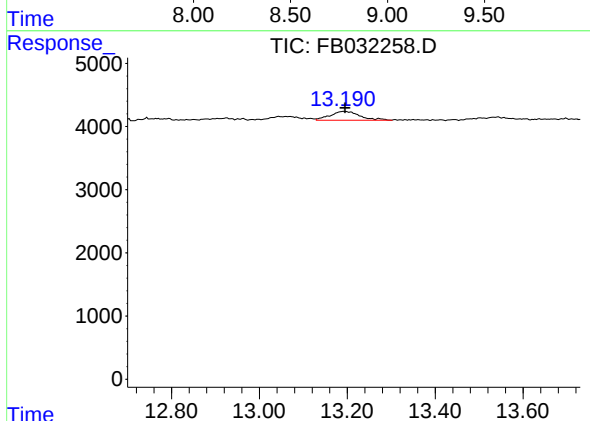


#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: -0.002 min
Response: 6519
Conc: 0.19 ng/ml

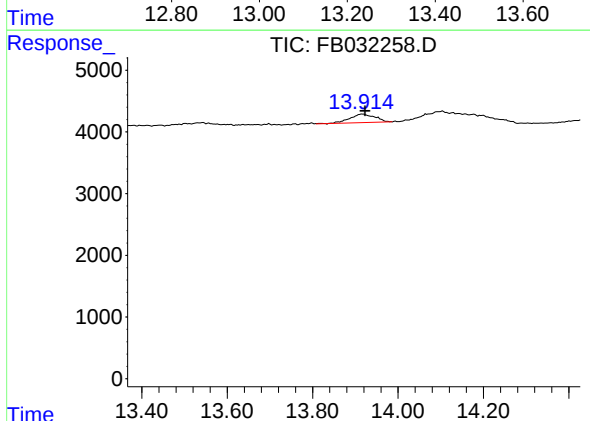

#9 o-Xylene

R.T.: 13.917 min
Delta R.T.: -0.006 min
Response: 5617
Conc: 0.17 ng/ml

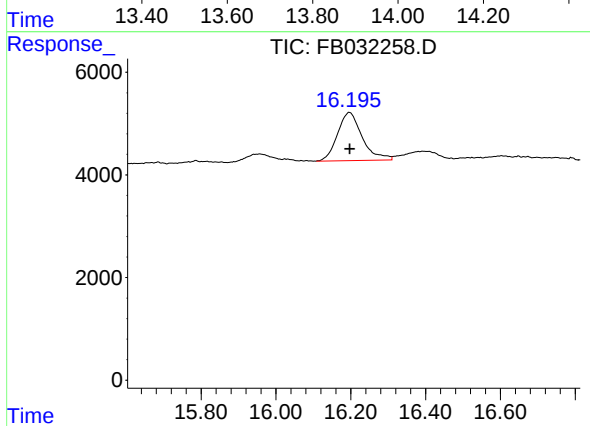

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.000 min
Response: 43015
Conc: 1.54 ng/ml