

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101725\
 Data File : FB032256.D
 Signal(s) : FID2B.CH
 Acq On : 17 Oct 2025 11:01
 Operator : YP/AJ
 Sample : BSF1017S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1017S1

Integration File: Calibrat.e
 Quant Time: Oct 17 23:03:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
 Quant Title :
 QLast Update : Mon Sep 22 12:16:10 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	366673	20.485 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	624841	23.137 ng/mlm
2) t 2,2,4-Trimethylpentane	7.419	760238	26.912 ng/ml
3) t n-Heptane	7.753	227518	8.327 ng/ml
4) t Benzene	7.893	294523	8.150 ng/ml
6) t Toluene	10.622	894713	24.022 ng/ml
7) t Ethylbenzene	13.058	262999	8.046 ng/ml
8) t m-Xylene	13.191	554065	16.256 ng/ml
9) t O-Xylene	13.919	553323	16.945 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	463934	16.586 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101725\
Data File : FB032256.D
Signal(s) : FID2B.CH
Acq On : 17 Oct 2025 11:01
Operator : YP/AJ
Sample : BSF1017S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1017S1

Integration File: Calibrat.e
Quant Time: Oct 17 23:03:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

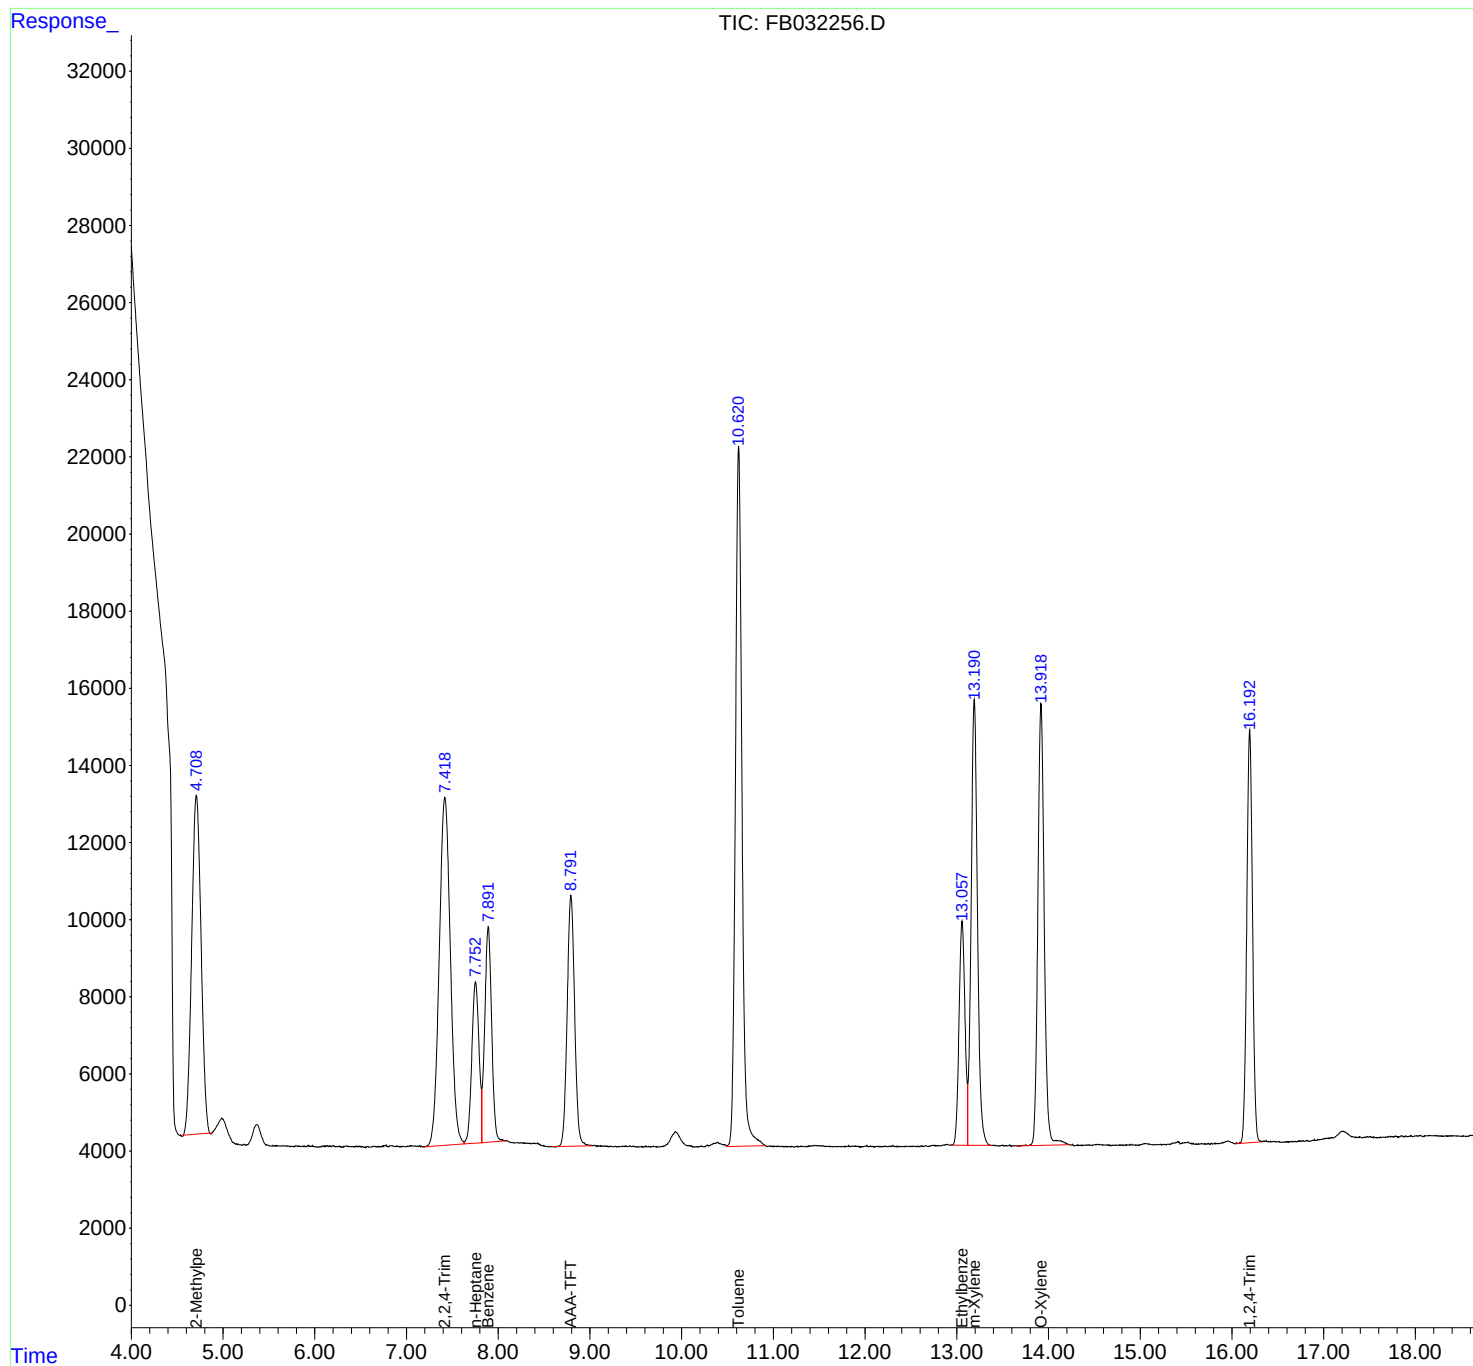


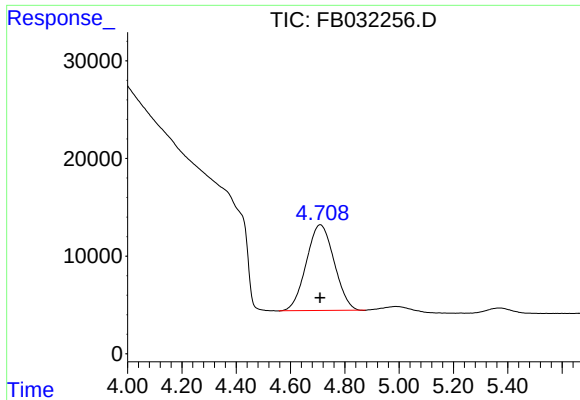

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.001 min
Response: 624841
Conc: 23.14 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1017S1

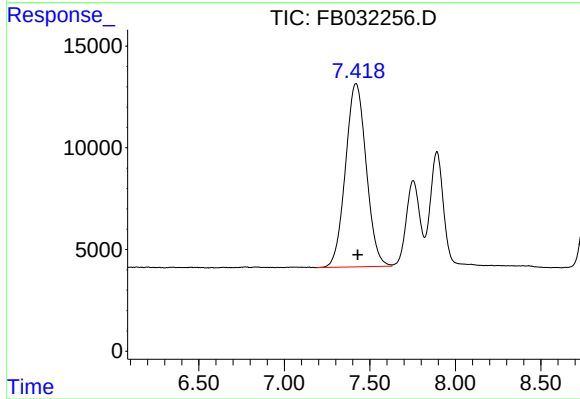


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: -0.011 min
Response: 760238
Conc: 26.91 ng/ml

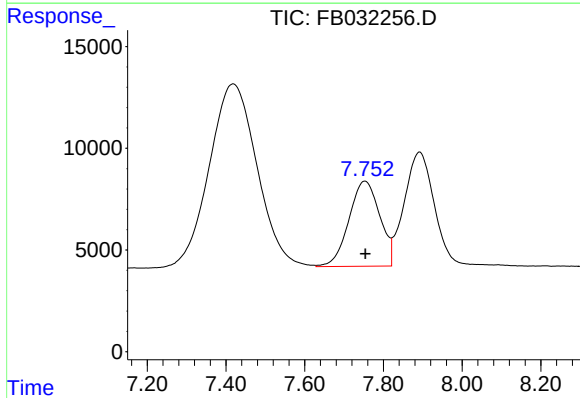


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.001 min
Response: 227518
Conc: 8.33 ng/ml

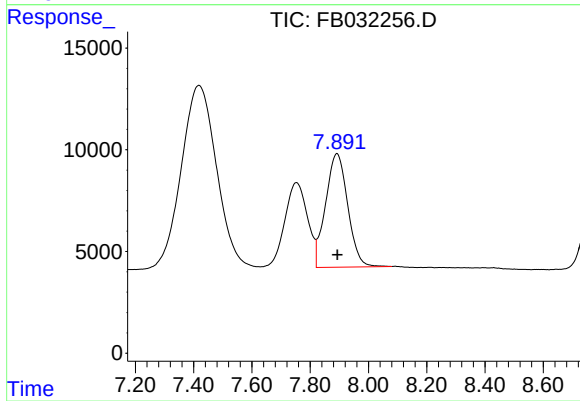

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 294523
Conc: 8.15 ng/ml

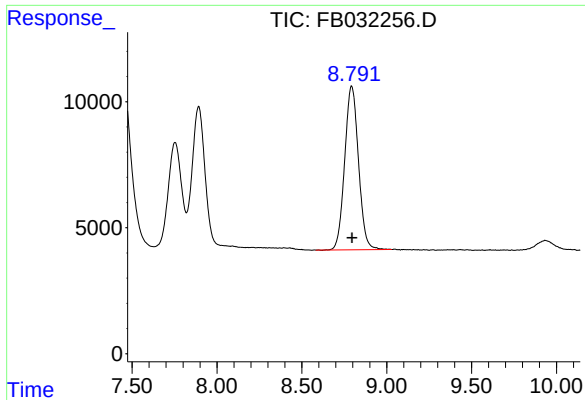

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.003 min
Response: 366673
Conc: 20.49 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1017S1

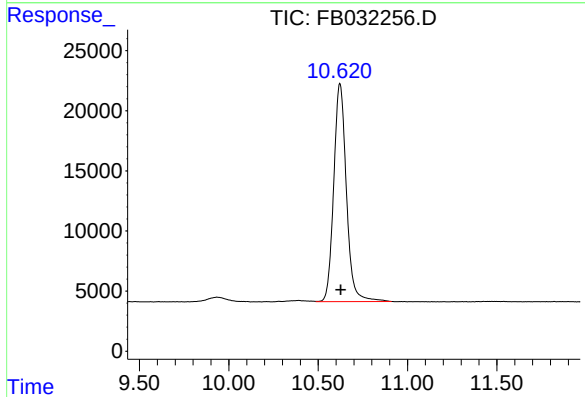


#6 Toluene

R.T.: 10.622 min
Delta R.T.: -0.004 min
Response: 894713
Conc: 24.02 ng/ml

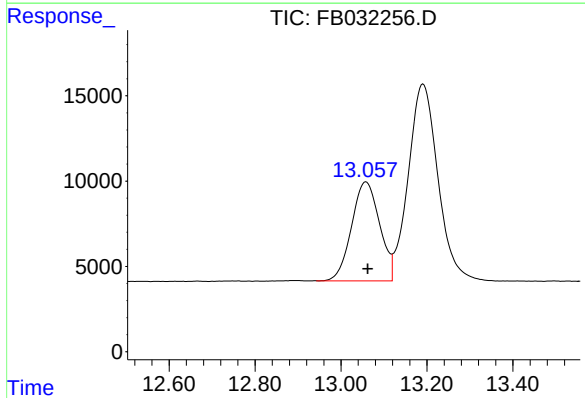


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: -0.004 min
Response: 262999
Conc: 8.05 ng/ml

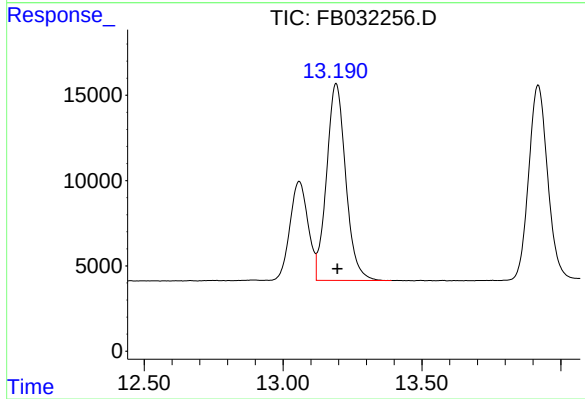

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: -0.004 min
Response: 554065
Conc: 16.26 ng/ml

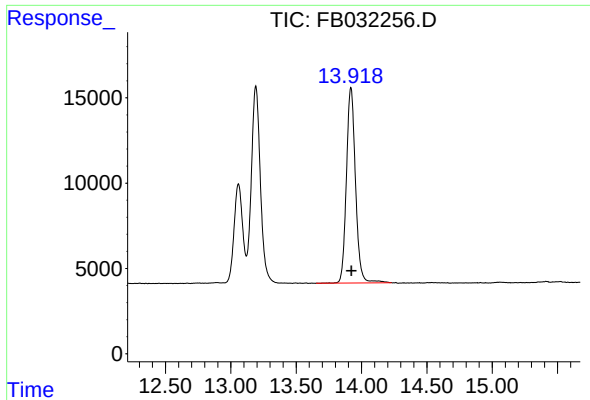

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.004 min
Response: 553323
Conc: 16.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1017S1

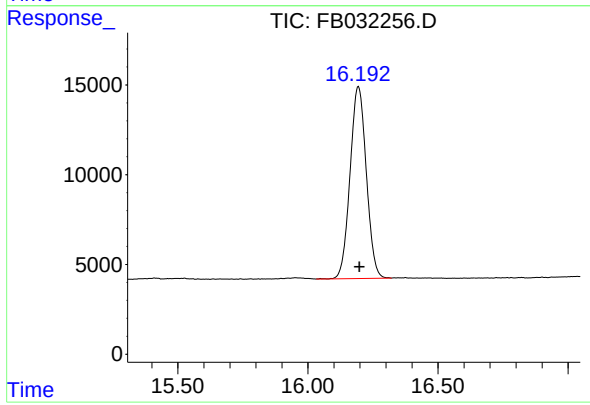

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: -0.003 min
Response: 463934
Conc: 16.59 ng/ml