

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101725\
 Data File : FB032257.D
 Signal(s) : FID2B.CH
 Acq On : 17 Oct 2025 11:28
 Operator : YP/AJ
 Sample : BSF1017S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1017S2

Integration File: Calibrat.e
 Quant Time: Oct 17 23:03:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
 Quant Title :
 QLast Update : Mon Sep 22 12:16:10 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	388290	21.693 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	811112	30.034 ng/mlm
2) t 2,2,4-Trimethylpentane	7.421	943456	33.398 ng/ml
3) t n-Heptane	7.754	296739	10.860 ng/ml
4) t Benzene	7.893	359111	9.937 ng/ml
6) t Toluene	10.623	1038066	27.871 ng/ml
7) t Ethylbenzene	13.059	313923	9.604 ng/ml
8) t m-Xylene	13.192	647040	18.983 ng/ml
9) t O-Xylene	13.919	625682	19.161 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	534513	19.109 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101725\
Data File : FB032257.D
Signal(s) : FID2B.CH
Acq On : 17 Oct 2025 11:28
Operator : YP/AJ
Sample : BSF1017S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1017S2

Integration File: Calibrat.e
Quant Time: Oct 17 23:03:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

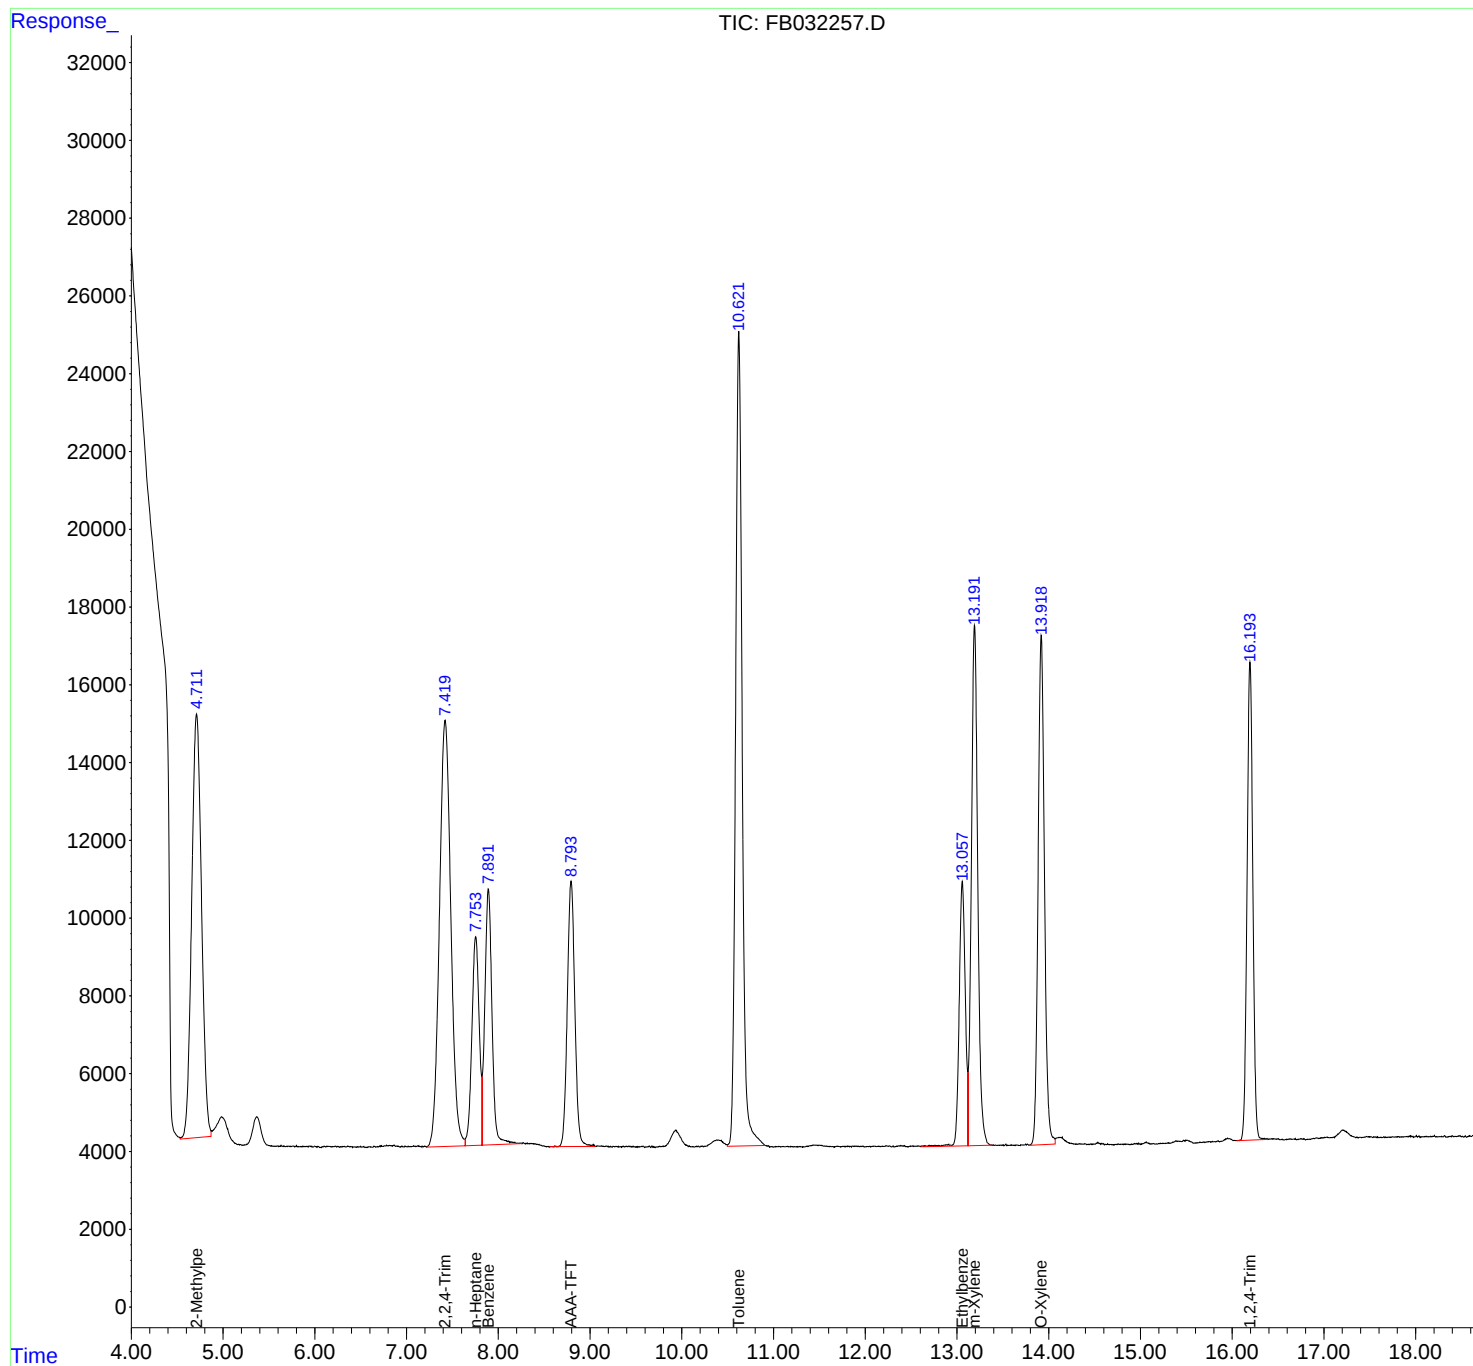


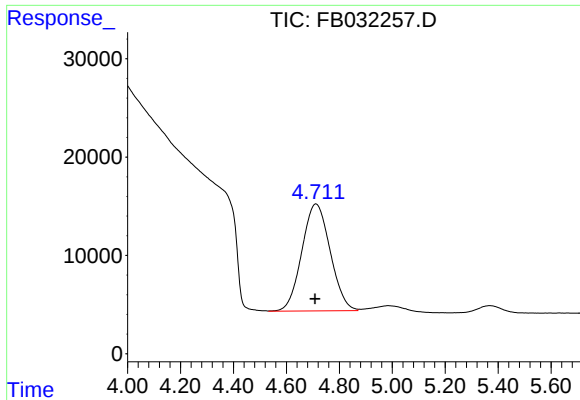

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.002 min
Response: 811112
Conc: 30.03 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1017S2

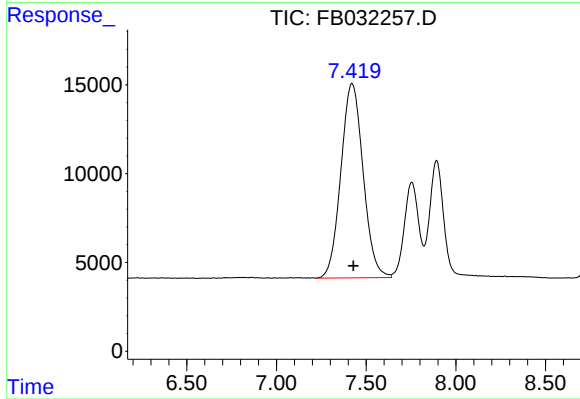


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: -0.010 min
Response: 943456
Conc: 33.40 ng/ml

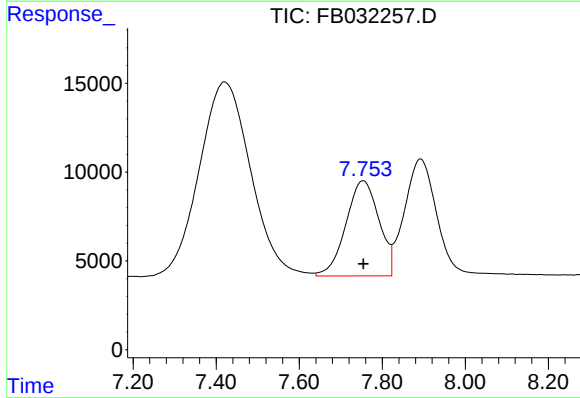


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.000 min
Response: 296739
Conc: 10.86 ng/ml

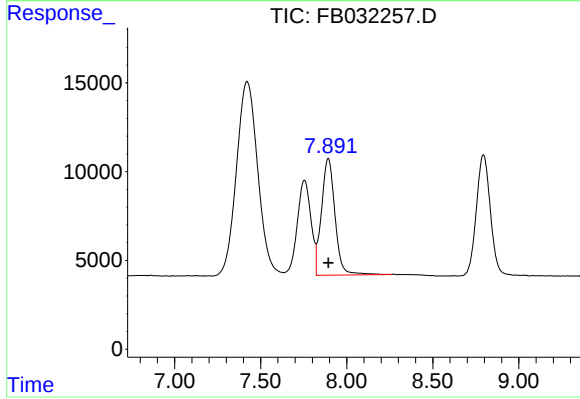

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 359111
Conc: 9.94 ng/ml

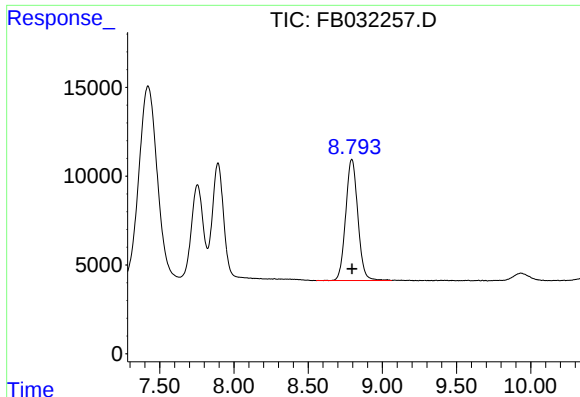

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.002 min
Response: 388290
Conc: 21.69 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1017S2

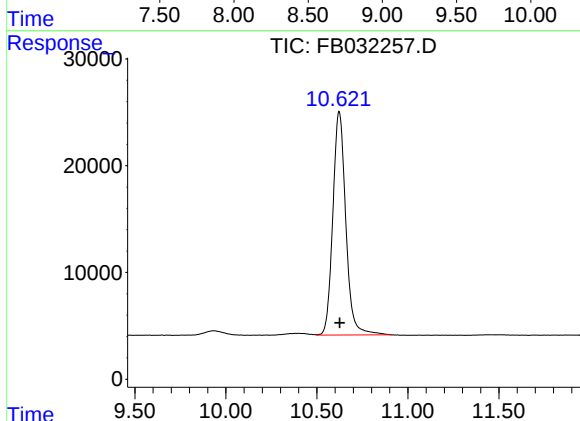


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.003 min
Response: 1038066
Conc: 27.87 ng/ml

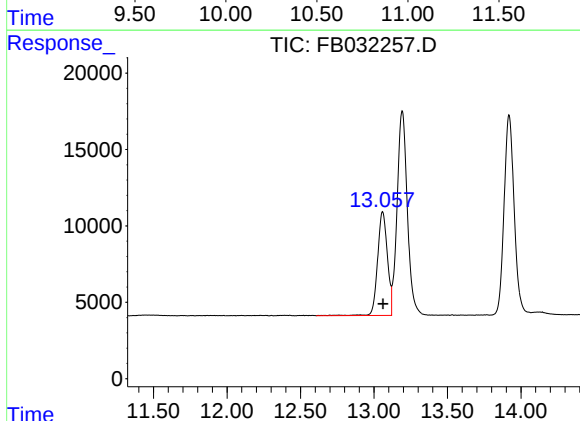


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: -0.003 min
Response: 313923
Conc: 9.60 ng/ml

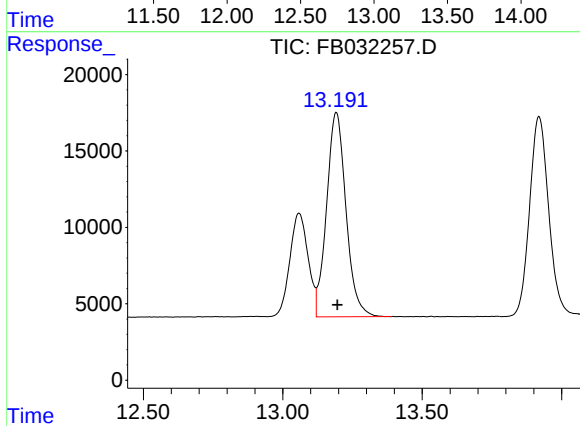

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: -0.003 min
Response: 647040
Conc: 18.98 ng/ml

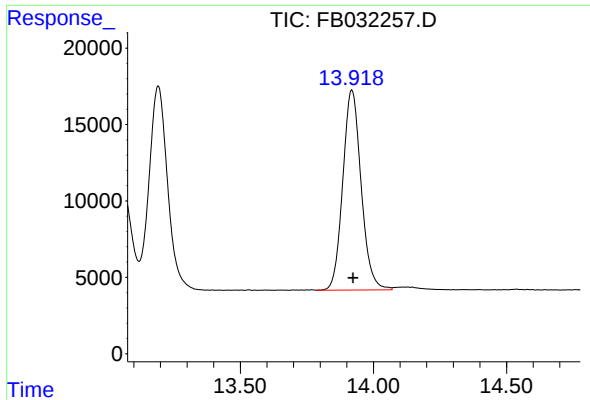

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.004 min
Response: 625682
Conc: 19.16 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1017S2

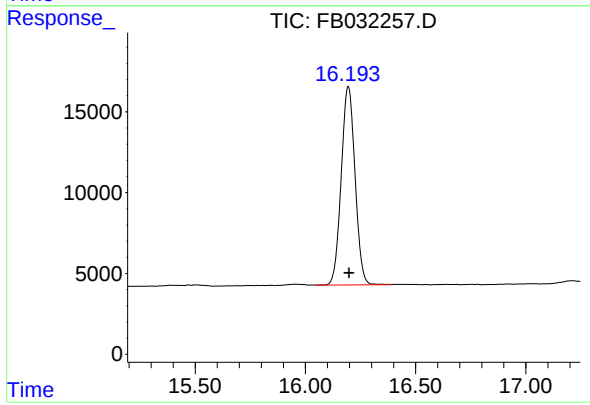

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.003 min
Response: 534513
Conc: 19.11 ng/ml