

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110425\
 Data File : FB032286.D
 Signal(s) : FID2B.CH
 Acq On : 4 Nov 2025 9:14
 Operator : YP/AJ
 Sample : VBF1104S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 04 22:35:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
 Quant Title :
 QLast Update : Tue Oct 28 04:57:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	448499	22.112 ng/ml
Target Compounds			
6) t Toluene	10.619	23515	0.657 ng/ml
7) t Ethylbenzene	13.062	6617	0.208 ng/ml
8) t m-Xylene	13.189	28094	0.844 ng/ml
9) t O-Xylene	13.920	14264	0.444 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	27441	0.992 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110425\
Data File : FB032286.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2025 9:14
Operator : YP/AJ
Sample : VBF1104S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 04 22:35:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

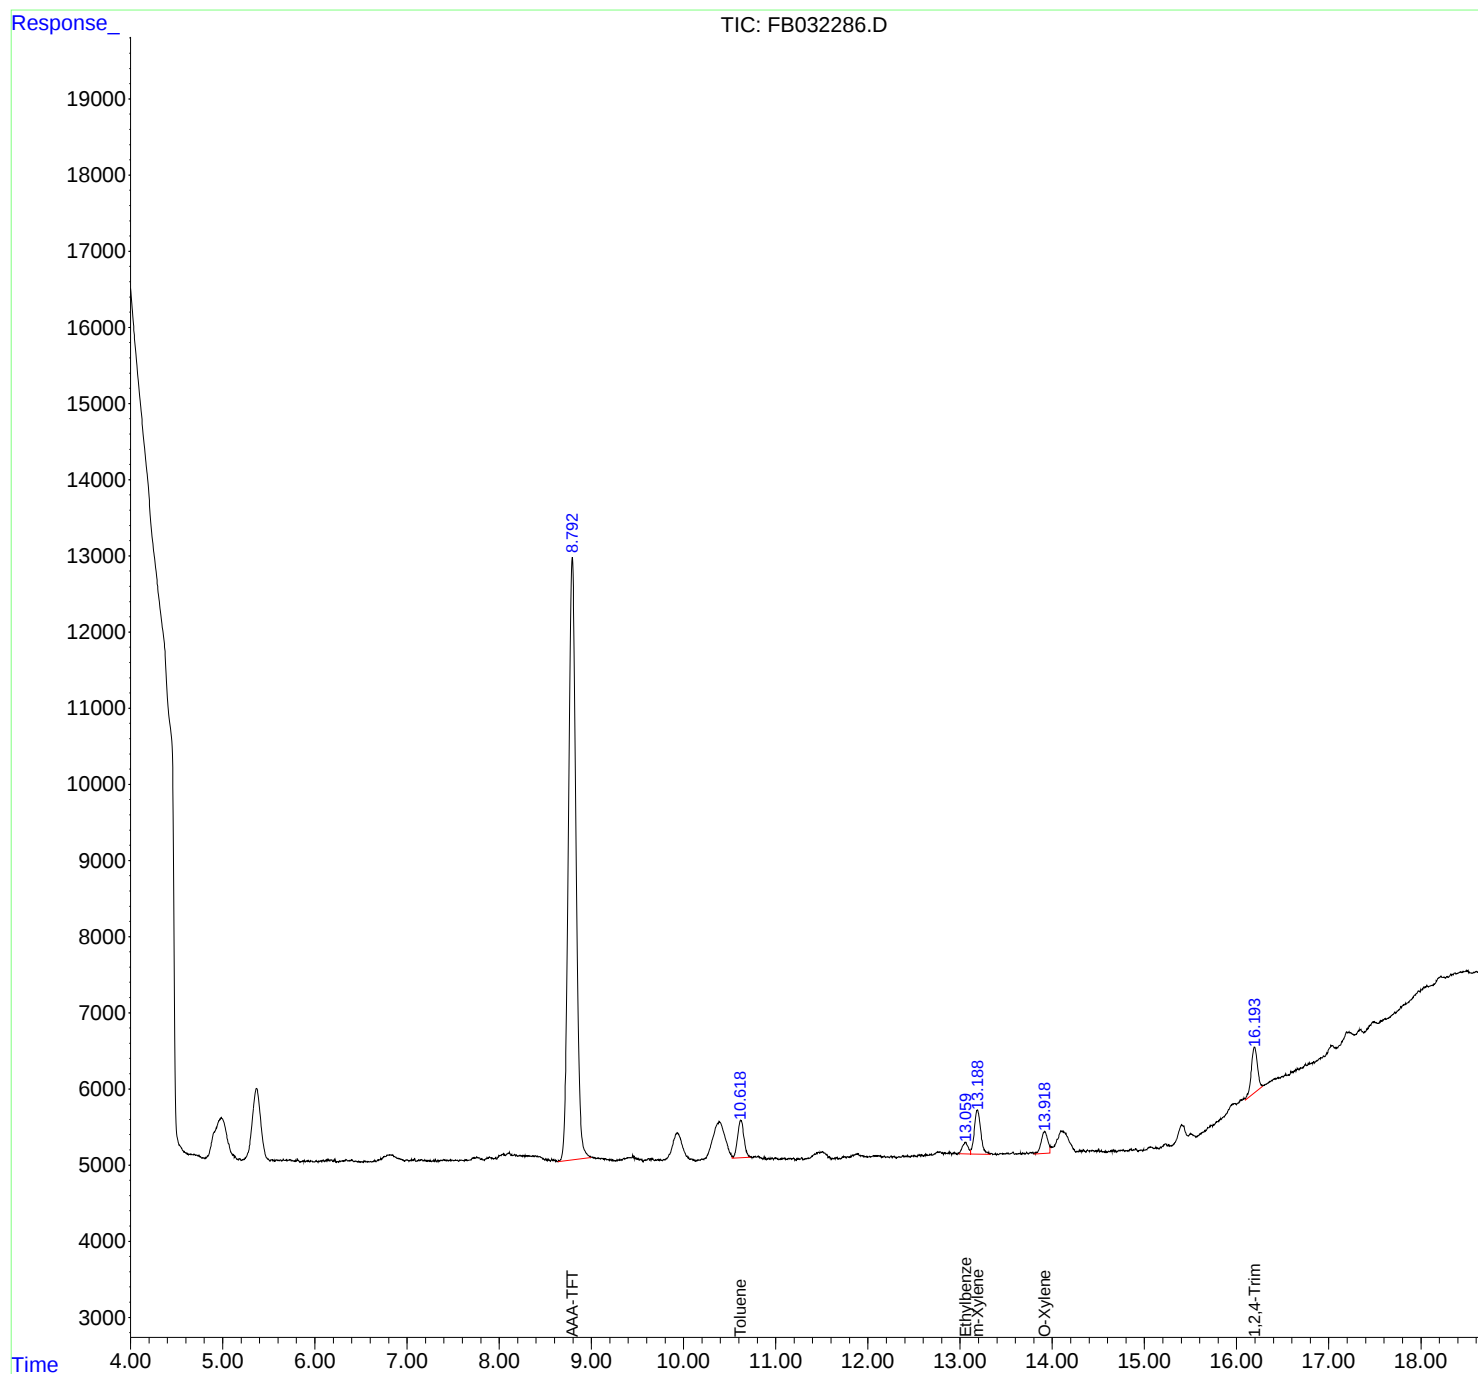


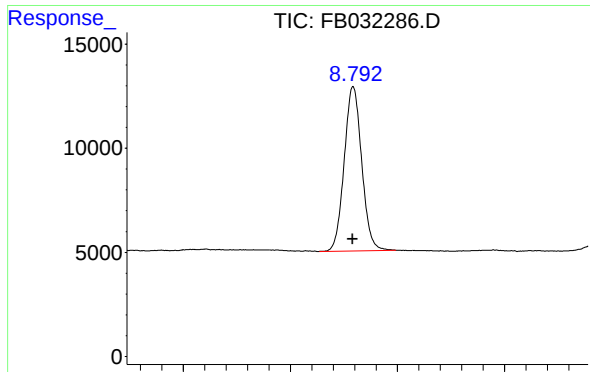

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 448499
Conc: 22.11 ng/ml

Instrument :
FID_B
ClientSampleId :

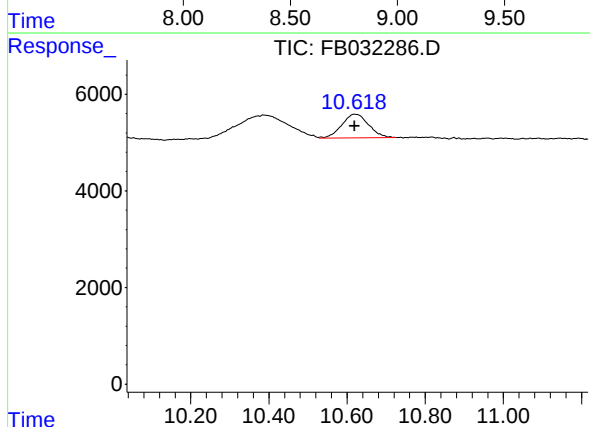


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 23515
Conc: 0.66 ng/ml

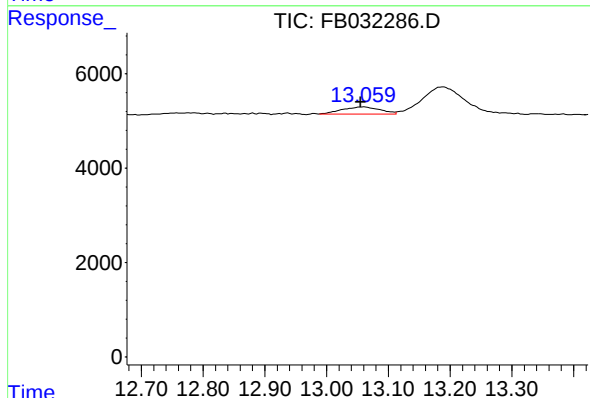


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: 0.007 min
Response: 6617
Conc: 0.21 ng/ml

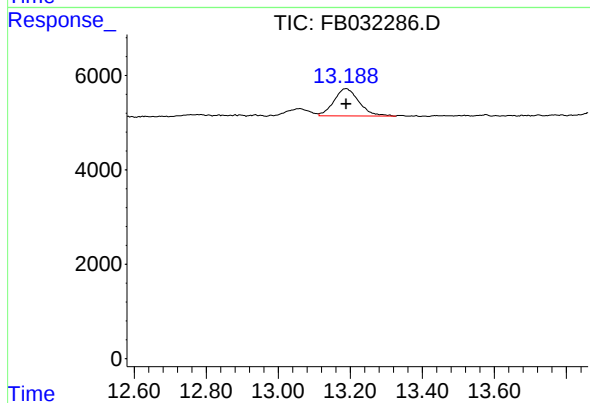

#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 28094
Conc: 0.84 ng/ml

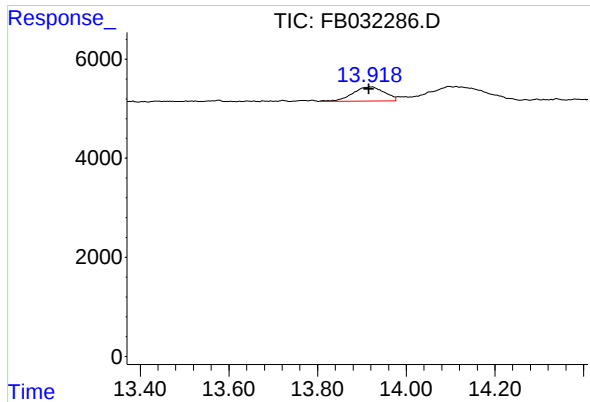


#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.004 min
Response: 14264
Conc: 0.44 ng/ml

Instrument :

FID_B

ClientSampleId :

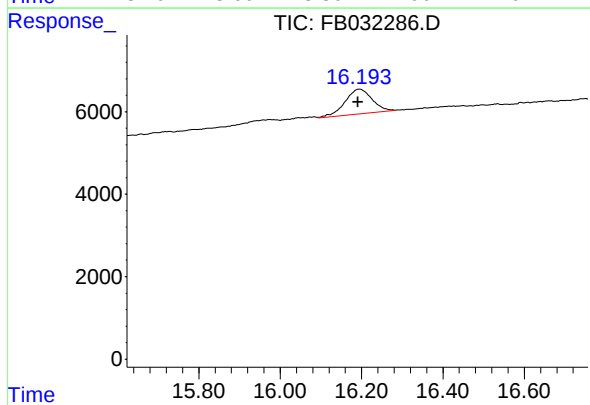

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.004 min
Response: 27441
Conc: 0.99 ng/ml