

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110525\
 Data File : FB032304.D
 Signal(s) : FID2B.CH
 Acq On : 5 Nov 2025 10:16
 Operator : YP/AJ
 Sample : BSF1105S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1105S1

Integration File: Calibration.e
 Quant Time: Nov 06 01:05:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
 Quant Title :
 QLast Update : Tue Oct 28 04:57:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	402666	19.853 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	841112	30.703 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	978209	31.750 ng/ml
3) t n-Heptane	7.753	306855	10.473 ng/ml
4) t Benzene	7.892	369009	10.659 ng/ml
6) t Toluene	10.622	1108350	30.976 ng/ml
7) t Ethylbenzene	13.059	328577	10.331 ng/ml
8) t m-Xylene	13.191	692192	20.785 ng/ml
9) t O-Xylene	13.918	656757	20.452 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	557459	20.147 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110525\
Data File : FB032304.D
Signal(s) : FID2B.CH
Acq On : 5 Nov 2025 10:16
Operator : YP/AJ
Sample : BSF1105S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1105S1

Integration File: Calibration.e
Quant Time: Nov 06 01:05:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

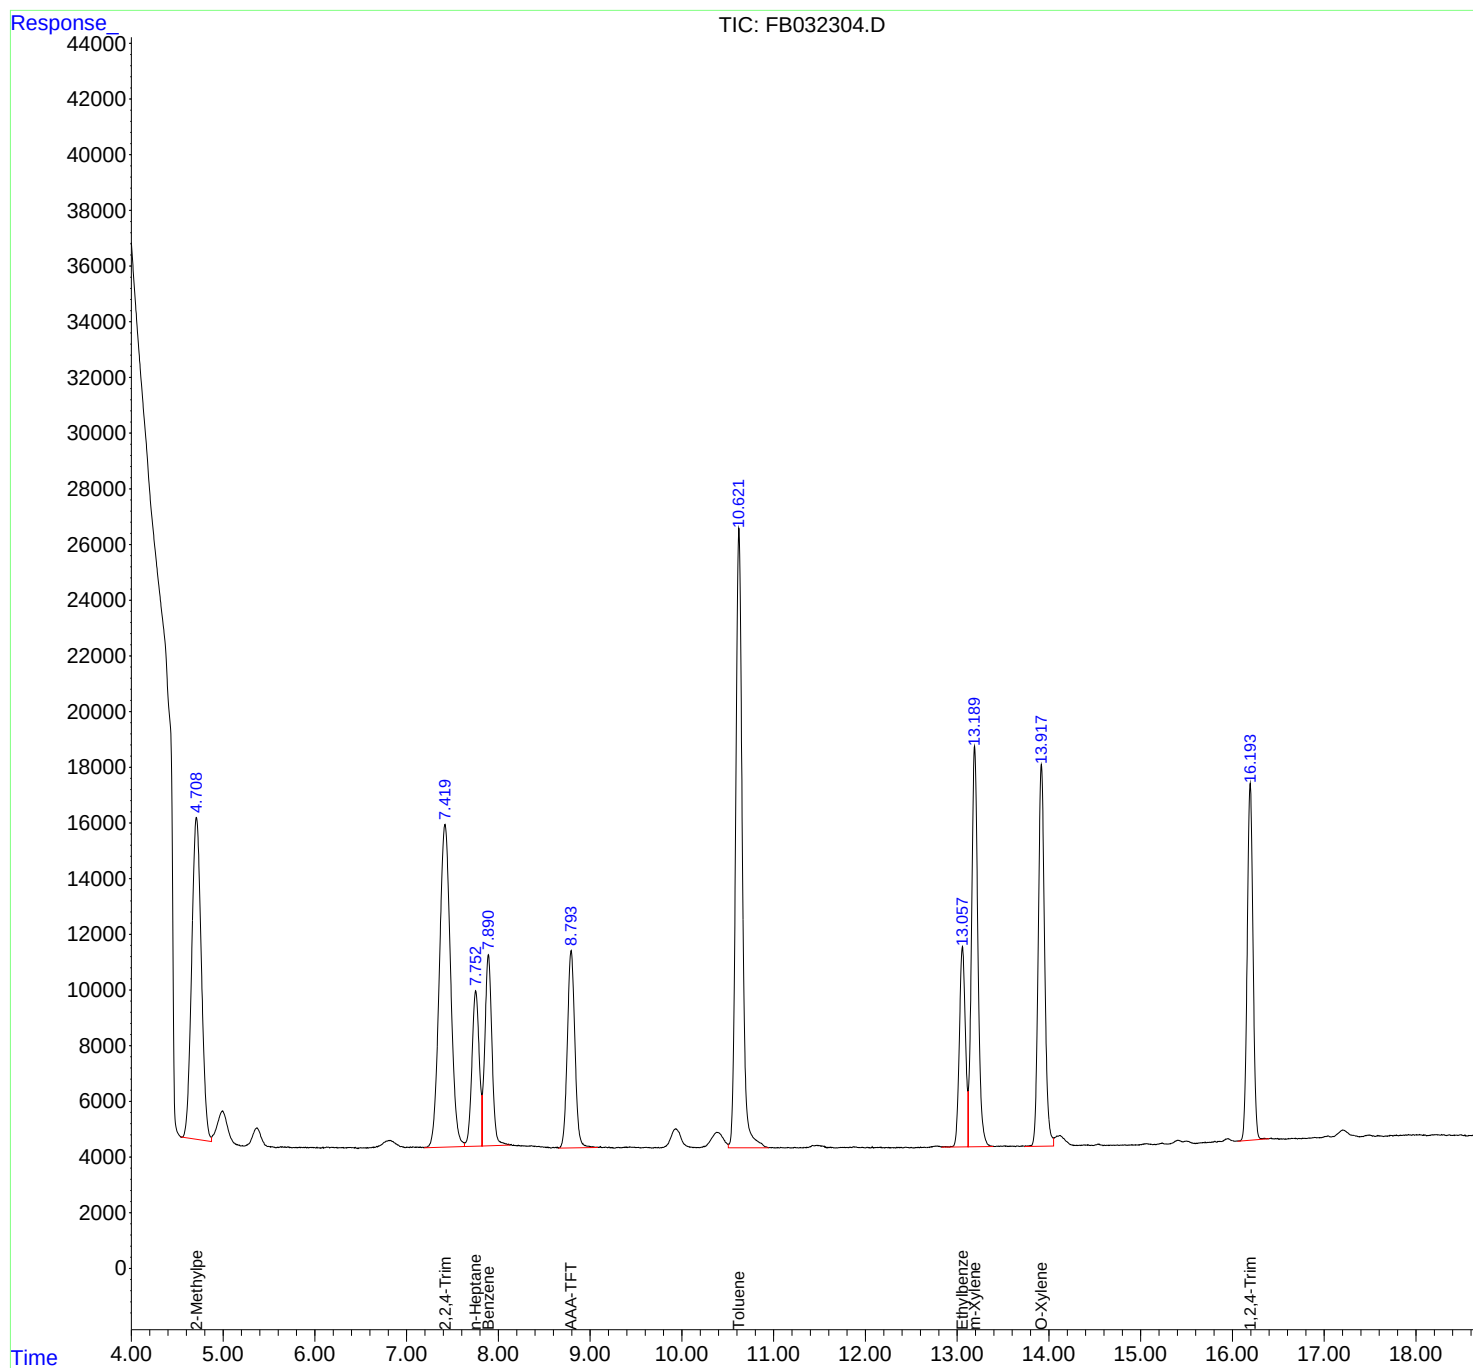


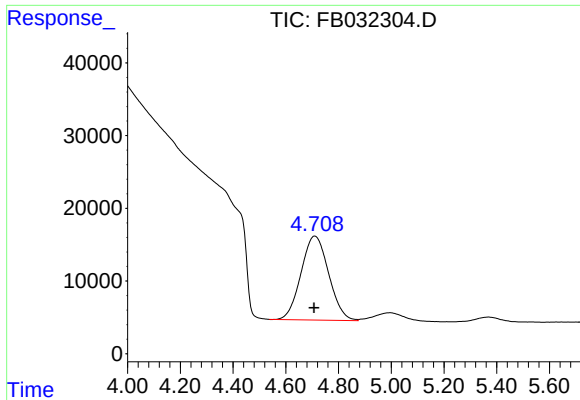

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.003 min
Response: 841112
Conc: 30.70 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1105S1

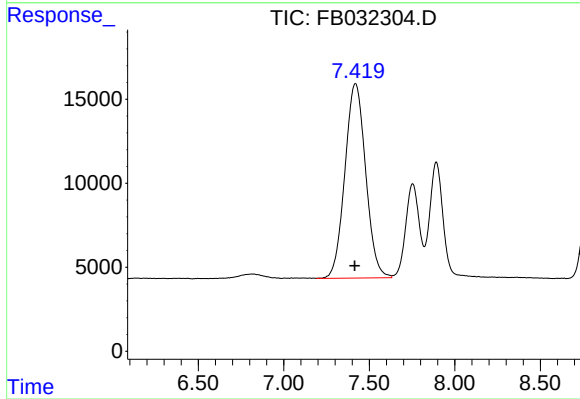


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.004 min
Response: 978209
Conc: 31.75 ng/ml

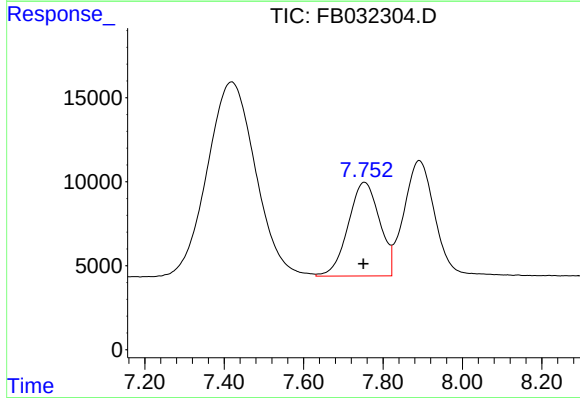


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.003 min
Response: 306855
Conc: 10.47 ng/ml

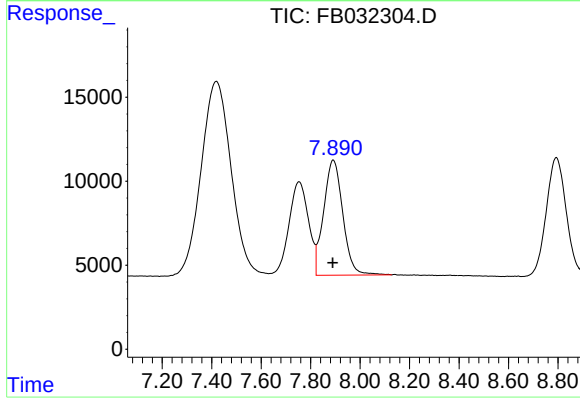

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.003 min
Response: 369009
Conc: 10.66 ng/ml

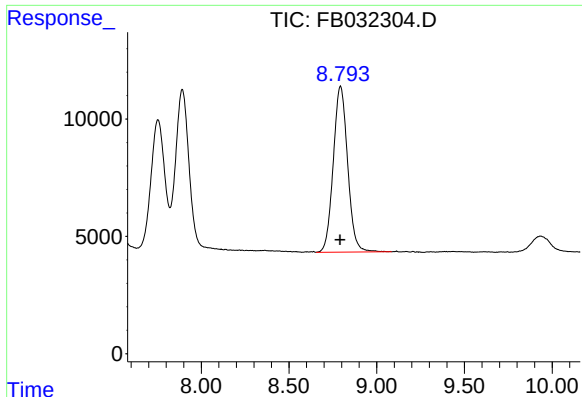

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 402666
Conc: 19.85 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1105S1

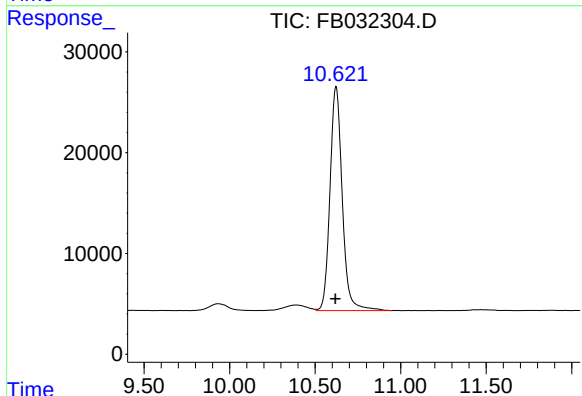


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.003 min
Response: 1108350
Conc: 30.98 ng/ml

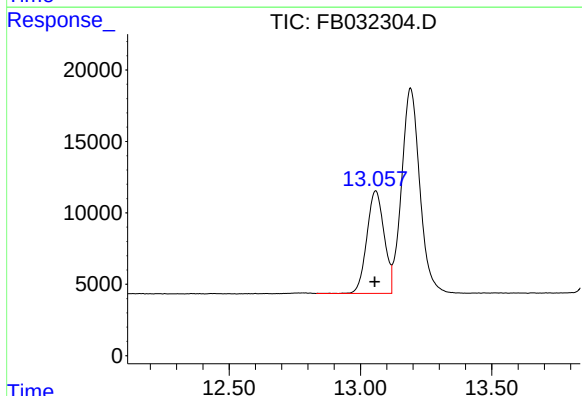


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.004 min
Response: 328577
Conc: 10.33 ng/ml

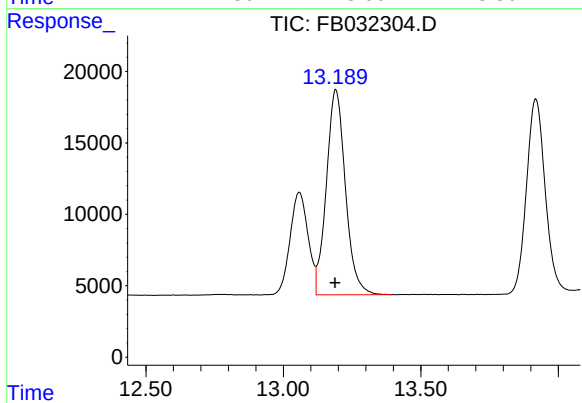

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 692192
Conc: 20.78 ng/ml

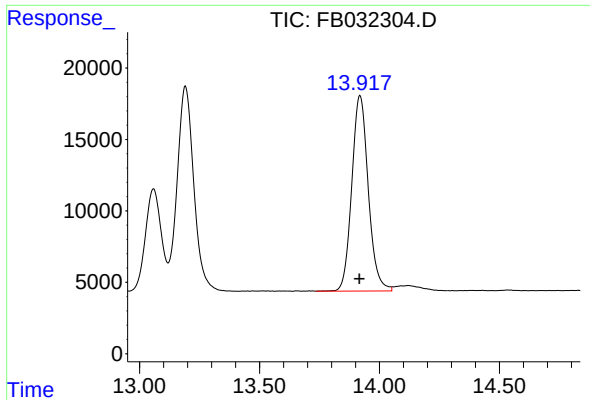

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.003 min
Response: 656757
Conc: 20.45 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1105S1

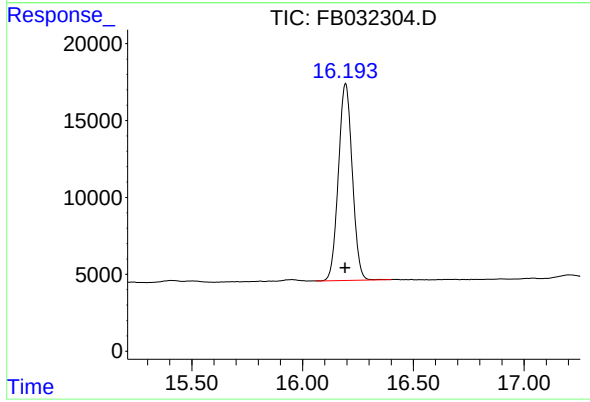

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.003 min
Response: 557459
Conc: 20.15 ng/ml