

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110625\
 Data File : FB032319.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2025 11:12
 Operator : YP/AJ
 Sample : BSF1106S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 VBF1106S2

Integration File: Calibration.e
 Quant Time: Nov 07 00:57:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
 Quant Title :
 QLast Update : Tue Oct 28 04:57:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	427165	21.060 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.714	893315	32.609 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1030436	33.445 ng/ml
3) t n-Heptane	7.755	321595	10.976 ng/ml
4) t Benzene	7.893	386836	11.174 ng/ml
6) t Toluene	10.623	1137971	31.804 ng/ml
7) t Ethylbenzene	13.059	338056	10.629 ng/ml
8) t m-Xylene	13.192	714783	21.463 ng/ml
9) t O-Xylene	13.920	683352	21.280 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	579760	20.953 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110625\
Data File : FB032319.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2025 11:12
Operator : YP/AJ
Sample : BSF1106S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF1106S2

Integration File: Calibration.e
Quant Time: Nov 07 00:57:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

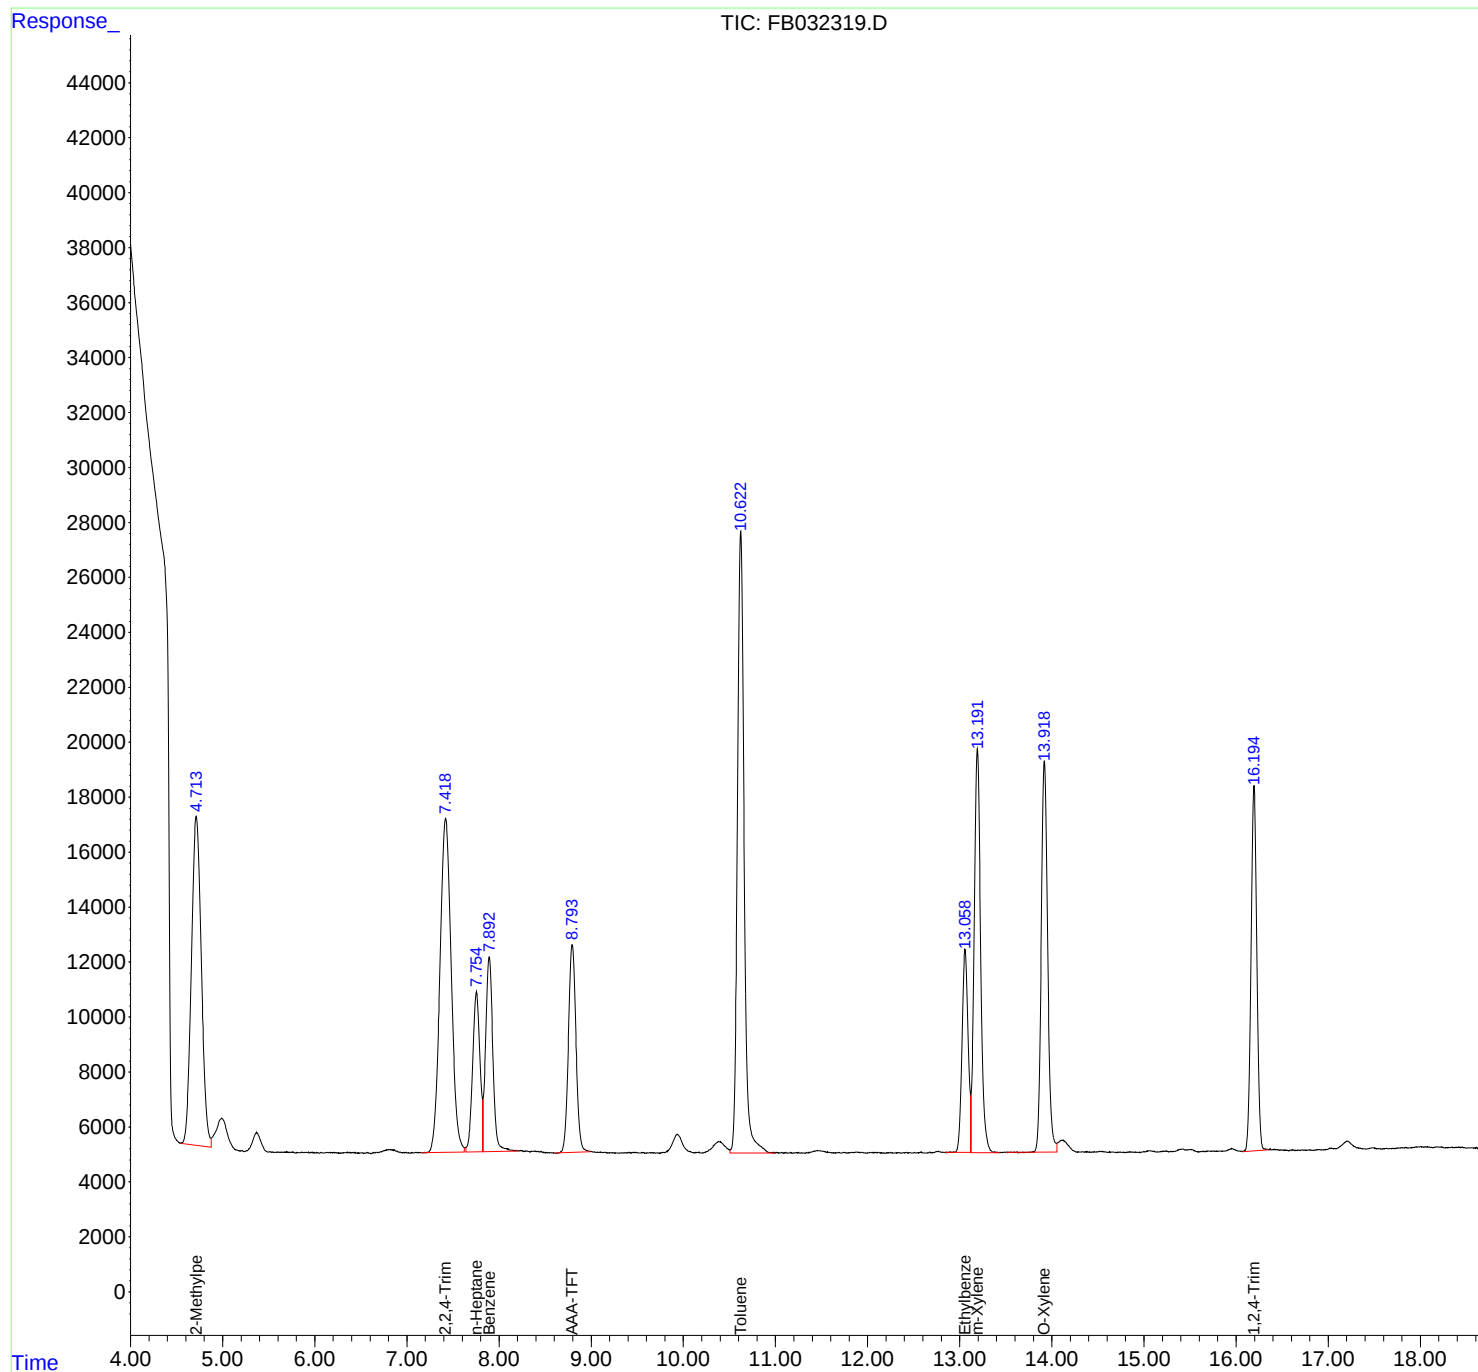


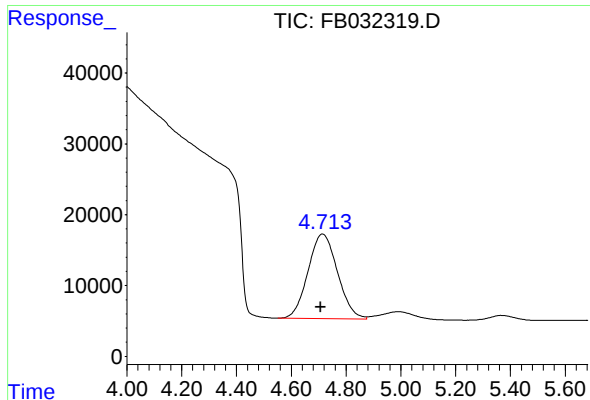

#1 2-Methylpentane


R.T.: 4.714 min
Delta R.T.: 0.007 min
Response: 893315
Conc: 32.61 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1106S2

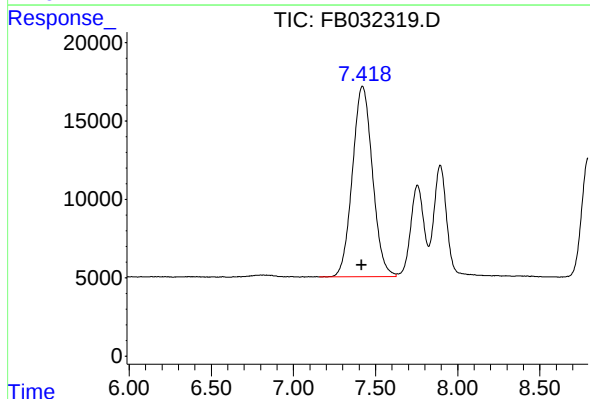


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.003 min
Response: 1030436
Conc: 33.45 ng/ml

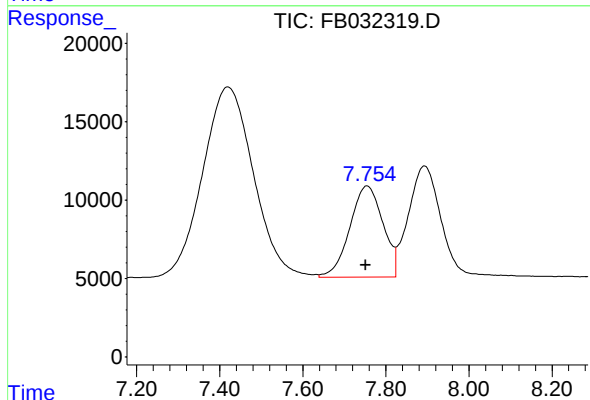


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.005 min
Response: 321595
Conc: 10.98 ng/ml

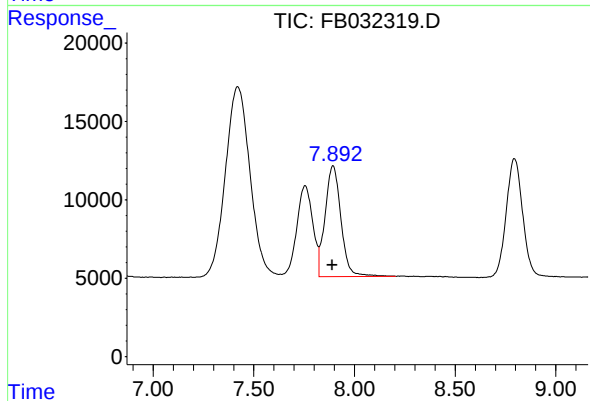

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.005 min
Response: 386836
Conc: 11.17 ng/ml

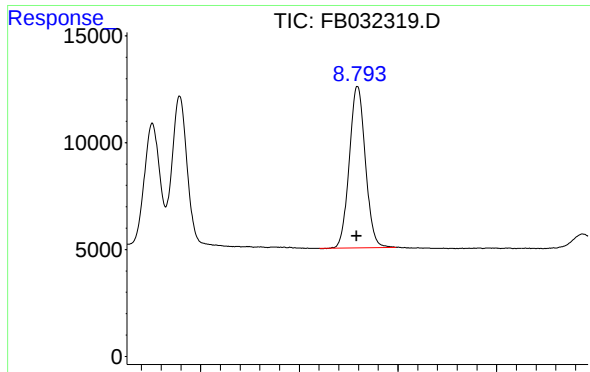

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.004 min
Response: 427165
Conc: 21.06 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1106S2

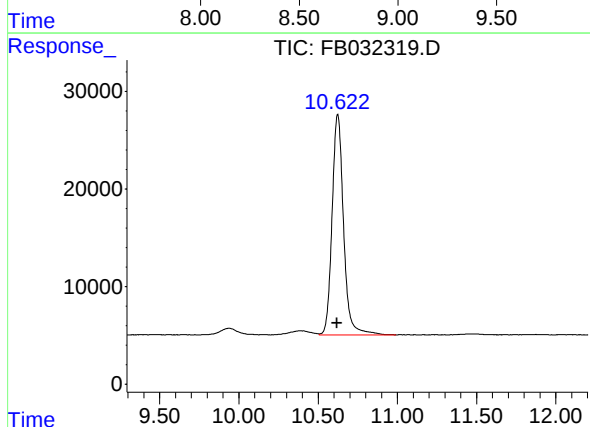


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.004 min
Response: 1137971
Conc: 31.80 ng/ml

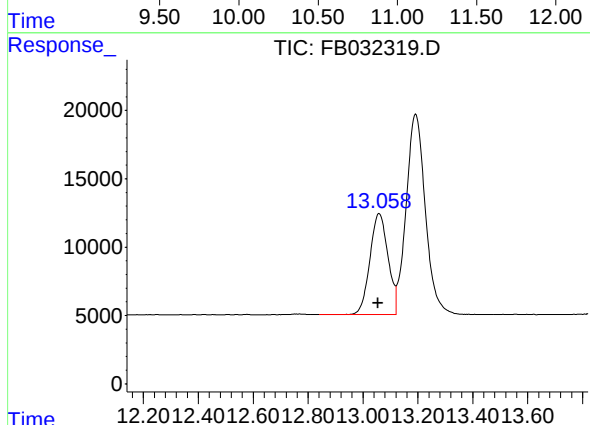


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.004 min
Response: 338056
Conc: 10.63 ng/ml

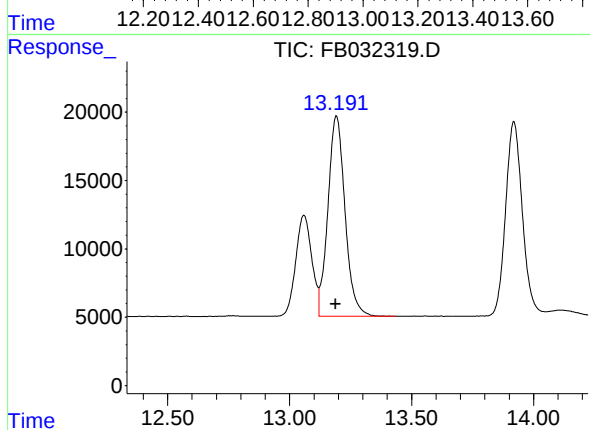

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.003 min
Response: 714783
Conc: 21.46 ng/ml

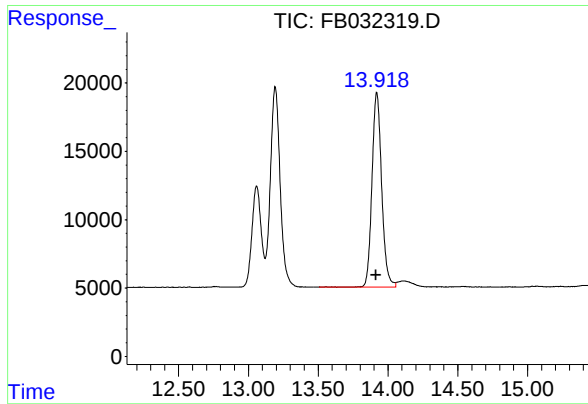

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.004 min
Response: 683352
Conc: 21.28 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1106S2

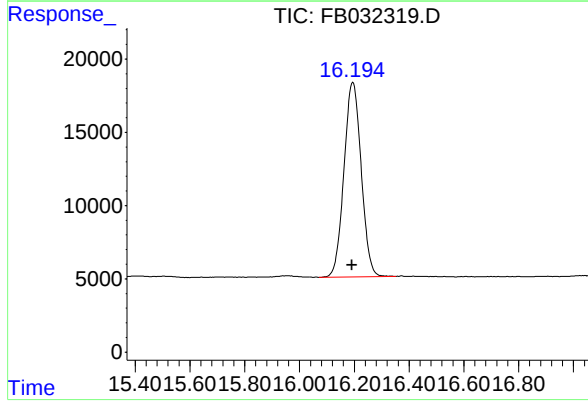

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.003 min
Response: 579760
Conc: 20.95 ng/ml