

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111425\
 Data File : FB032381.D
 Signal(s) : FID2B.CH
 Acq On : 14 Nov 2025 11:07
 Operator : YP/AJ
 Sample : BSF1114S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1114S1

Integration File: Calibrat.e
 Quant Time: Nov 14 14:28:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
 Quant Title :
 QLast Update : Tue Oct 28 04:57:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	368170	18.152 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	670192	24.464 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	871759	28.295 ng/ml
3) t n-Heptane	7.753	257680	8.794 ng/ml
4) t Benzene	7.892	344453	9.950 ng/ml
6) t Toluene	10.622	1020187	28.512 ng/ml
7) t Ethylbenzene	13.058	304354	9.570 ng/ml
8) t m-Xylene	13.191	632793	19.001 ng/ml
9) t O-Xylene	13.919	606812	18.897 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	523032	18.902 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111425\
Data File : FB032381.D
Signal(s) : FID2B.CH
Acq On : 14 Nov 2025 11:07
Operator : YP/AJ
Sample : BSF1114S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1114S1

Integration File: Calibrat.e
Quant Time: Nov 14 14:28:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

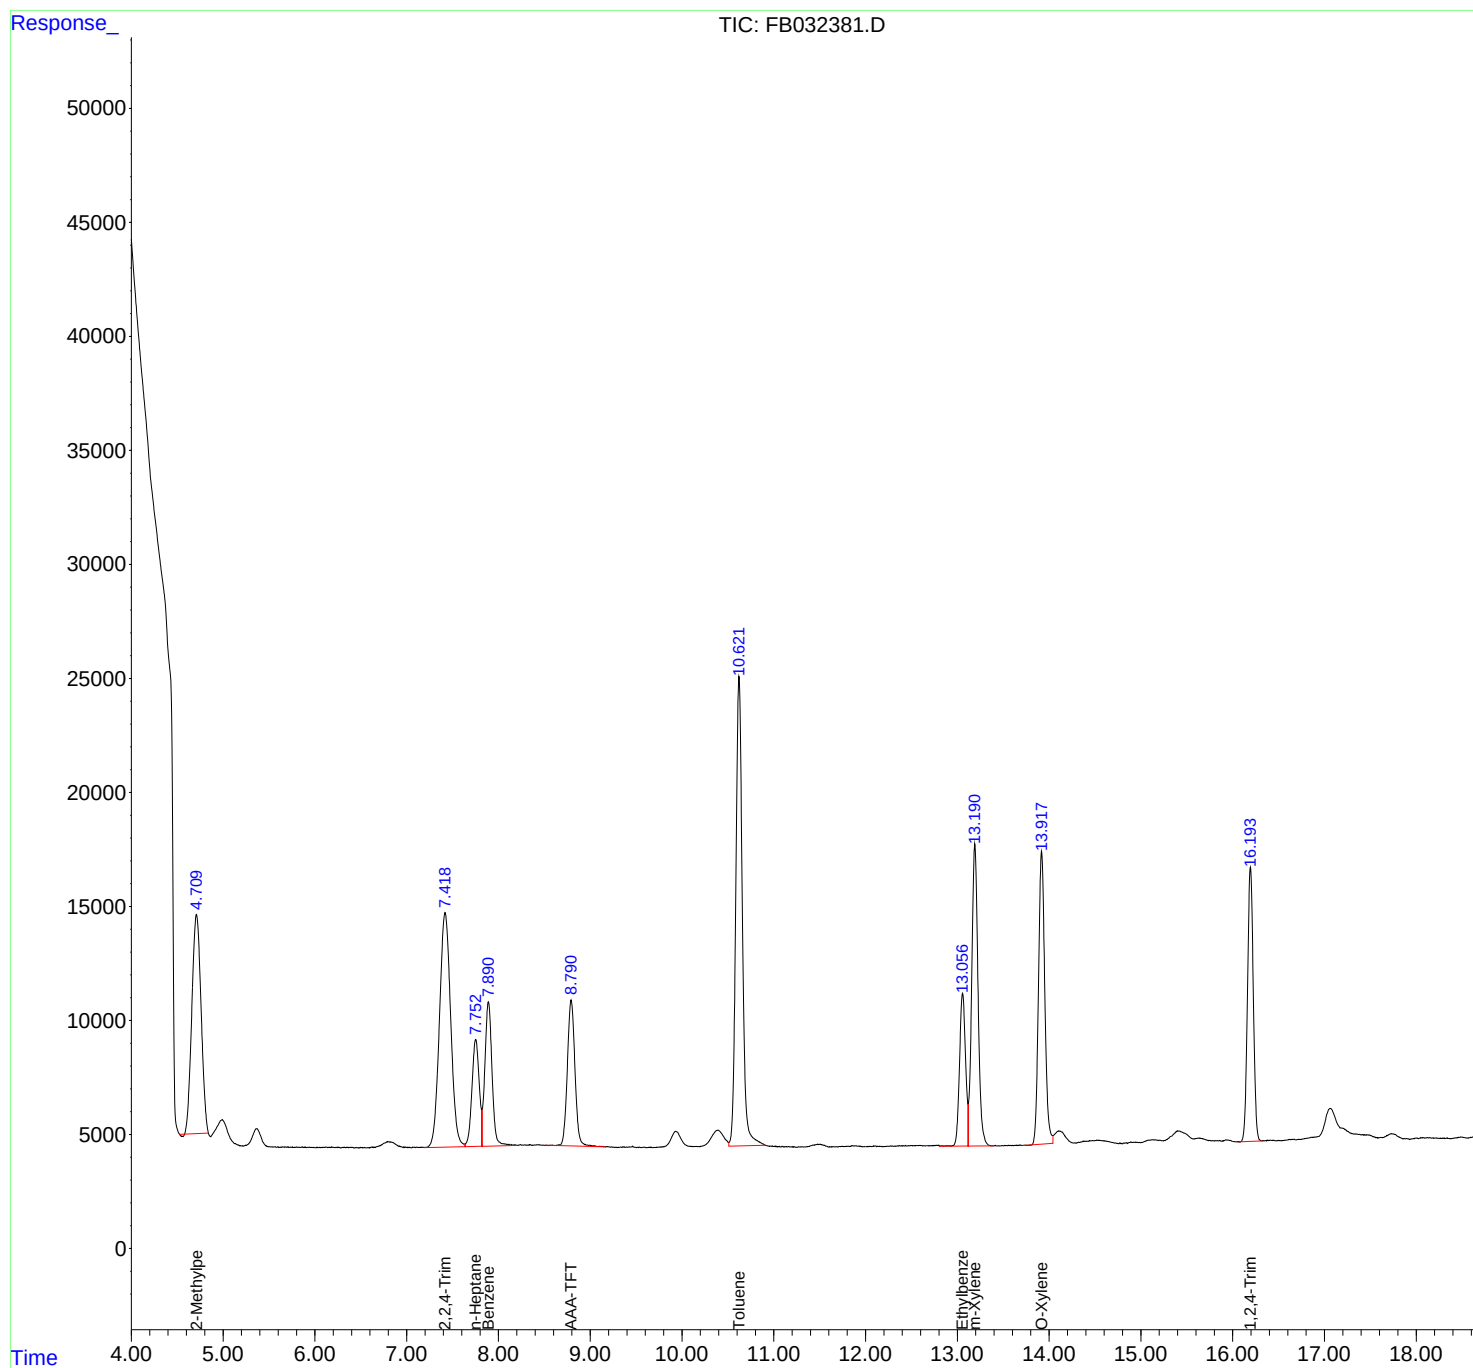


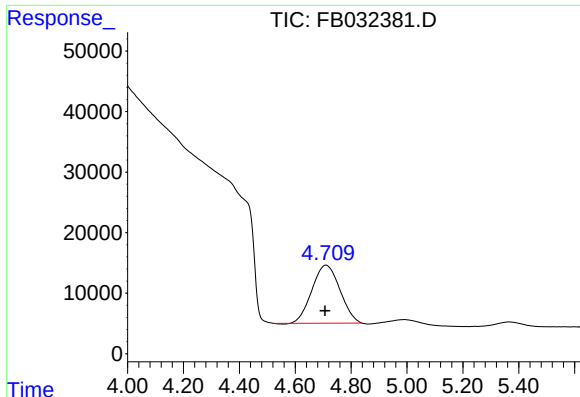

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.003 min
Response: 670192
Conc: 24.46 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S1

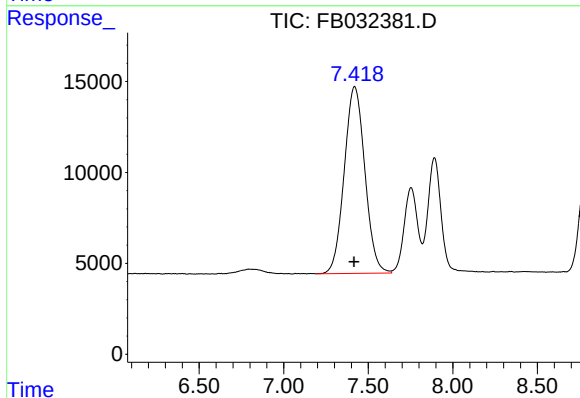


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.003 min
Response: 871759
Conc: 28.30 ng/ml

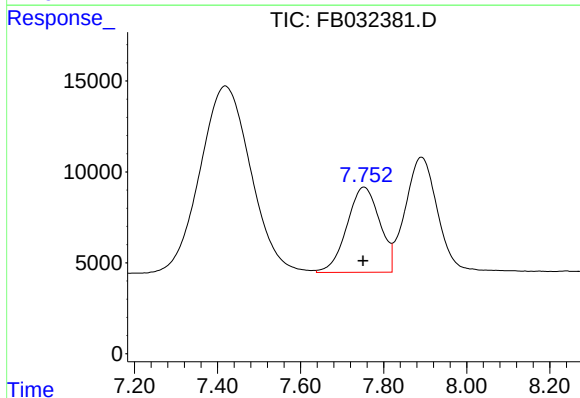


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.002 min
Response: 257680
Conc: 8.79 ng/ml

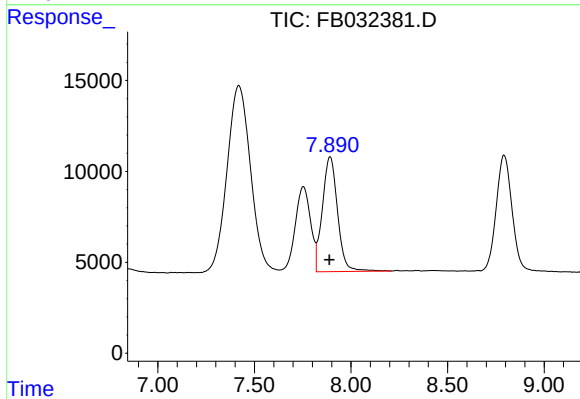

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.003 min
Response: 344453
Conc: 9.95 ng/ml

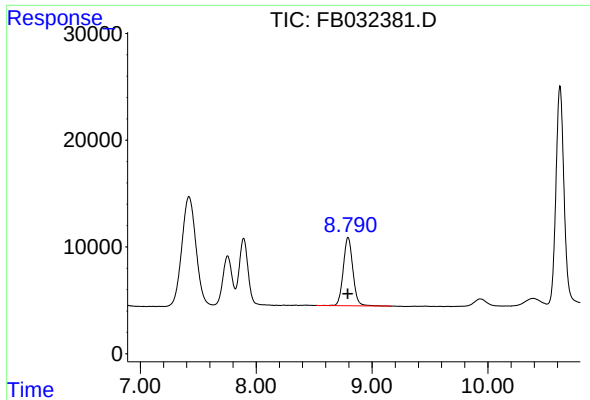

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.002 min
Response: 368170
Conc: 18.15 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S1

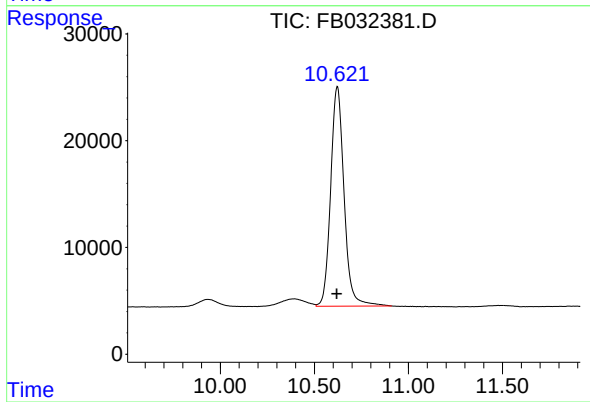


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.003 min
Response: 1020187
Conc: 28.51 ng/ml

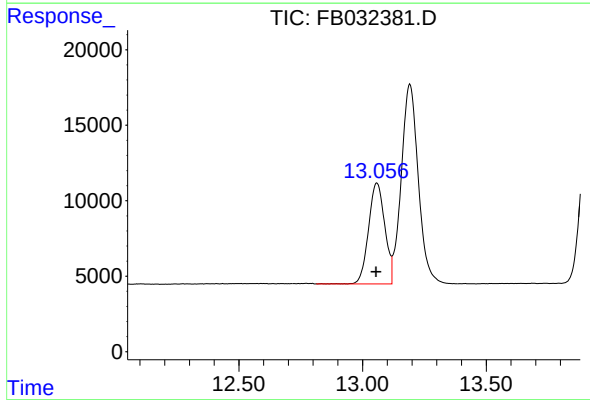


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.003 min
Response: 304354
Conc: 9.57 ng/ml

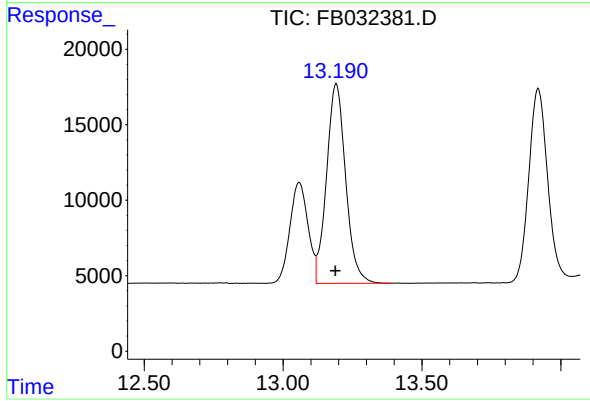

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.003 min
Response: 632793
Conc: 19.00 ng/ml

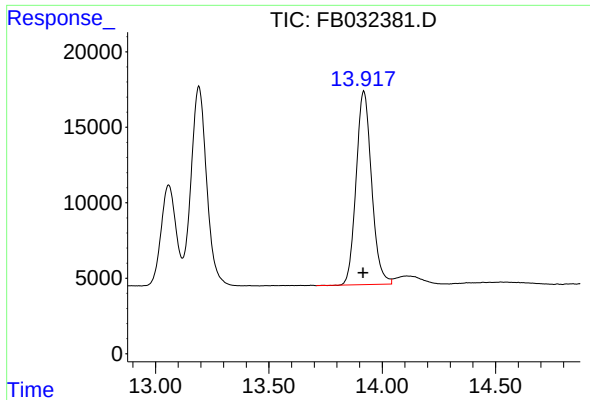

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.003 min
Response: 606812
Conc: 18.90 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1114S1

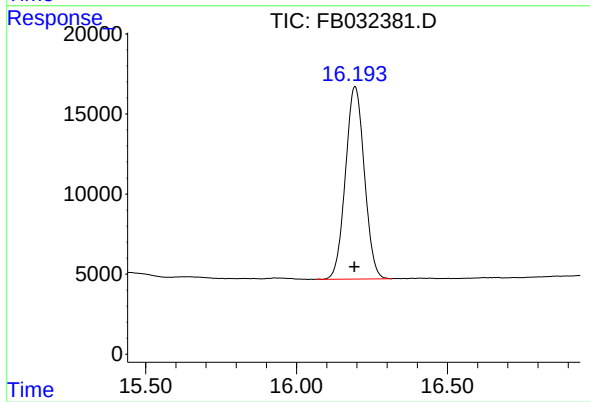

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.003 min
Response: 523032
Conc: 18.90 ng/ml