

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121019\
 Data File : FB023181.D
 Signal(s) : FID2B.CH
 Acq On : 10 Dec 2019 13:47
 Operator : DD/AJ
 Sample : K6204-13MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 11 00:19:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	462184	18.816 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	778086	23.811 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	894104	25.641 ng/ml
3) t n-Heptane	7.757	290957	8.462 ng/ml
4) t Benzene	7.892	377960	9.071 ng/ml
6) t Toluene	10.632	1099948	27.305 ng/ml
7) t Ethylbenzene	13.072	336166	8.712 ng/ml
8) t m-Xylene	13.204	641281	17.623 ng/ml
9) t O-Xylene	13.933	626724	18.050 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	528894	18.860 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121019\
Data File : FB023181.D
Signal(s) : FID2B.CH
Acq On : 10 Dec 2019 13:47
Operator : DD/AJ
Sample : K6204-13MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 11 00:19:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

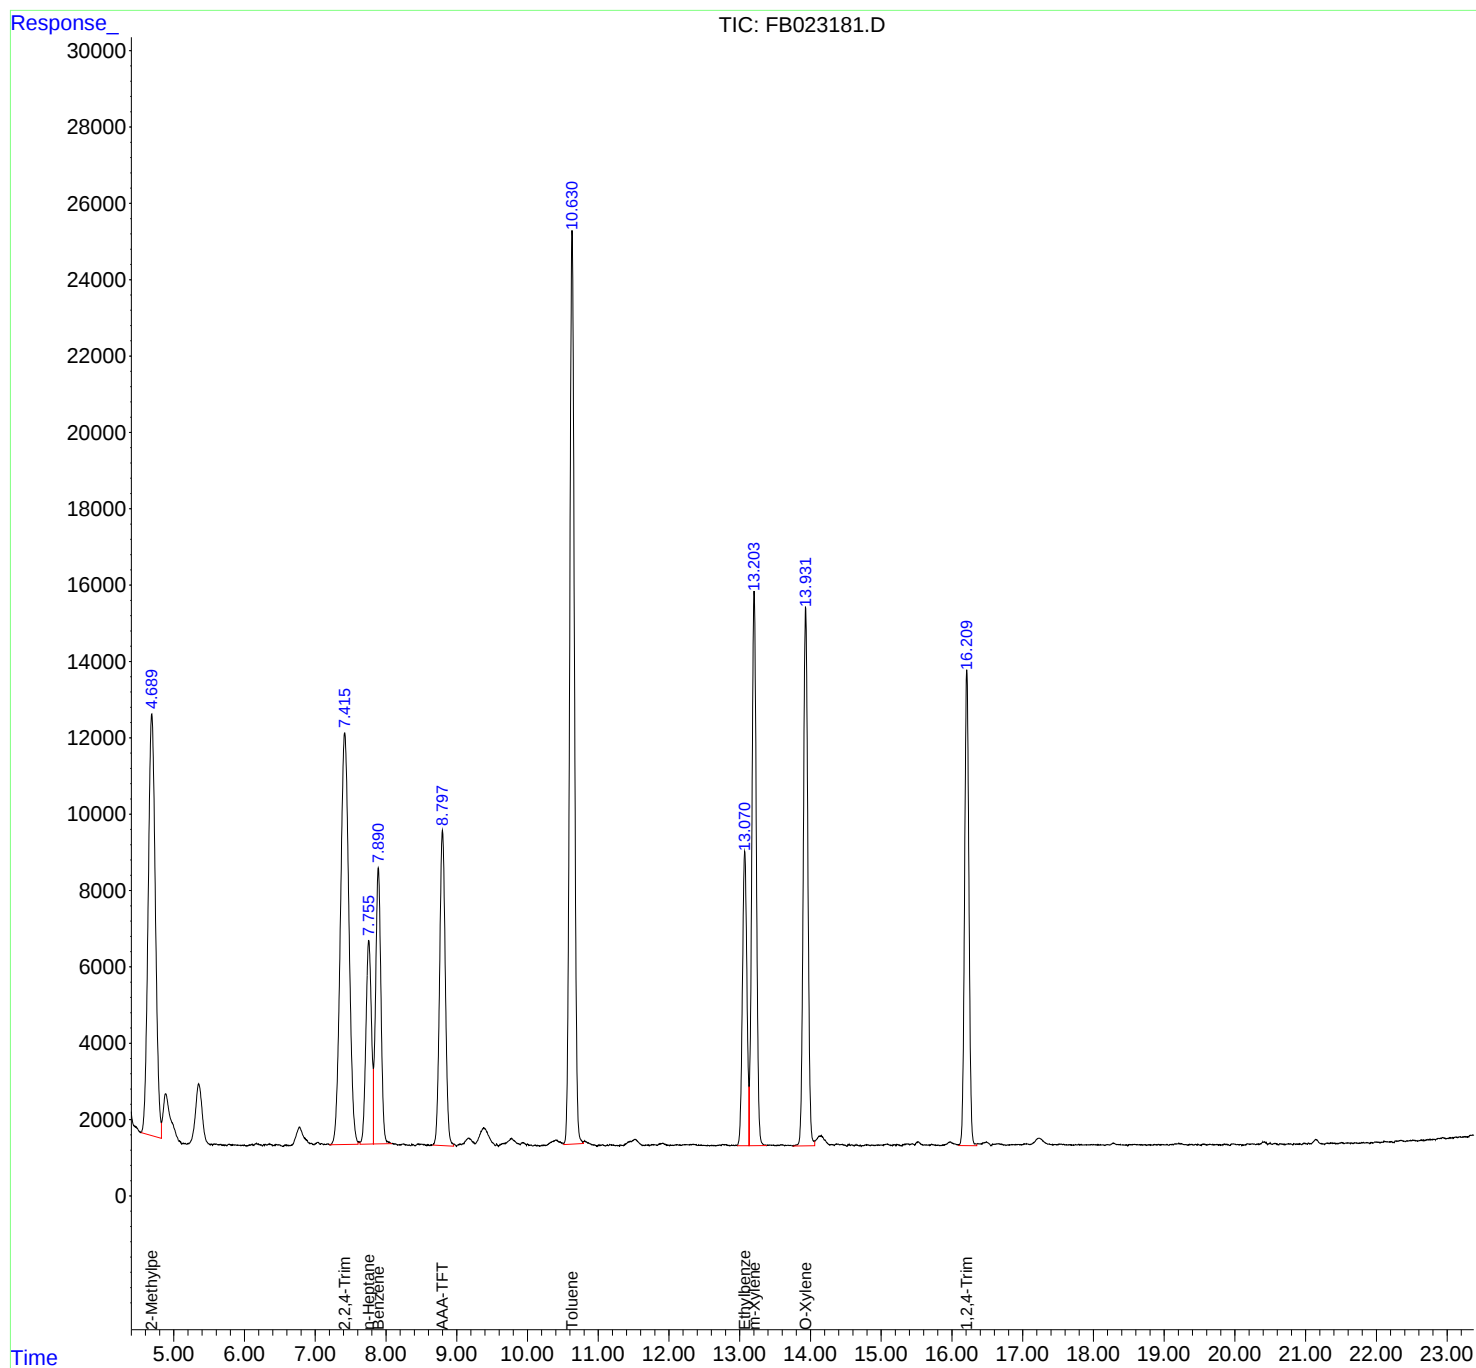

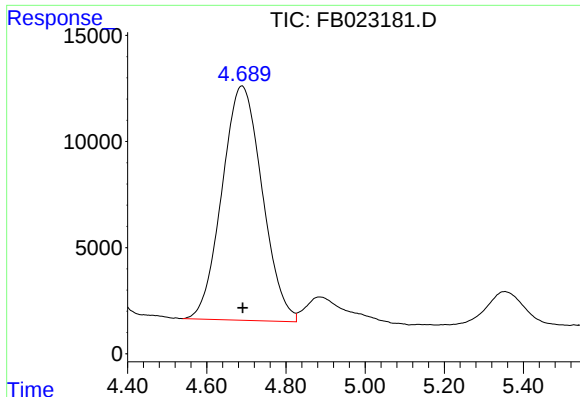


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: -0.001 min
Response: 778086
Conc: 23.81 ng/ml

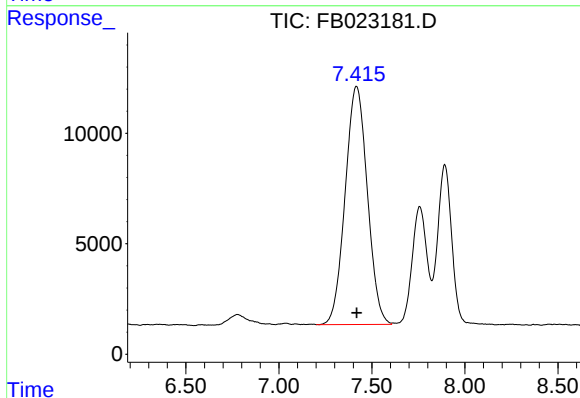


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.001 min
Response: 894104
Conc: 25.64 ng/ml

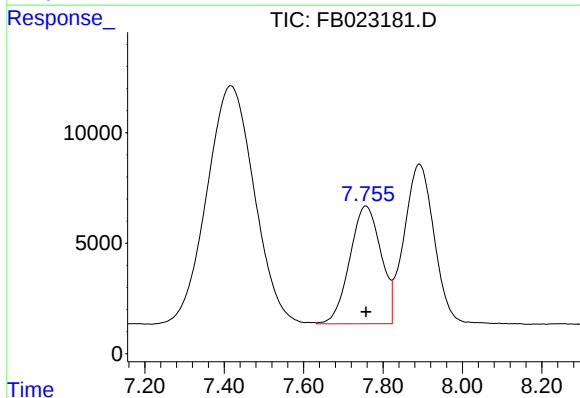


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 290957
Conc: 8.46 ng/ml

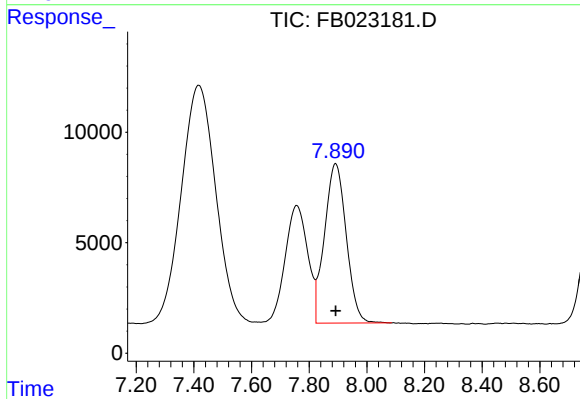


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 377960
Conc: 9.07 ng/ml

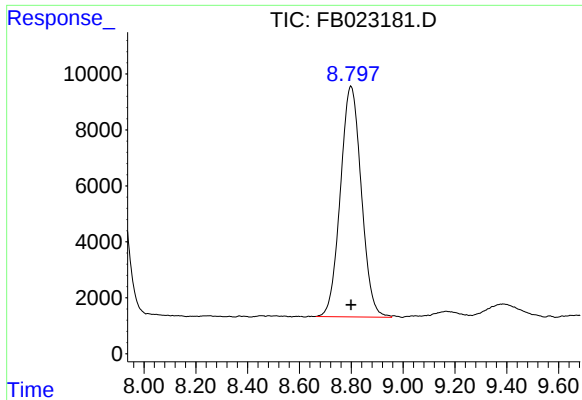


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 462184
Conc: 18.82 ng/ml

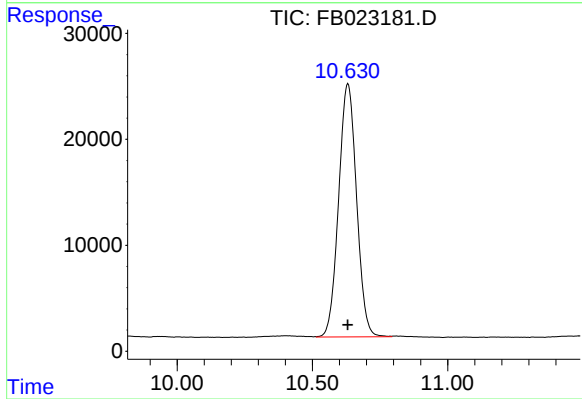


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.001 min
Response: 1099948
Conc: 27.30 ng/ml

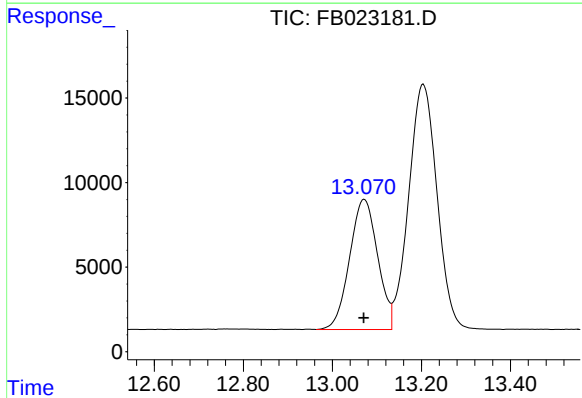


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.001 min
Response: 336166
Conc: 8.71 ng/ml

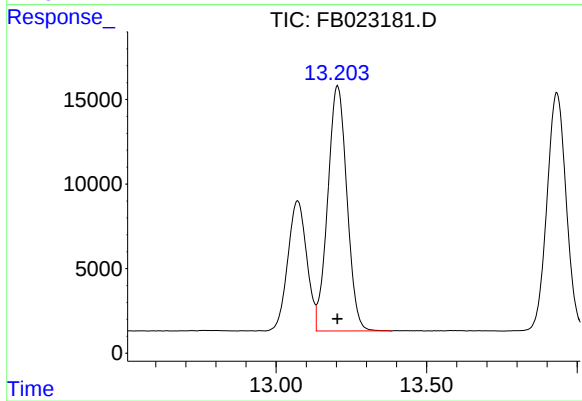


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 641281
Conc: 17.62 ng/ml

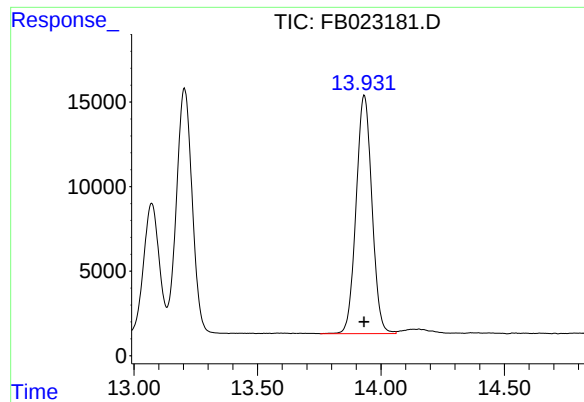

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.001 min
Response: 626724
Conc: 18.05 ng/ml

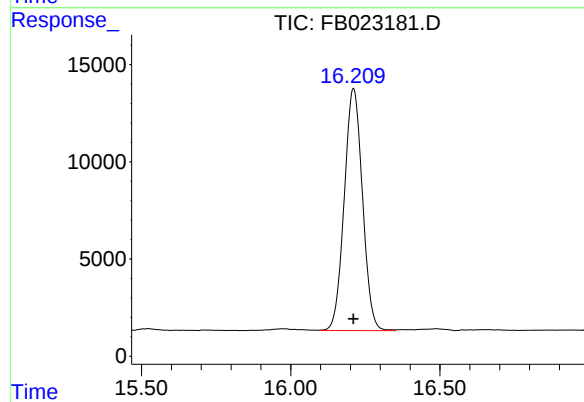

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 528894
Conc: 18.86 ng/ml