

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121019\
 Data File : FB023178.D
 Signal(s) : FID2B.CH
 Acq On : 10 Dec 2019 10:47
 Operator : DD/AJ
 Sample : BSF1210S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 11 00:19:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.799	496887	20.228 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.688	867257	26.539 ng/ml
2) t	2,2,4-Trimethylpentane	7.417	998252	28.627 ng/ml
3) t	n-Heptane	7.757	322204	9.371 ng/ml
4) t	Benzene	7.892	390185	9.365 ng/ml
6) t	Toluene	10.630	1157156	28.725 ng/ml
7) t	Ethylbenzene	13.070	361707	9.374 ng/ml
8) t	m-Xylene	13.203	684570	18.812 ng/ml
9) t	O-Xylene	13.931	660998	19.038 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	550946	19.646 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121019\
Data File : FB023178.D
Signal(s) : FID2B.CH
Acq On : 10 Dec 2019 10:47
Operator : DD/AJ
Sample : BSF1210S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 11 00:19:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

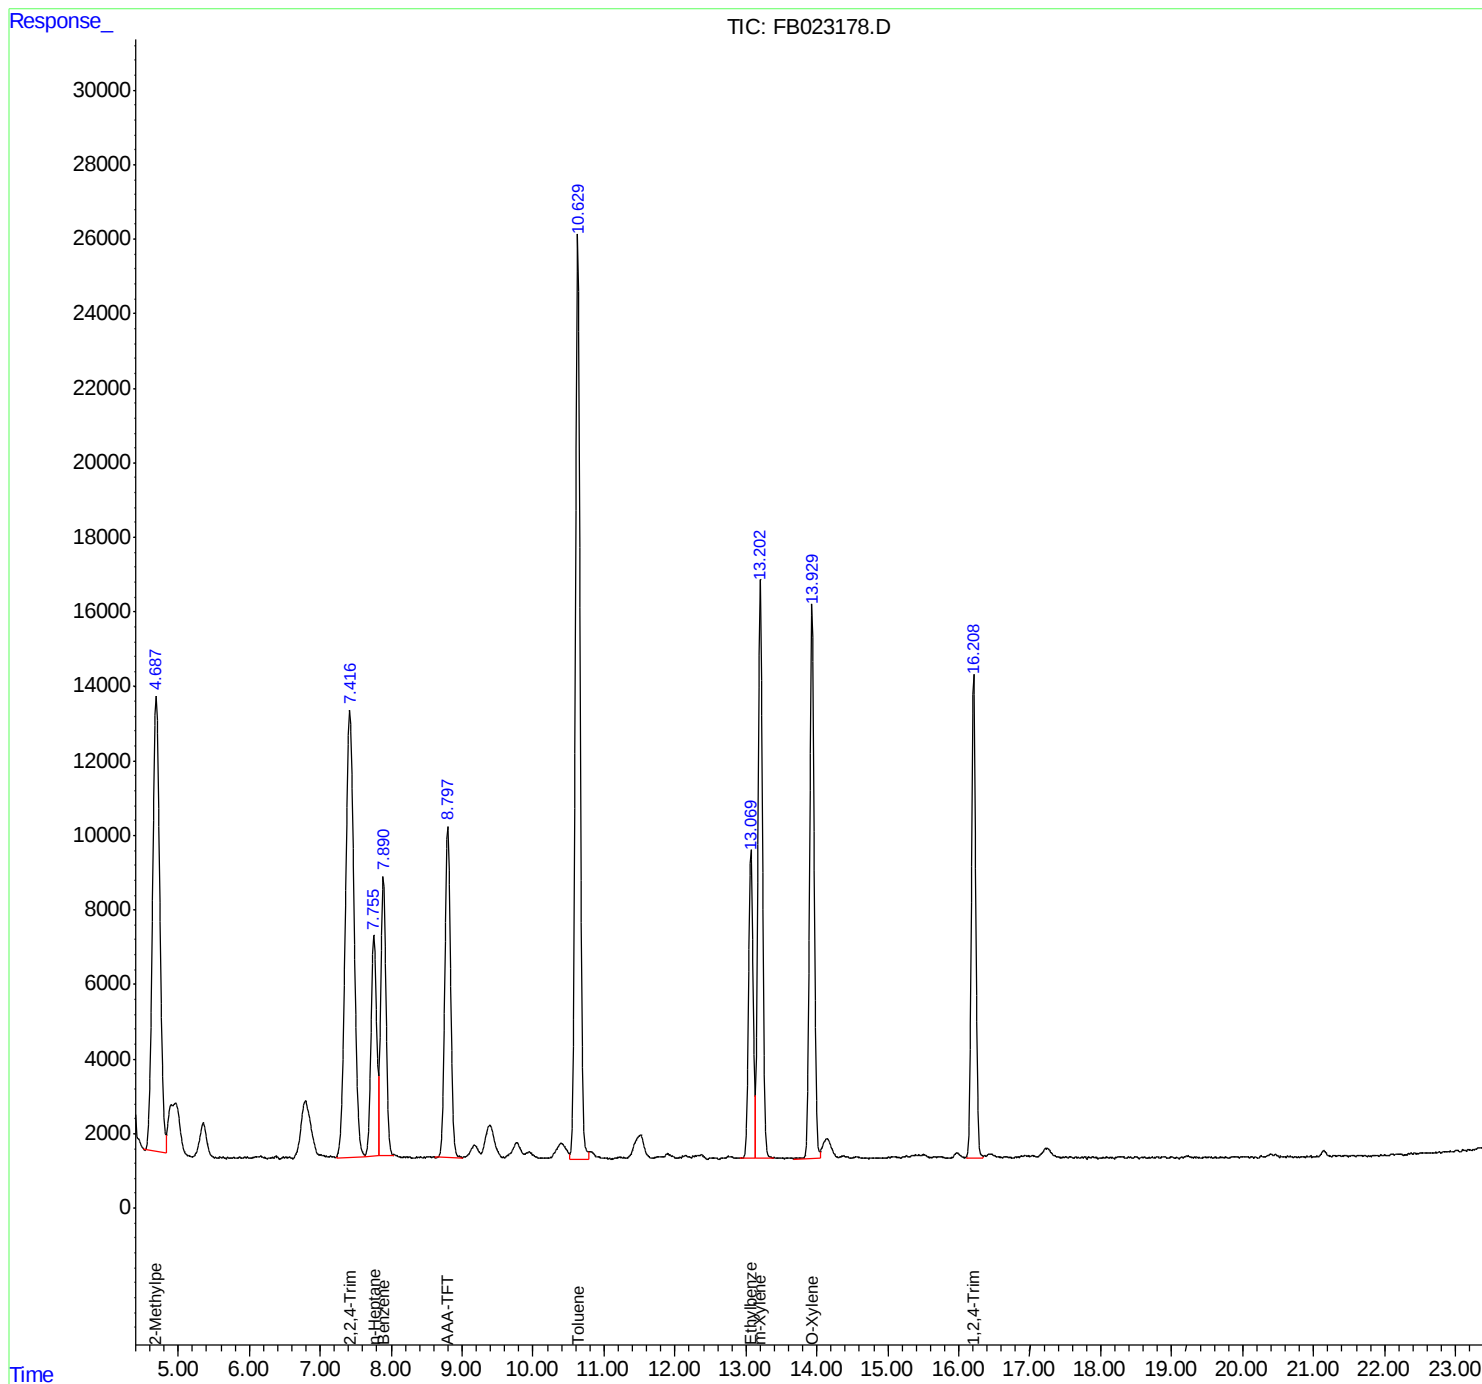

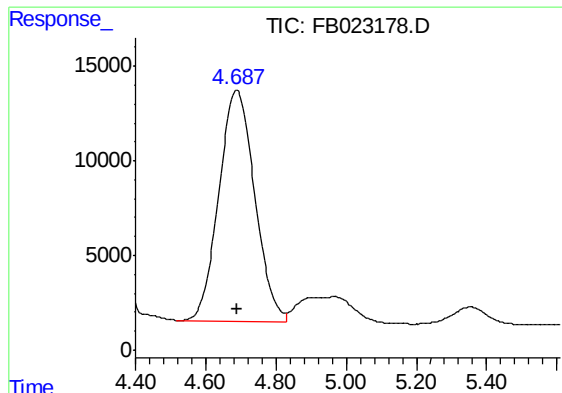


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.003 min
Response: 867257
Conc: 26.54 ng/ml

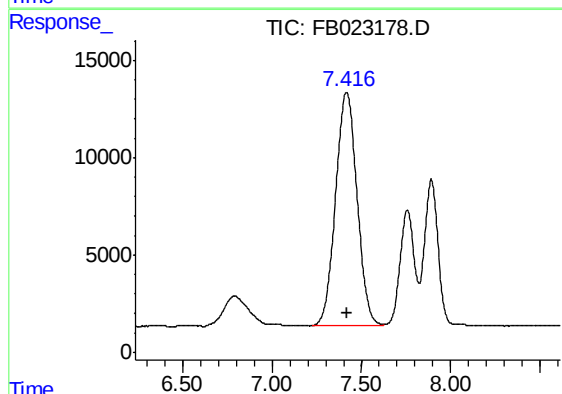


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 998252
Conc: 28.63 ng/ml

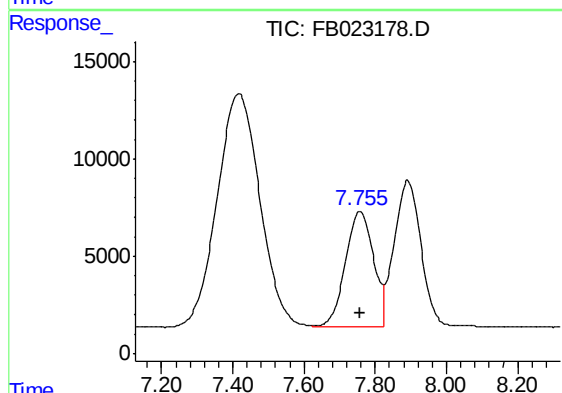


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 322204
Conc: 9.37 ng/ml

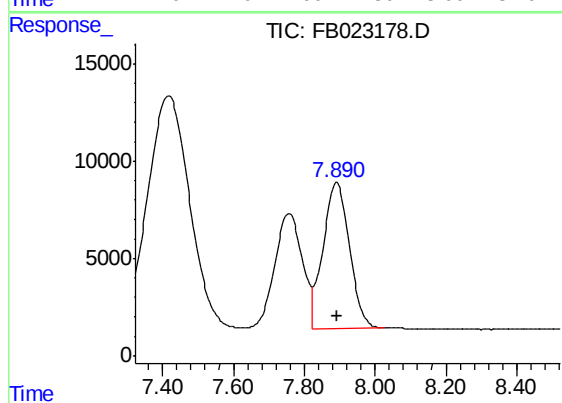


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 390185
Conc: 9.36 ng/ml

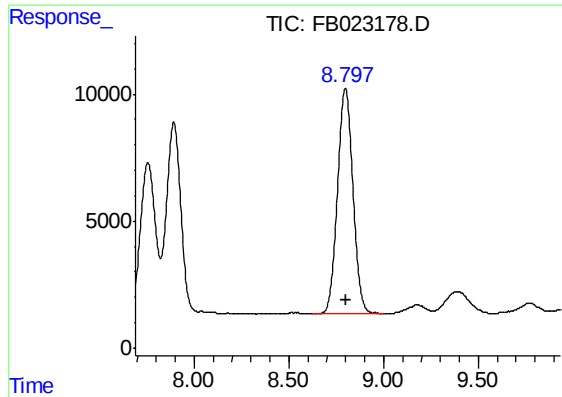


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 496887
Conc: 20.23 ng/ml

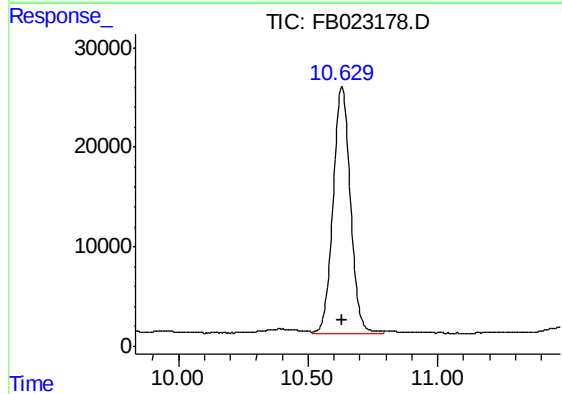


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1157156
Conc: 28.73 ng/ml

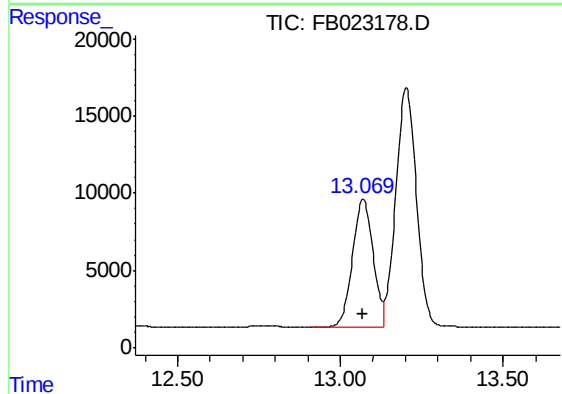


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 361707
Conc: 9.37 ng/ml

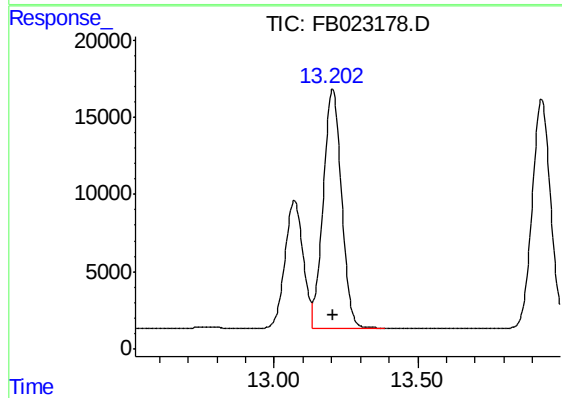


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 684570
Conc: 18.81 ng/ml

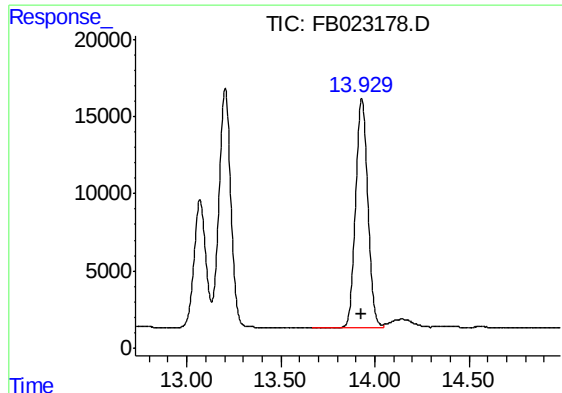

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 660998
Conc: 19.04 ng/ml

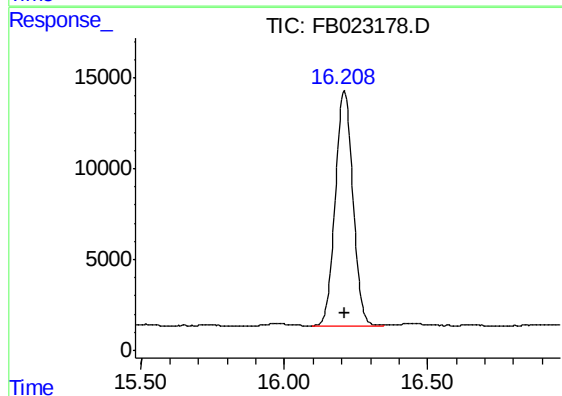

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 550946
Conc: 19.65 ng/ml